


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
Data File : BM025355.D
Acq On : 07 Mar 2020 18:15
Operator : CG/JU
Sample : L1616-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Mar 07 20:56:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Sat Mar 07 20:27:15 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBDQ0

Manual Integrations
APPROVED

mohammad
3/9/2020 3:02:00 PM

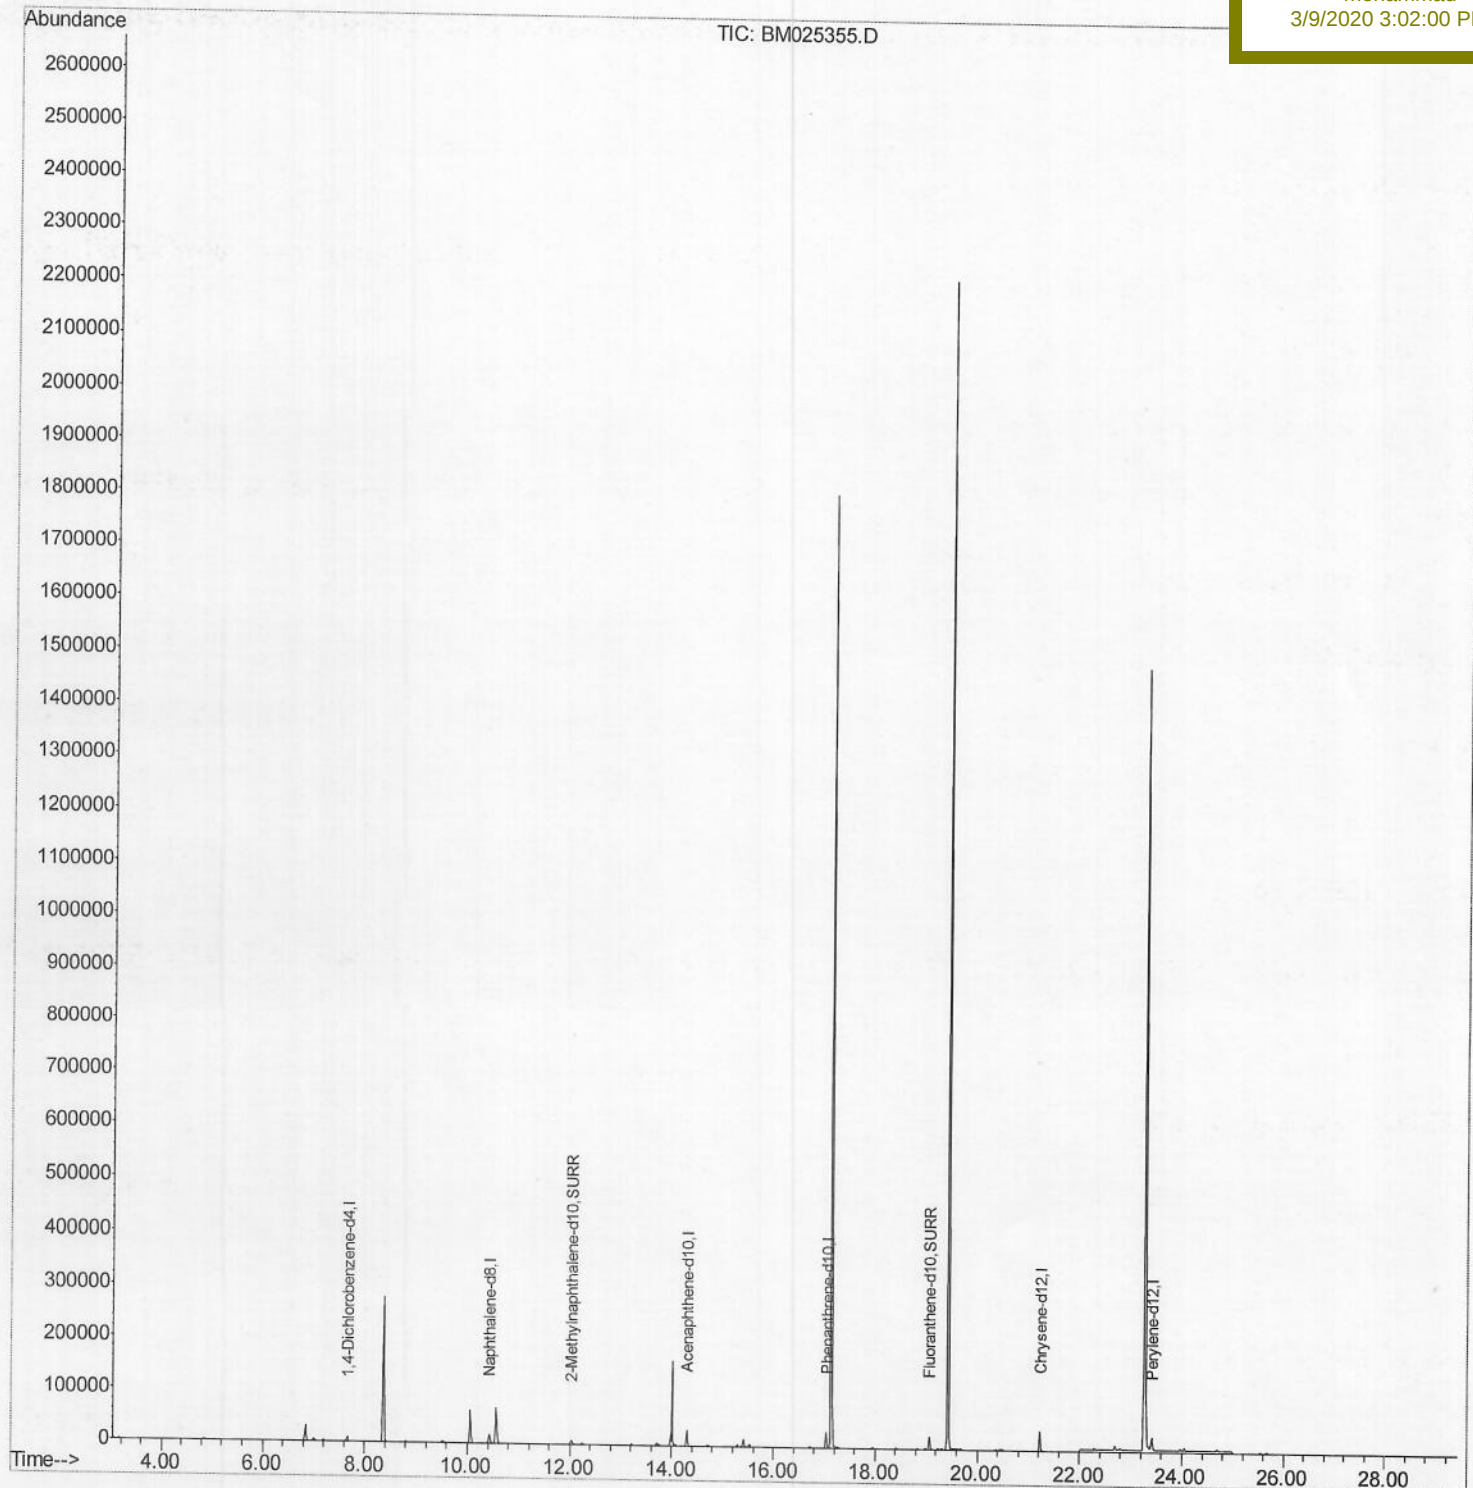

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\

Data File : BM025355.D

Acq On : 07 Mar 2020 18:15

Operator : CG/JU

Sample : L1616-06

Misc :

ALS Vial : 41 Sample Multiplier: 1

Quant Time: Mar 07 20:55:51 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sat Mar 07 20:27:15 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBDQ0

Manual Integrations

APPROVED

mohammad

3/9/2020 3:02:00 PM

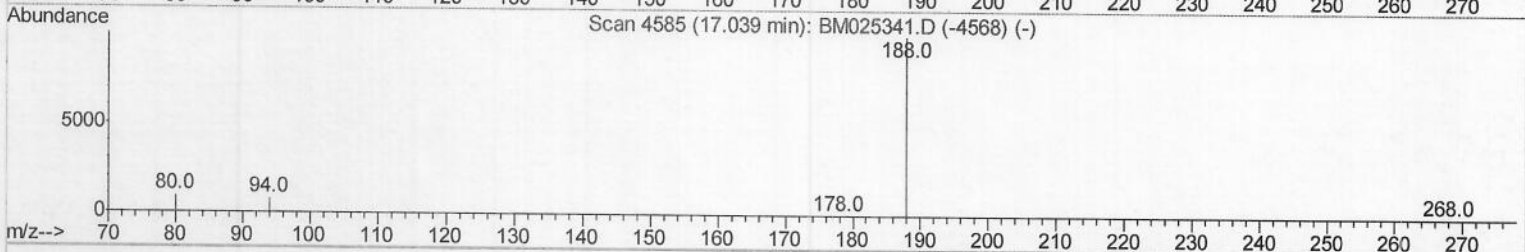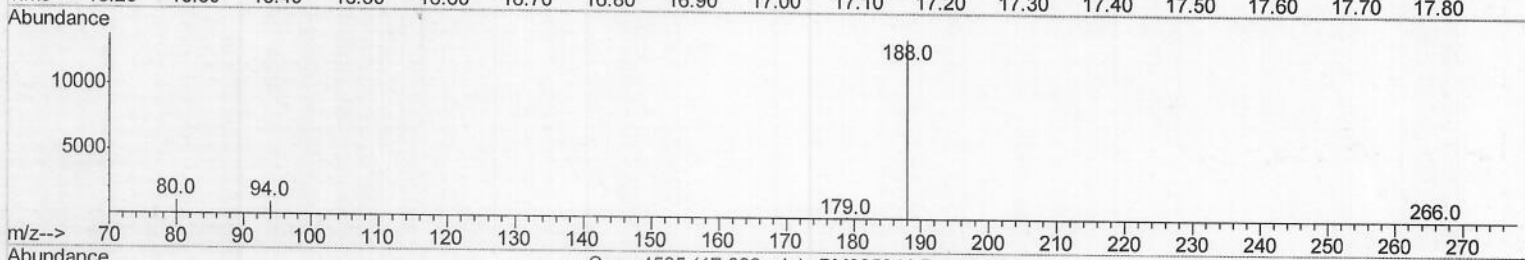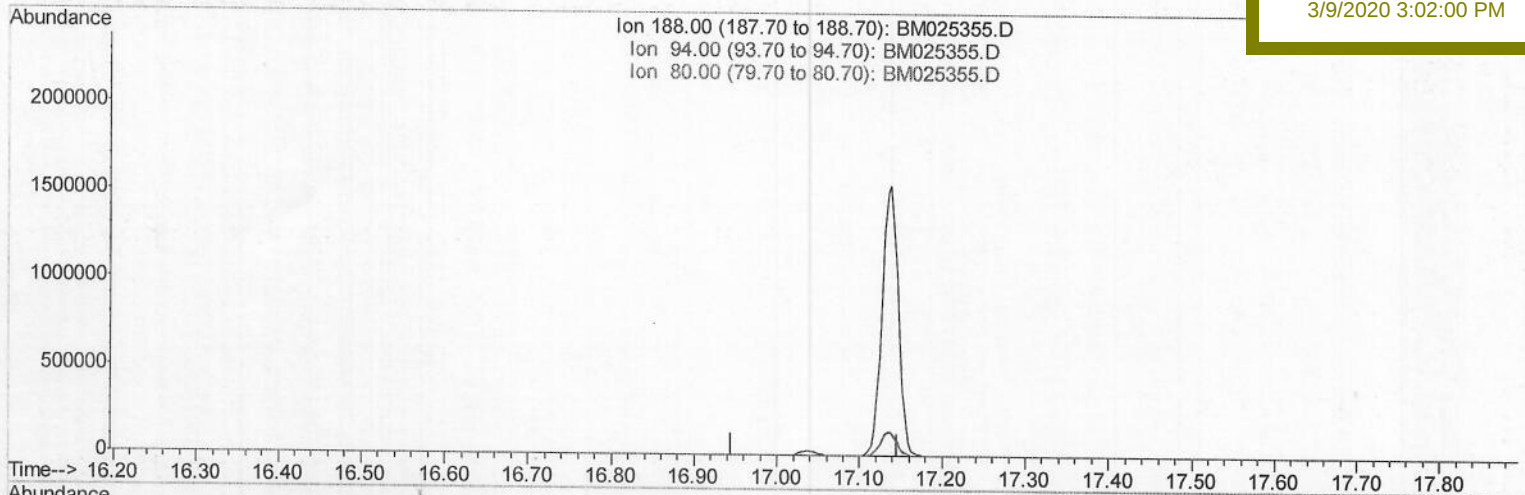

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\

Data File : BM025355.D

Acq On : 07 Mar 2020 18:15

Operator : CG/JU

Sample : L1616-06

Misc :

ALS Vial : 41 Sample Multiplier: 1

Quant Time: Mar 07 20:55:51 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sat Mar 07 20:27:15 2020

Response via : Initial Calibration

Instrument :

BNA_M




ClientSampleId :

DBDQ0

Manual Integrations
APPROVED

mohammad

3/9/2020 3:02:00 PM

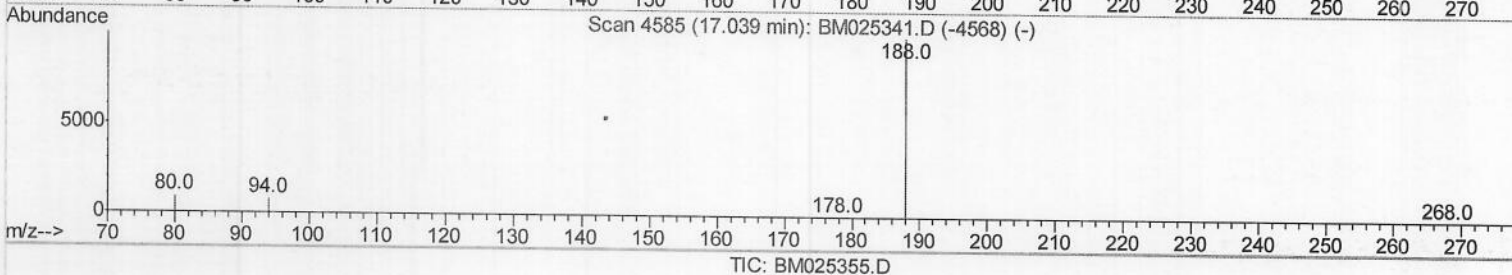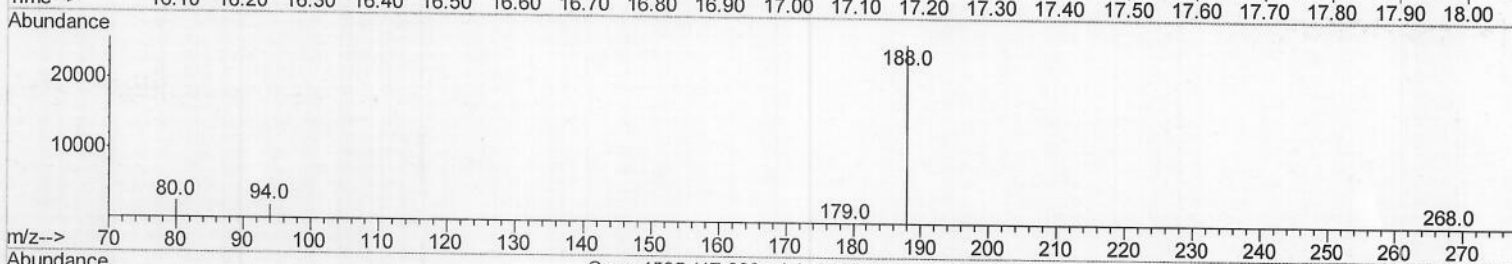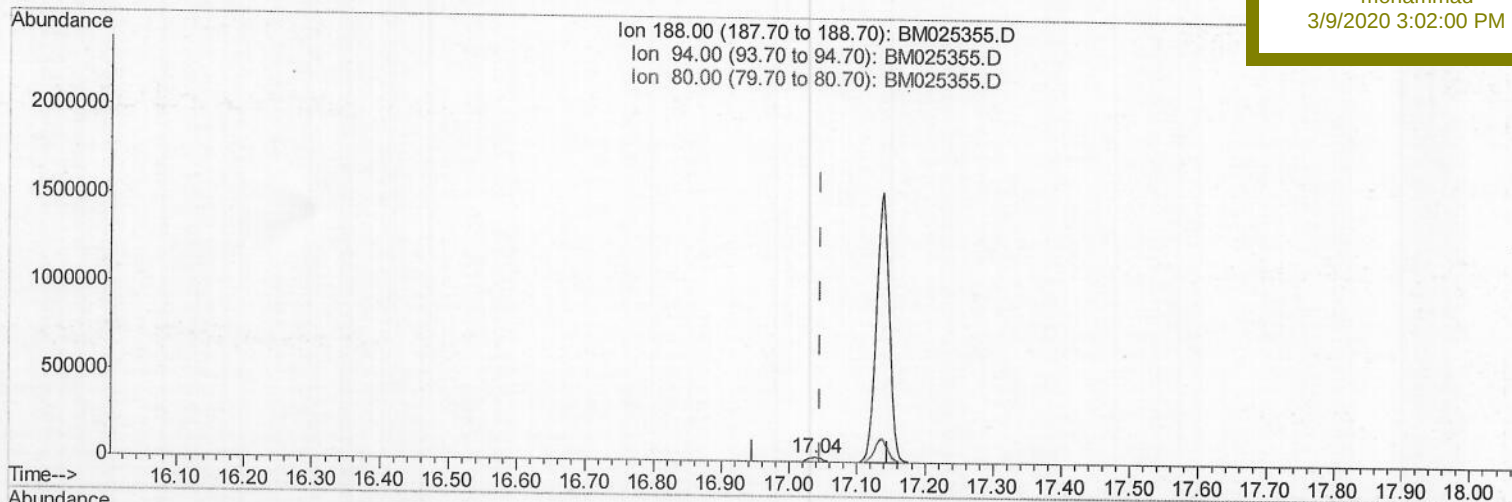

TIC: BM025355.D

(10) Phenanthrene-d10 (I)

17.038min (-0.009) 0.40ng/ul m > 0v 03/11/20

response 34753

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	8.07#
80.00	22.60	9.46#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
Data File : BM025355.D
Acq On : 07 Mar 2020 18:15
Operator : CG/JU
Sample : L1616-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Mar 07 20:56:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 07 20:27:15 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBDQ0

Manual Integrations
APPROVED

mohammad
3/9/2020 3:02:00 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	4651	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	20894	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	15159	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	34753m	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	31679	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	27598	0.40	ng/ul	-0.01

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.03	152	9763	0.25	ng/ul	-0.01
14) Fluoranthene-d10	19.07	212	26826	0.24	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SV 03/11/20