


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
Data File : BM025356.D
Acq On : 07 Mar 2020 18:51
Operator : CG/JU
Sample : L1616-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Quant Time: Mar 07 20:58:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 07 20:27:15 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBDQ2

Manual Integrations
APPROVED

mohammad
3/9/2020 3:02:02 PM

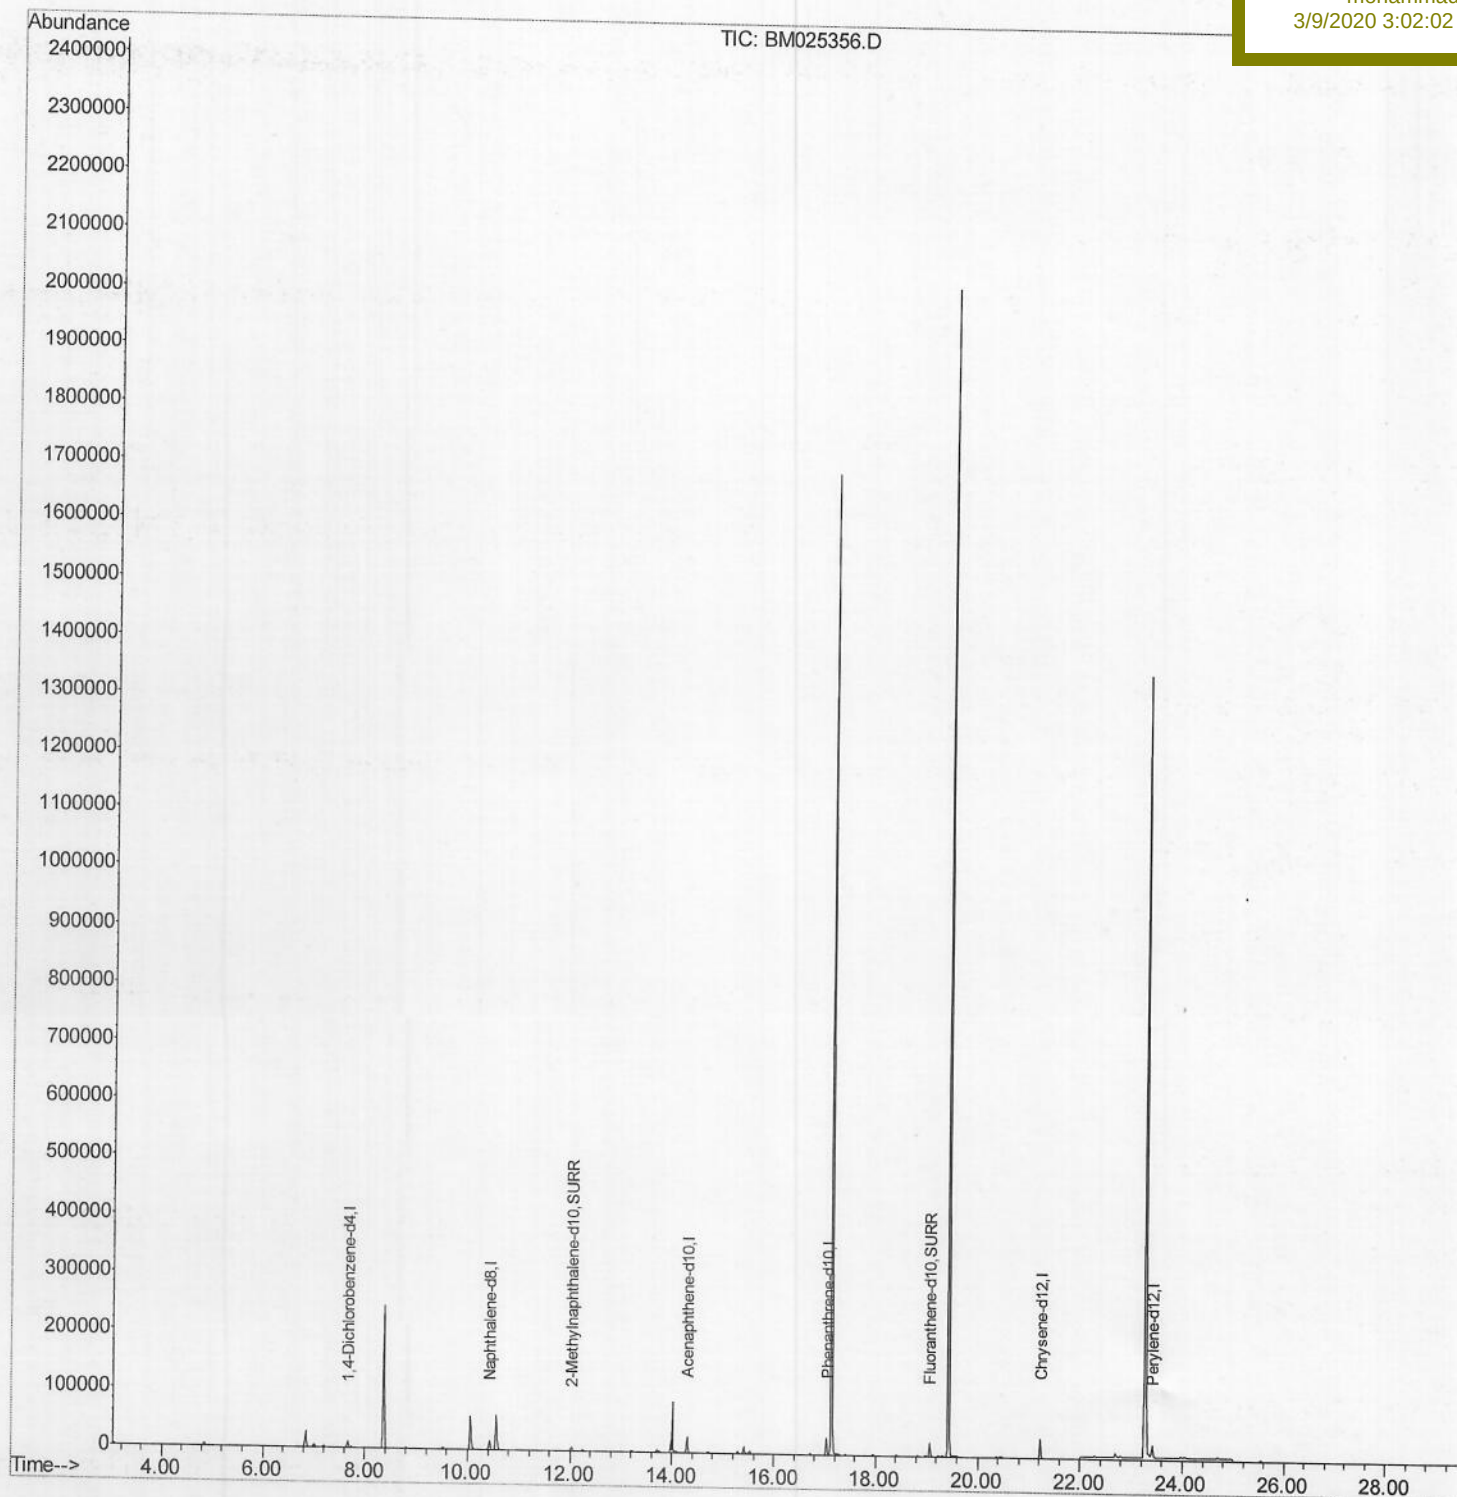

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
Data File : BM025356.D
Acq On : 07 Mar 2020 18:51
Operator : CG/JU
Sample : L1616-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Quant Time: Mar 07 20:57:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 07 20:27:15 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBDQ2

Manual Integrations
APPROVED

mohammad
3/9/2020 3:02:02 PM

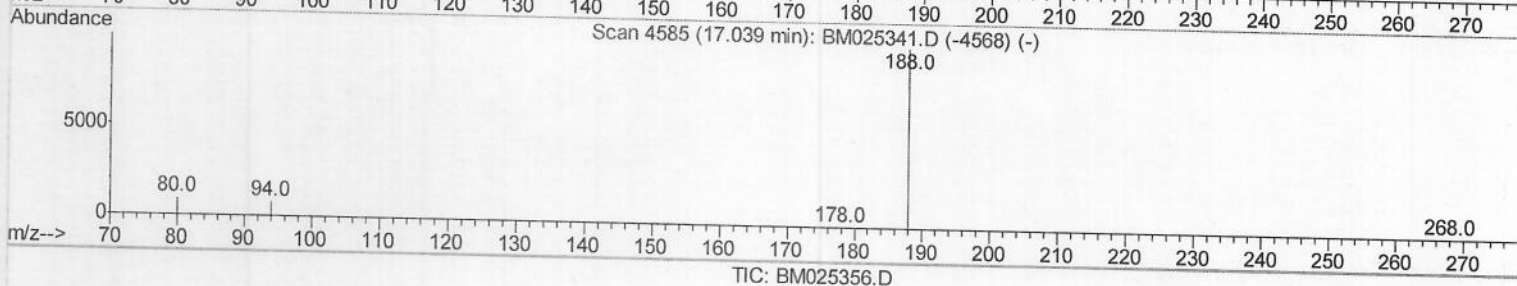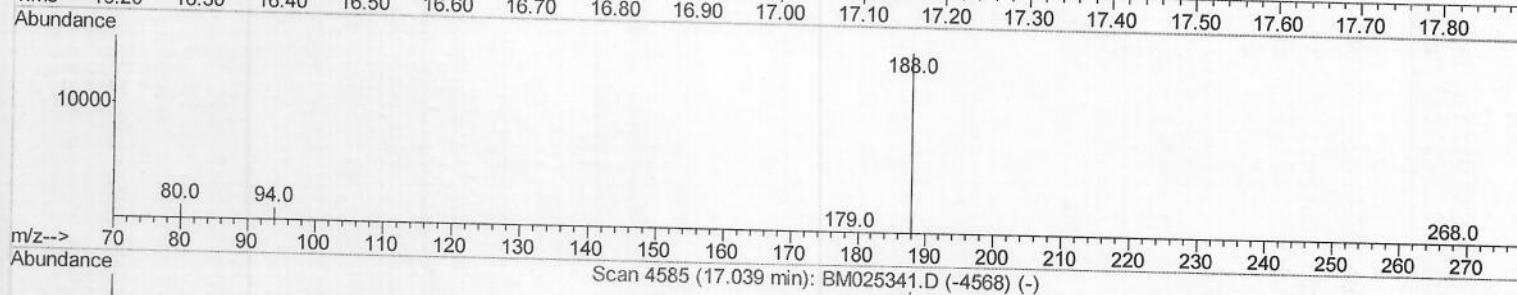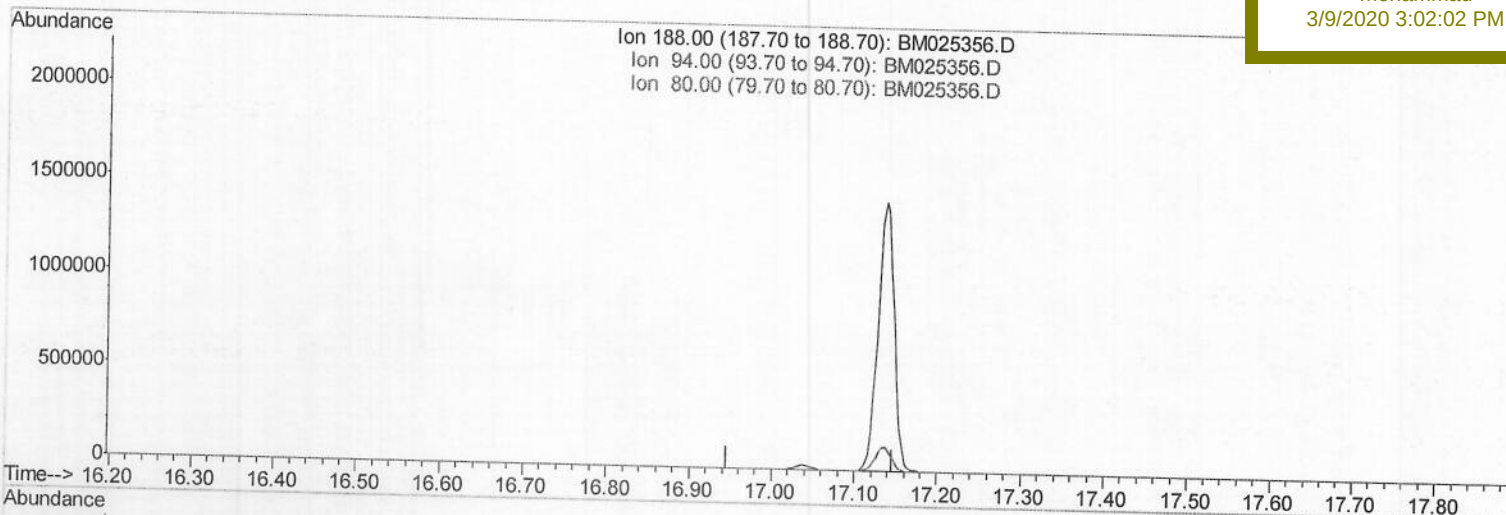

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
 Data File : BM025356.D
 Acq On : 07 Mar 2020 18:51
 Operator : CG/JU
 Sample : L1616-08
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Quant Time: Mar 07 20:57:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 07 20:27:15 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DBDQ2

Manual Integrations
 APPROVED

mohammad
 3/9/2020 3:02:02 PM

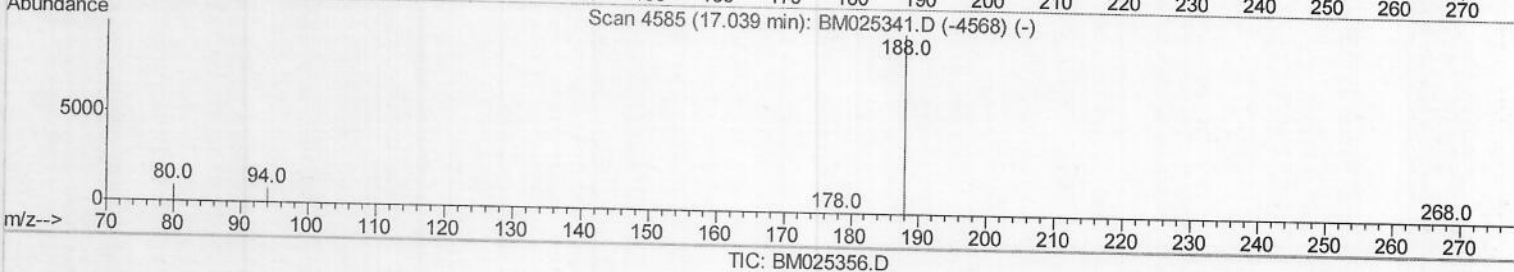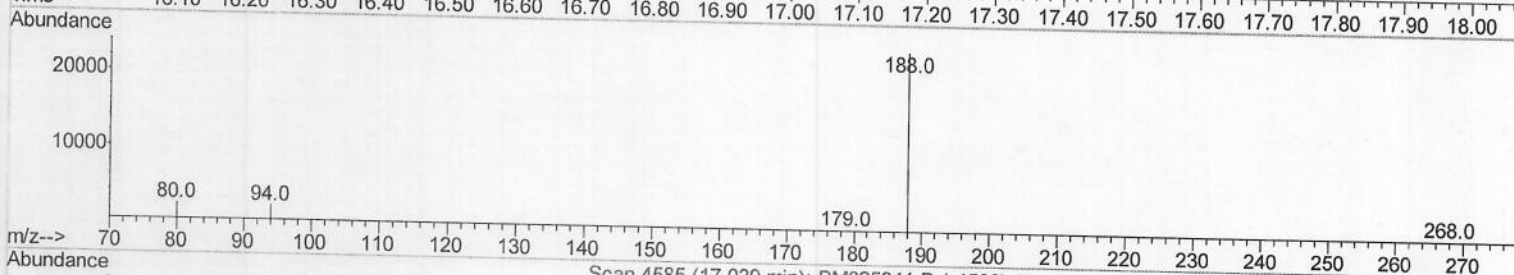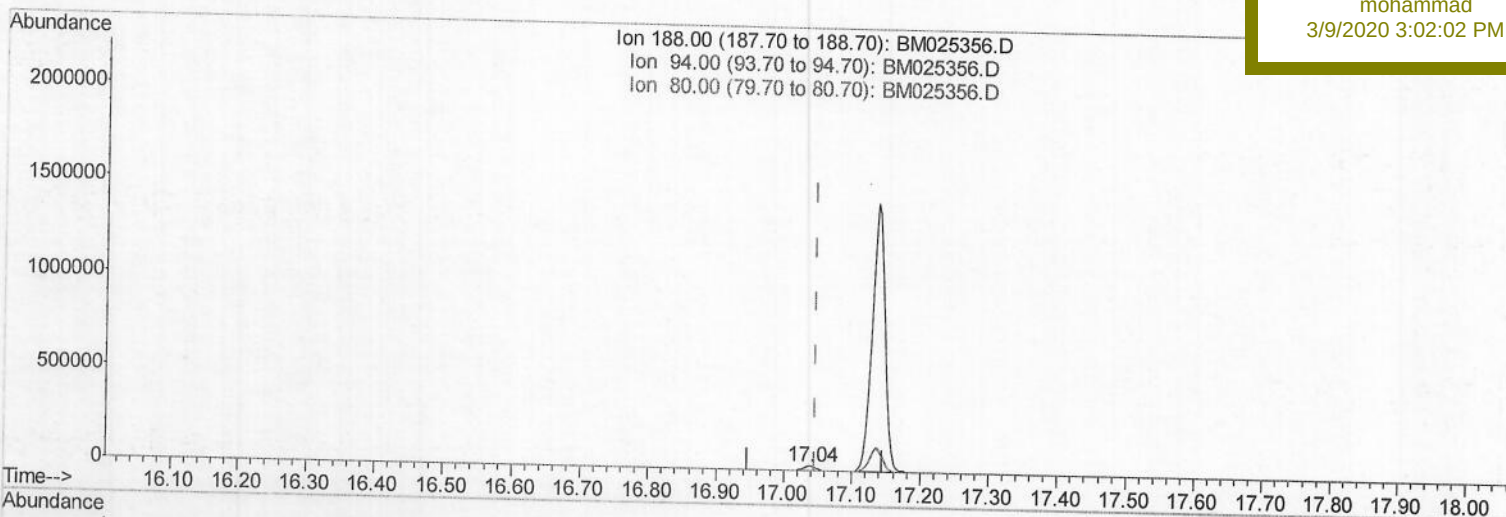

(10) Phenanthrene-d10 (I)

17.039min (-0.007) 0.40ng/ul m *ju* 03/11/20

response 32847

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	8.17#
80.00	22.60	9.05#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
Data File : BM025356.D
Acq On : 07 Mar 2020 18:51
Operator : CG/JU
Sample : L1616-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Quant Time: Mar 07 20:58:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 07 20:27:15 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBDQ2

Manual Integrations
APPROVED

mohammad
3/9/2020 3:02:02 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	4449	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	19806	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	14281	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.04	188	32847m)	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	29401	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	25892	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	8720	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	24670	0.23	ng/ul	0.00

Target Compounds

					Ovalue
--	--	--	--	--	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed