

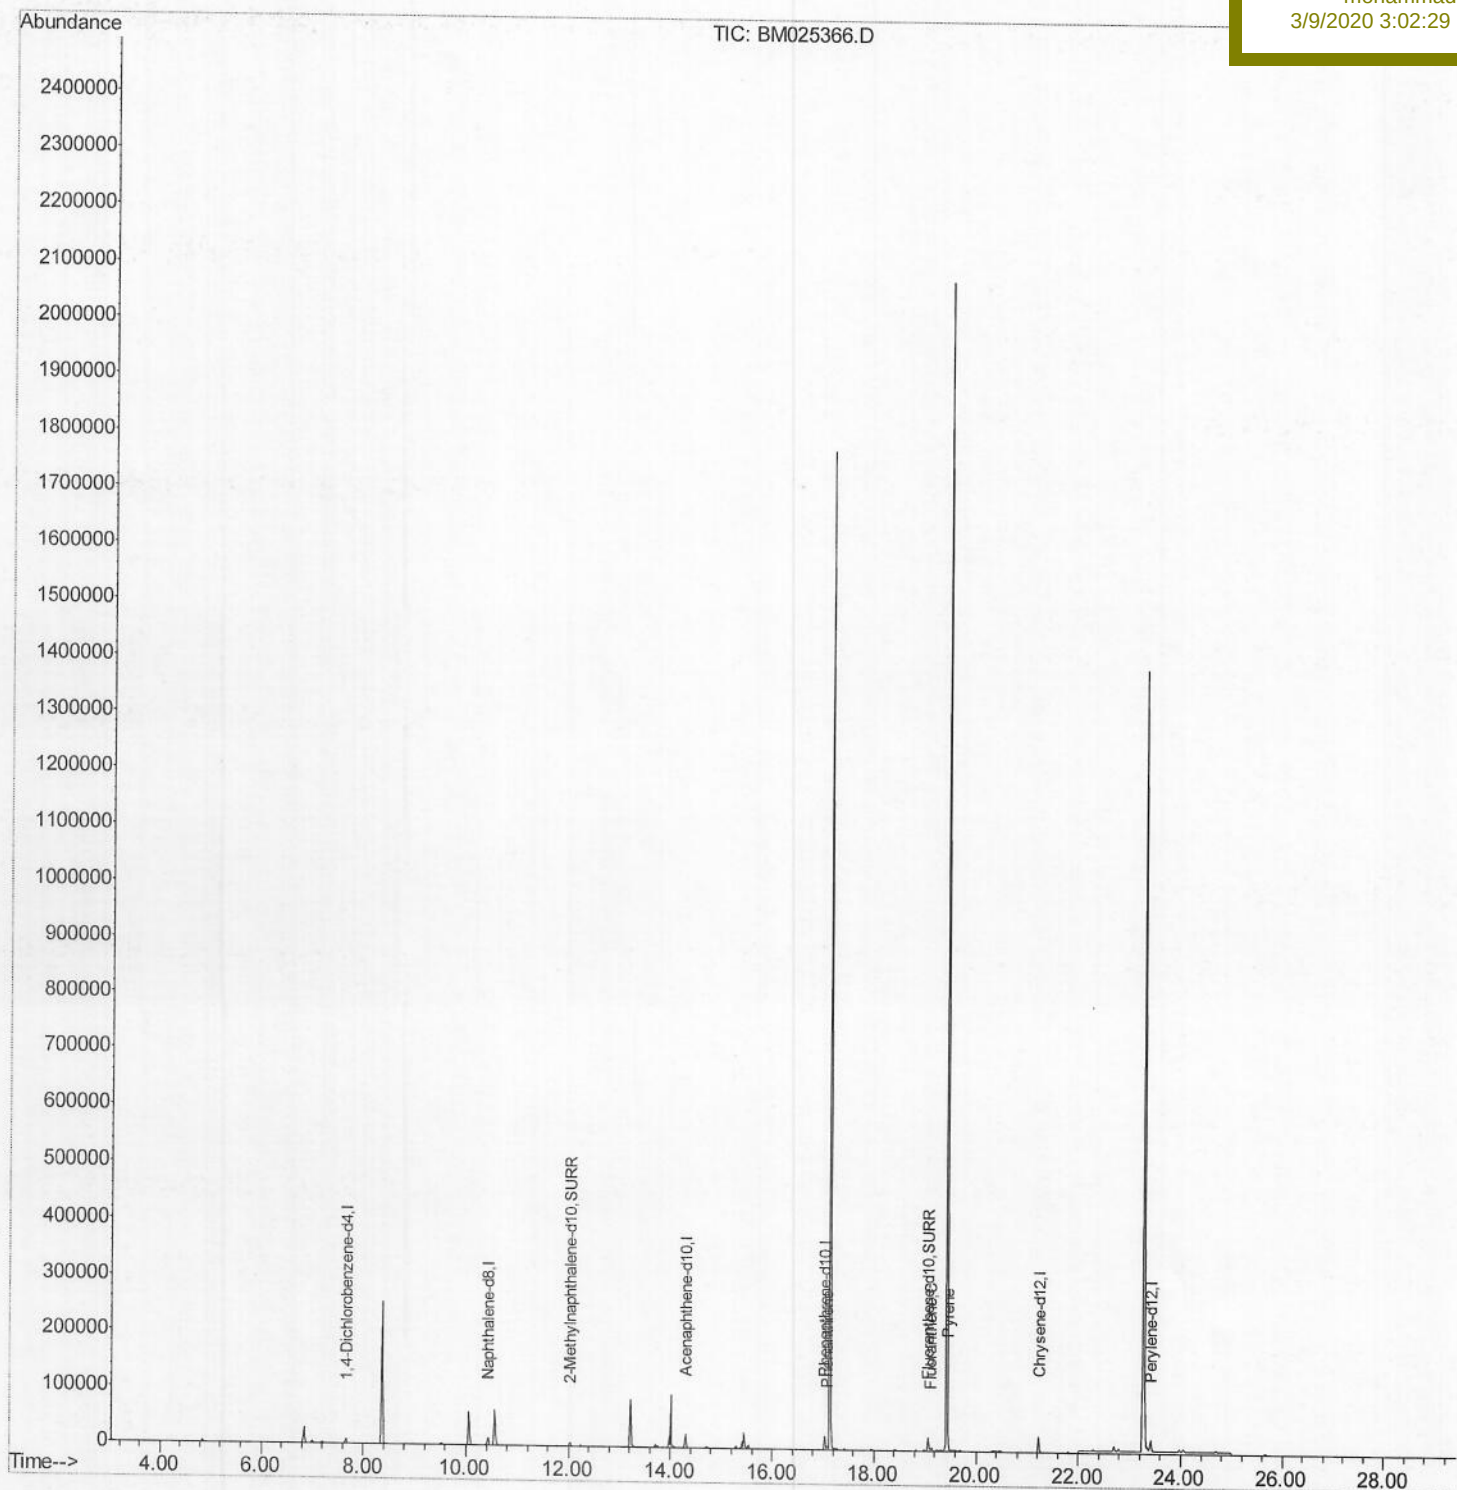
Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
Data File : BM025366.D
Acq On : 08 Mar 2020 01:26
Operator : CG/JU
Sample : L1615-22
Misc :
ALS Vial : 52 Sample Multiplier: 1

Quant Time: Mar 08 03:23:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 07 23:59:42 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBDP6

Manual Integrations
APPROVED

mohammad
3/9/2020 3:02:29 PM



Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\

Data File : BM025366.D

Acq On : 08 Mar 2020 01:26

Operator : CG/JU

Sample : L1615-22

Misc :

ALS Vial : 52 Sample Multiplier: 1

Quant Time: Mar 08 03:22:49 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sat Mar 07 23:59:42 2020




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

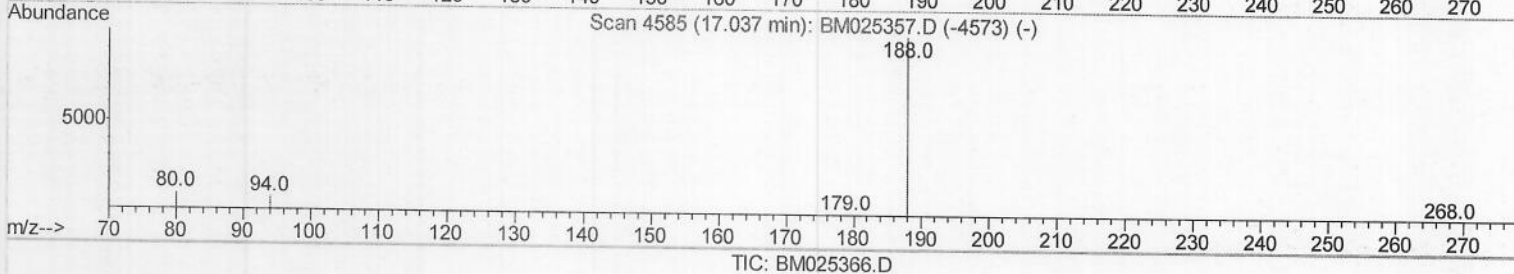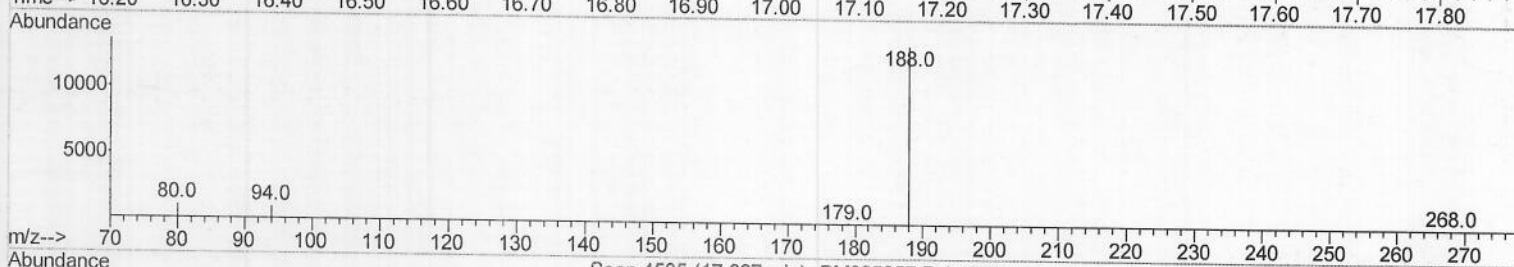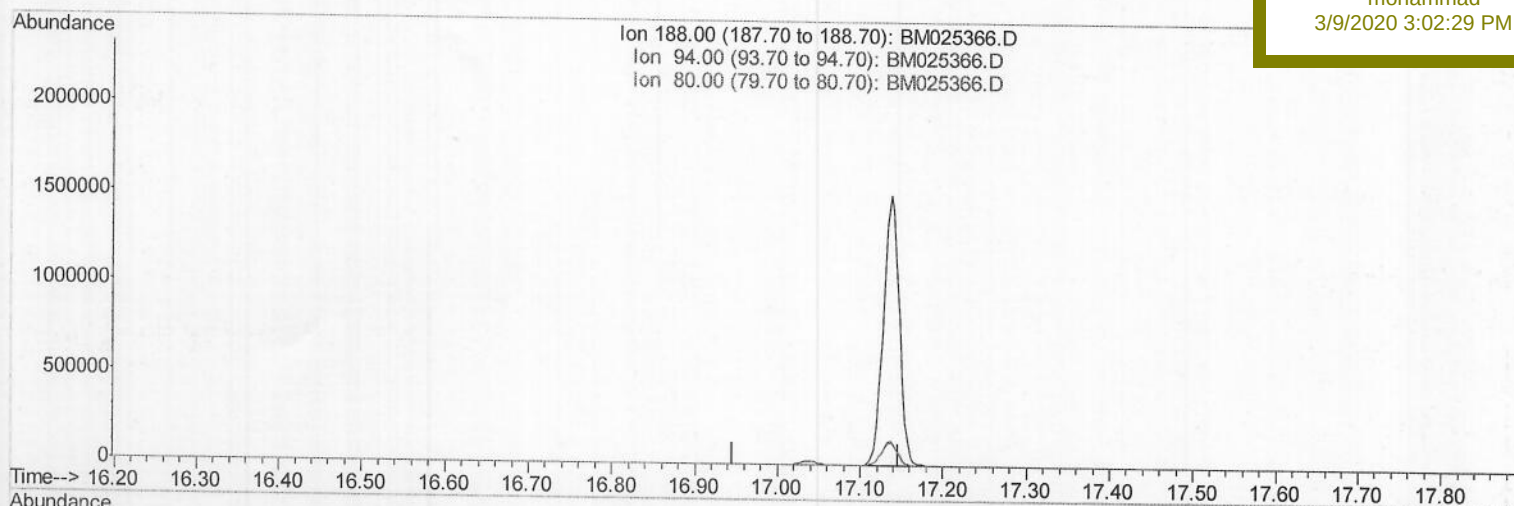DBDP6

Manual Integrations
APPROVEDmohammad
3/9/2020 3:02:29 PM

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

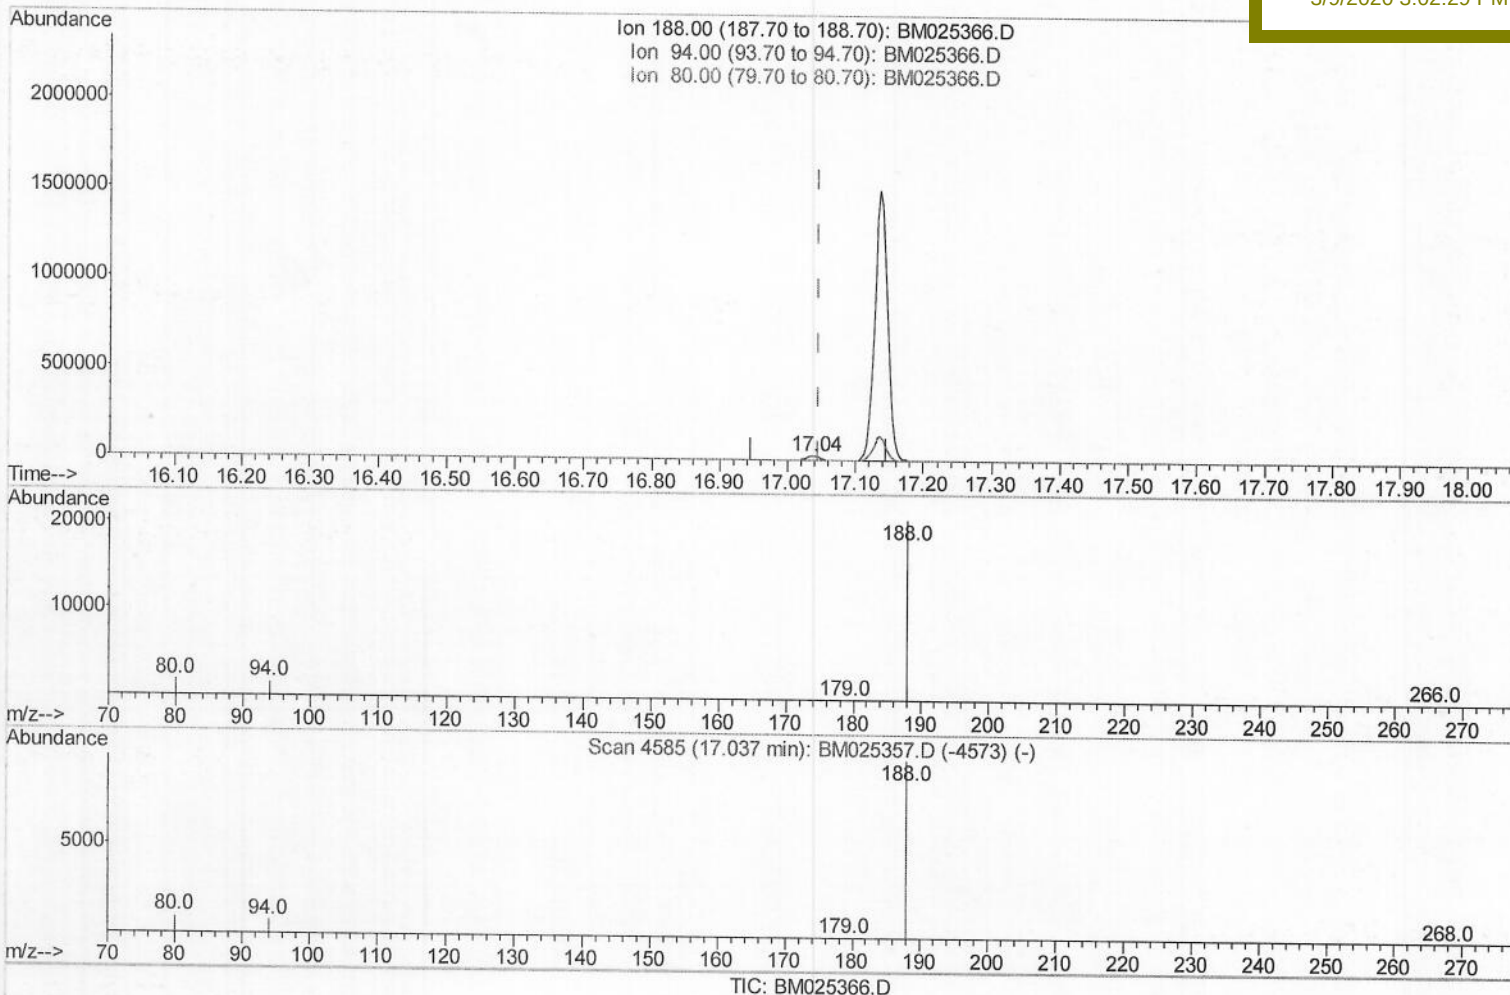
Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
 Data File : BM025366.D
 Acq On : 08 Mar 2020 01:26
 Operator : CG/JU
 Sample : L1615-22
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDP6

Quant Time: Mar 08 03:22:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 07 23:59:42 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 3/9/2020 3:02:29 PM



(10) Phenanthrene-d10 (I)

17.039min (-0.007) 0.40ng/ul m > 00 03/11/20

response 28596

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.88#
80.00	22.60	8.97#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
 Data File : BM025366.D
 Acq On : 08 Mar 2020 01:26
 Operator : CG/JU
 Sample : L1615-22
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDP6

Quant Time: Mar 08 03:23:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 07 23:59:42 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 3/9/2020 3:02:29 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	3869	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	17161	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	12476	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.04	188	28596m	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	25466	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	22613	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	9020	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	25958	0.28	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.08	178	5409	0.059	ng/ul	99
15) Fluoranthene	19.09	202	4125	0.036	ng/ul	94
17) Pyrene	19.46	202	2231	0.023	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed