


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
Data File : BM025380.D
Acq On : 08 Mar 2020 11:24
Operator : CG/JU
Sample : L1616-22
Misc :
ALS Vial : 66 Sample Multiplier: 1

Quant Time: Mar 09 01:55:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBDR6

Manual Integrations
APPROVED

mohammad
3/9/2020 3:03:17 PM

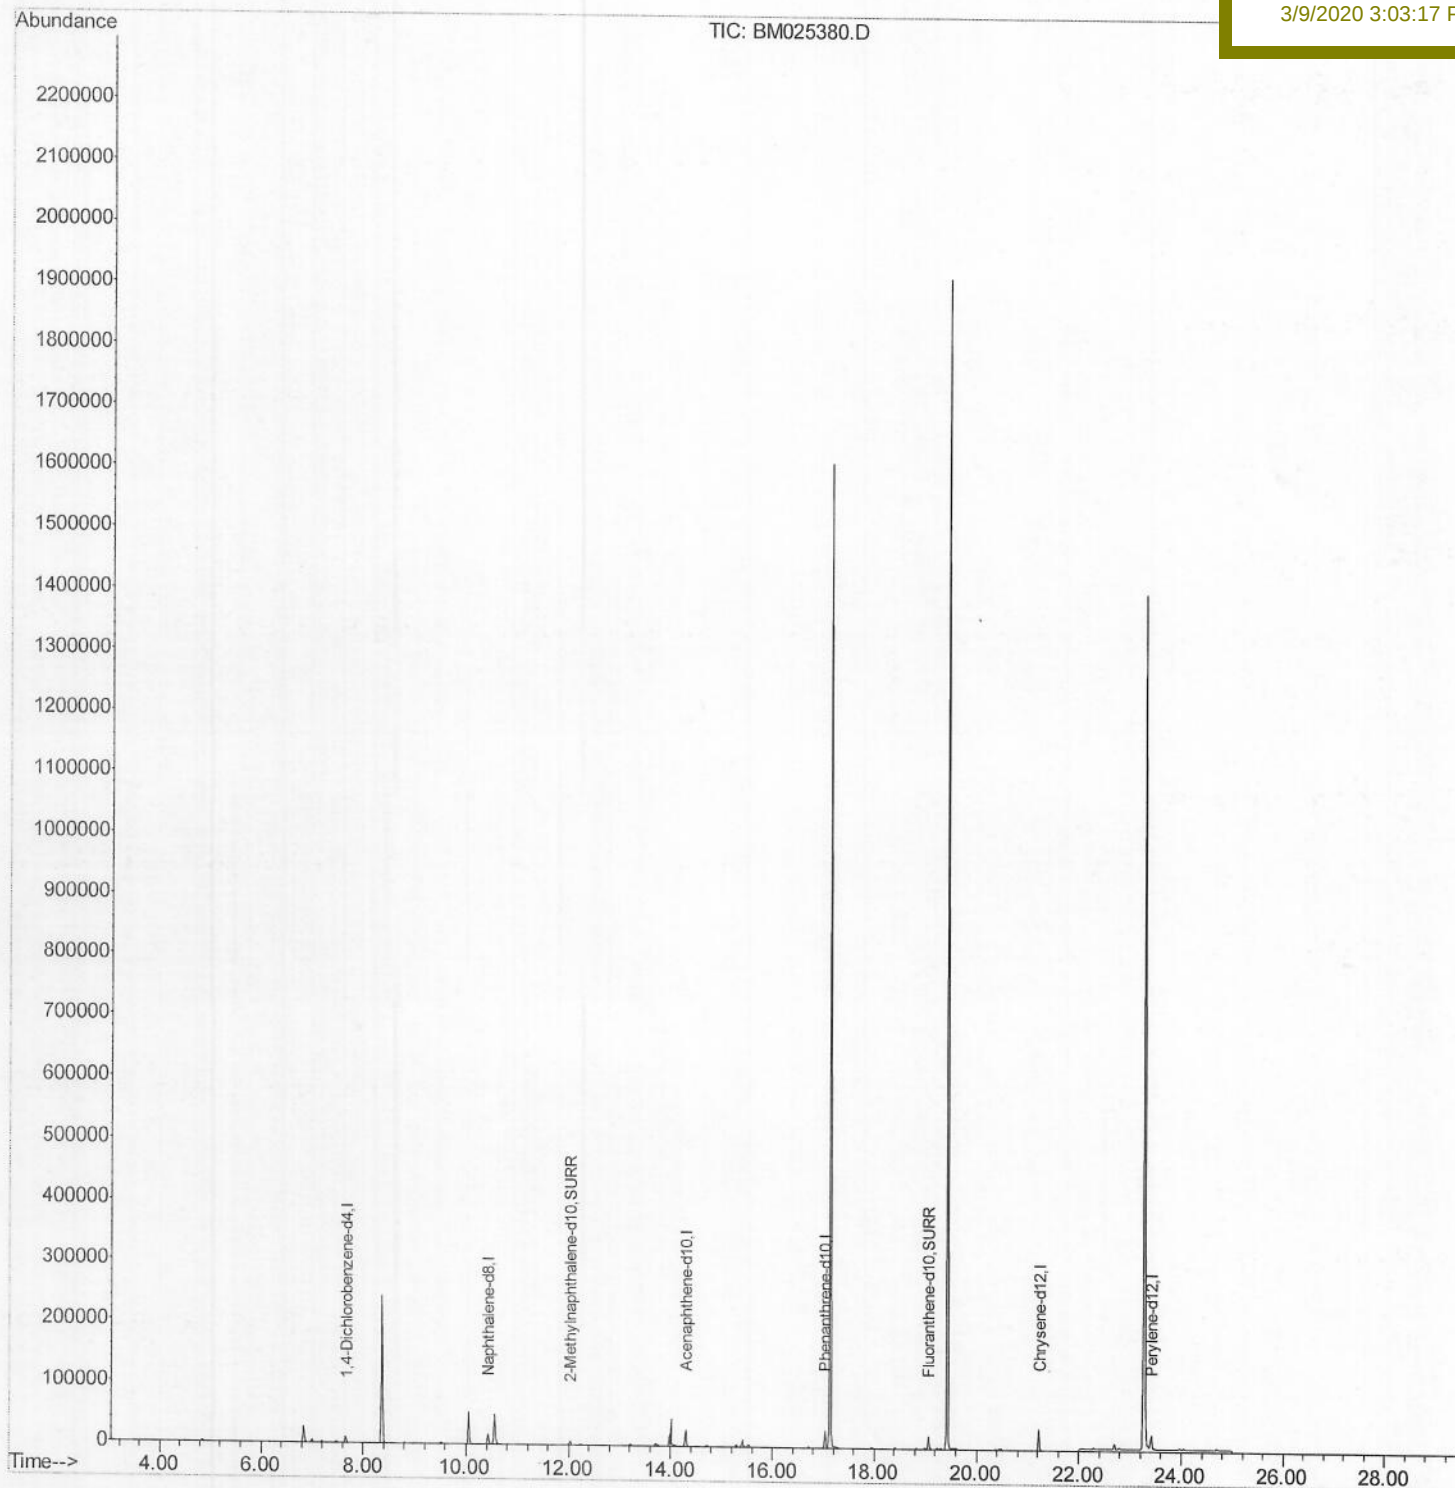

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\

Data File : BM025380.D

Acq On : 08 Mar 2020 11:24

Operator : CG/JU

Sample : L1616-22

Misc :

ALS Vial : 66 Sample Multiplier: 1

Quant Time: Mar 09 01:15:05 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 08:02:03 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBDR6

Manual Integrations

APPROVED

mohammad

3/9/2020 3:03:17 PM

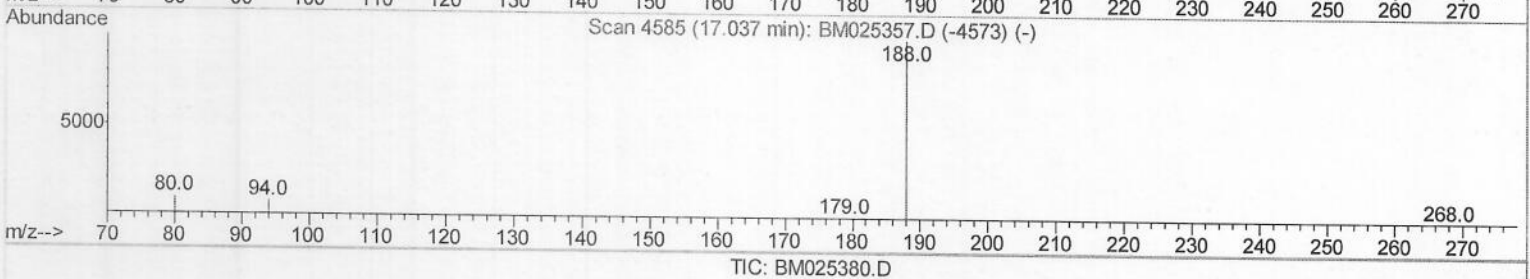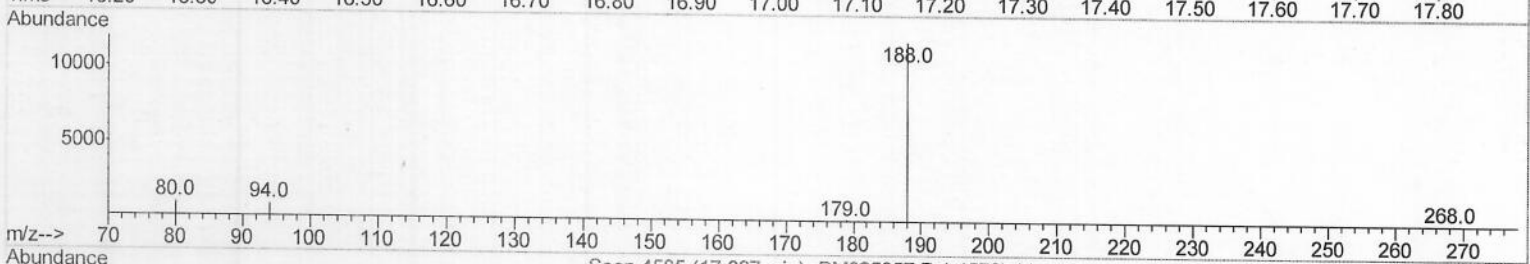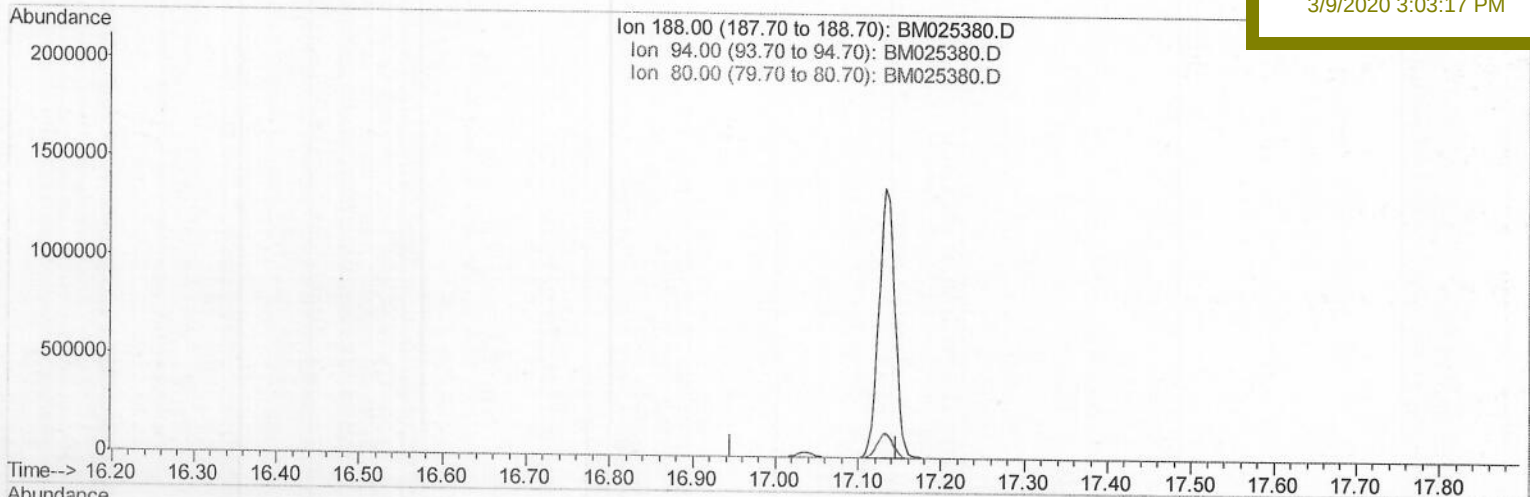

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\

Data File : BM025380.D

Acq On : 08 Mar 2020 11:24

Operator : CG/JU

Sample : L1616-22

Misc :

ALS Vial : 66 Sample Multiplier: 1

Quant Time: Mar 09 01:15:05 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 08:02:03 2020




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

DBDR6

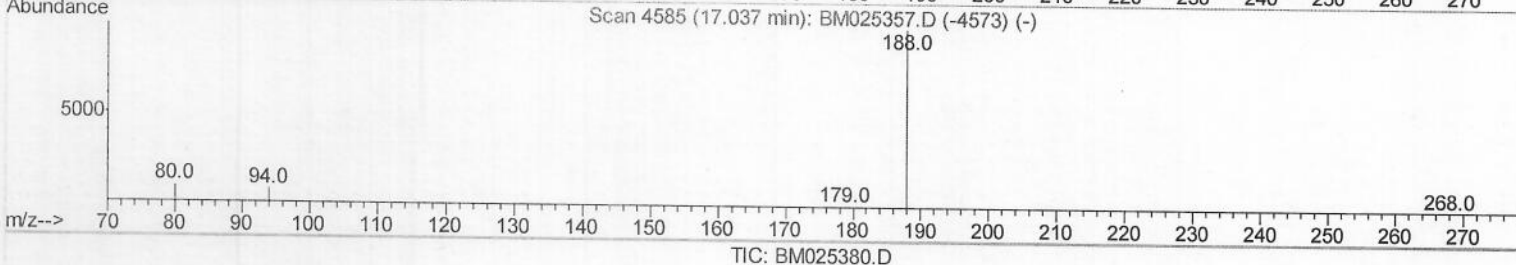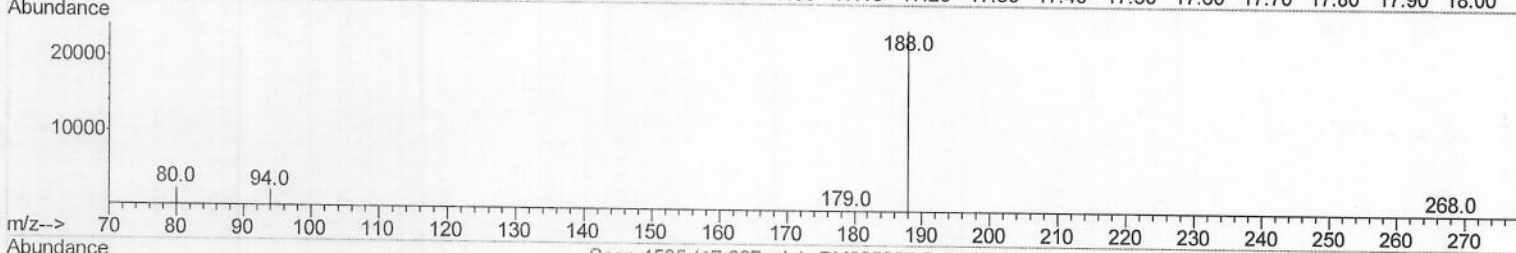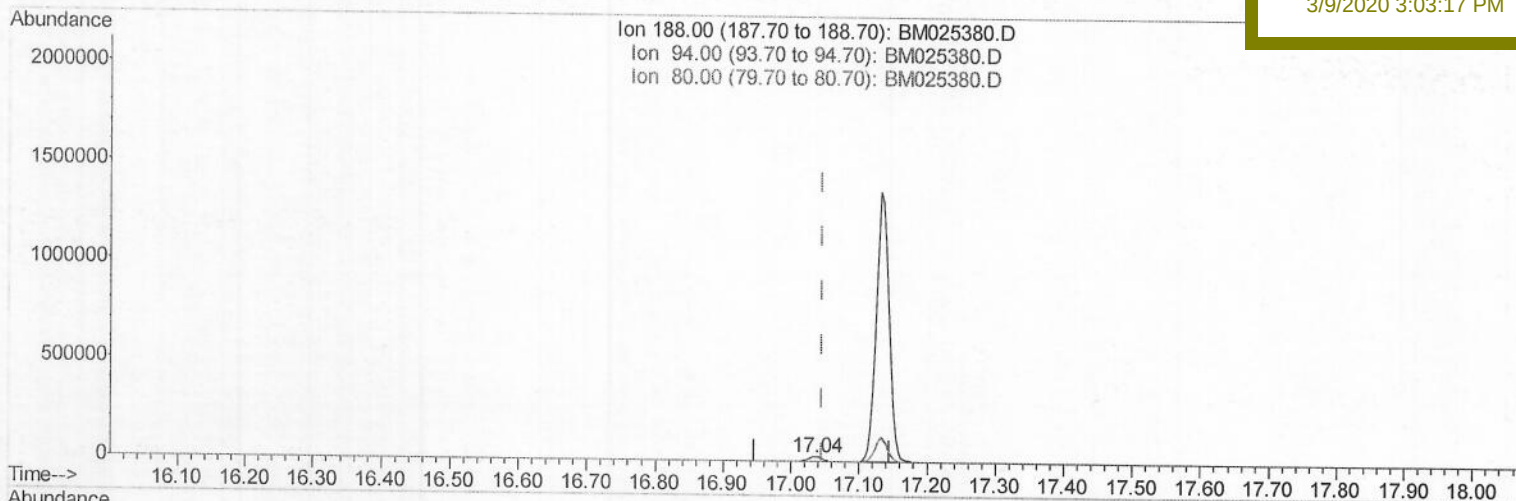Manual Integrations
APPROVEDmohammad
3/9/2020 3:03:17 PM

(10) Phenanthrene-d10 (I)

17.036min (-0.010) 0.40ng/ul m>Ju 03/11/20

response 32956

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	8.25#
80.00	22.60	9.45#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
 Data File : BM025380.D
 Acq On : 08 Mar 2020 11:24
 Operator : CG/JU
 Sample : L1616-22
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Quant Time: Mar 09 01:55:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DBDR6

Manual Integrations
 APPROVED

mohammad
 3/9/2020 3:03:17 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	4701	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.43	136	20096	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.29	164	14311	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.04	188	32956m)	0.40	ng/ul	-0.01
16) Chrysene-d12	21.22	240	29891	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	28752	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev (Min)
4) 2-Methylnaphthalene-d10	12.03	152	8511	0.23	ng/ul	-0.01
14) Fluoranthene-d10	19.06	212	23051	0.21	ng/ul	-0.01

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed