




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
 Data File : BM025390.D
 Acq On : 08 Mar 2020 17:58
 Operator : CG/JU
 Sample : L1617-06
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDS0

Manual Integrations
 APPROVED

mohammad
 3/9/2020 3:03:37 PM

Quant Time: Mar 09 02:13:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

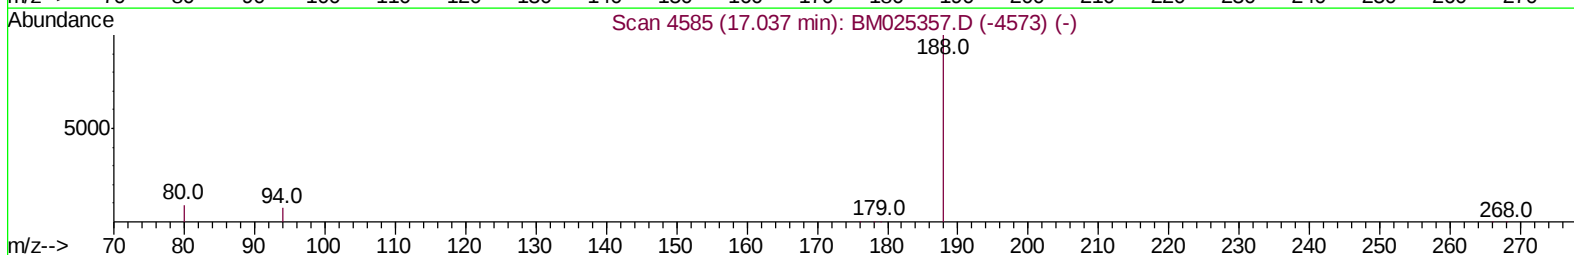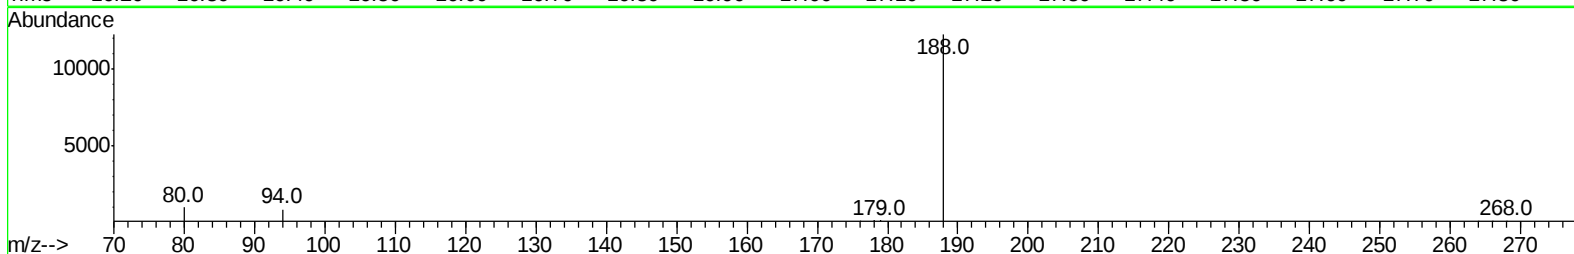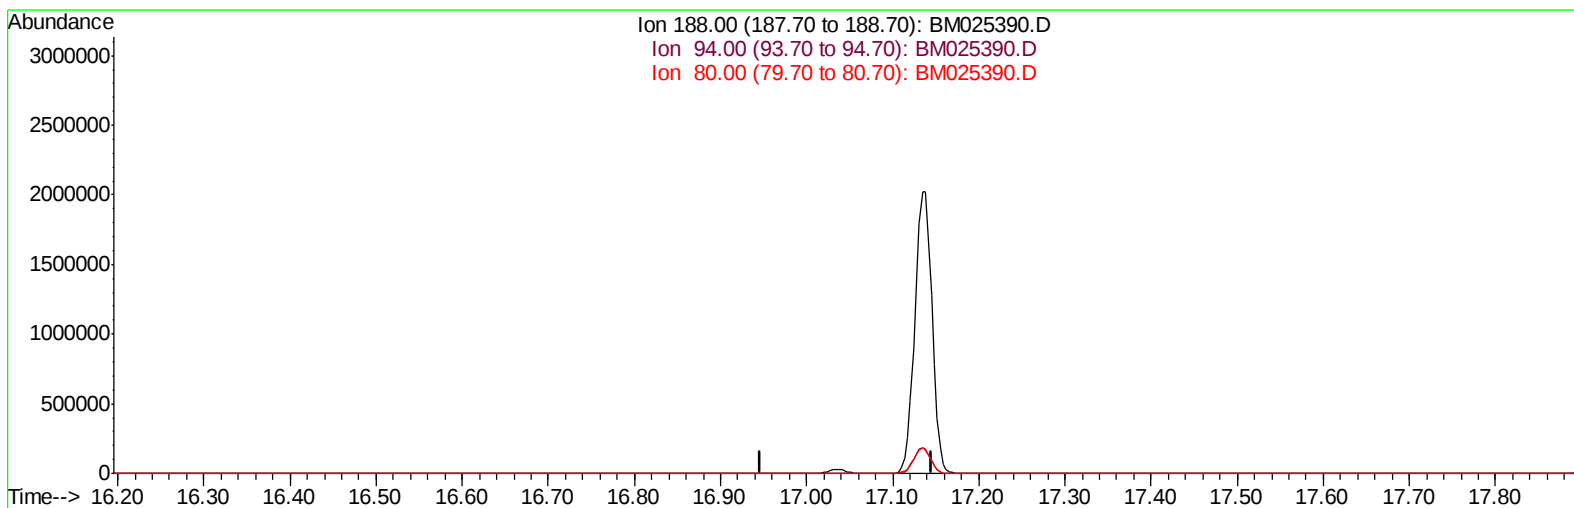

TIC: BM025390.D

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
Data File : BM025390.D
Acq On : 08 Mar 2020 17:58
Operator : CG/JU
Sample : L1617-06
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBDS0

Manual Integrations
APPROVED

mohammad
3/9/2020 3:03:37 PM

Quant Time: Mar 09 02:13:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

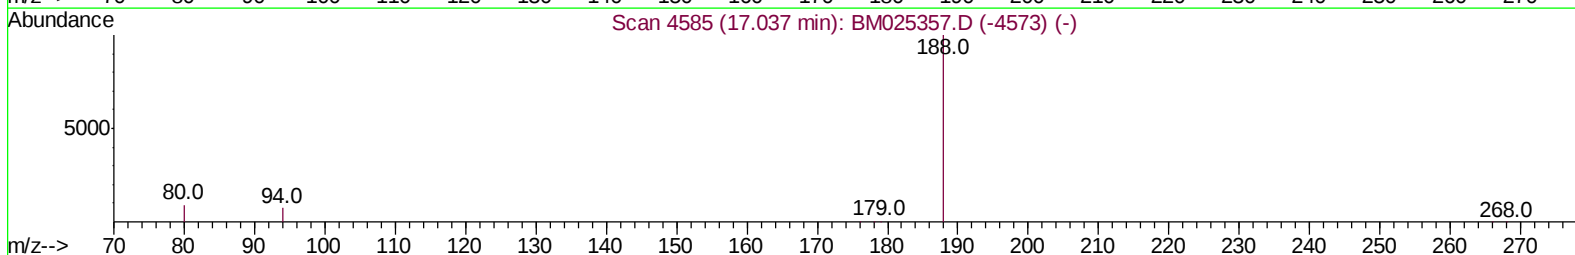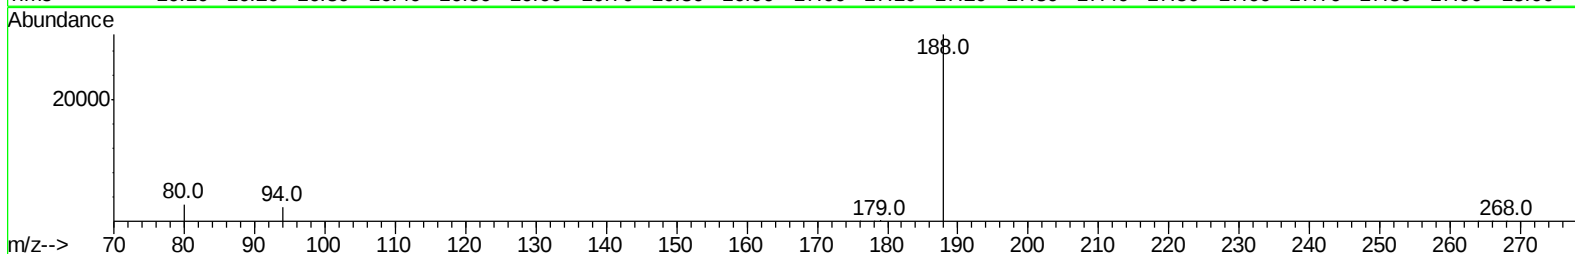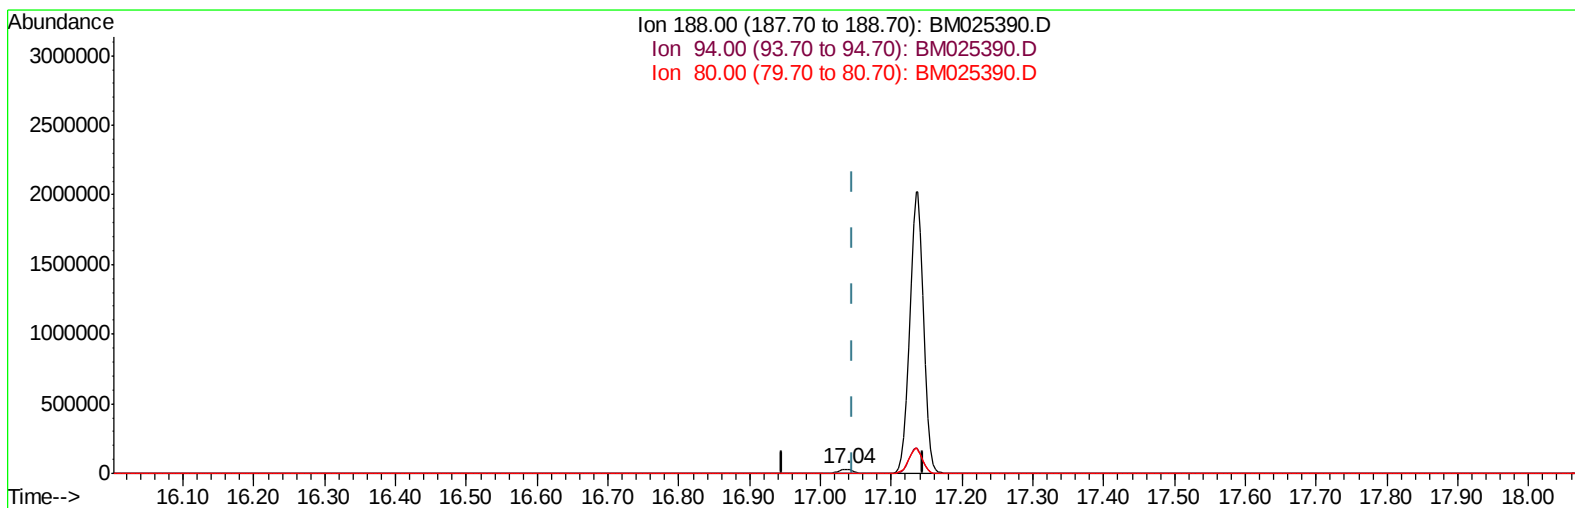

TIC: BM025390.D

(10) Phenanthrene-d10 (I)

17.037min (-0.009) 0.40ng/ul m

response 42107

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	8.03#
80.00	22.60	9.35#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
 Data File : BM025390.D
 Acq On : 08 Mar 2020 17:58
 Operator : CG/JU
 Sample : L1617-06
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDS0

Manual Integrations
 APPROVED

mohammad
 3/9/2020 3:03:37 PM

Quant Time: Mar 09 02:14:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	5793	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	25049	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.29	164	18047	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.04	188	42107m	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	36802	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	32485	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.02	152	13549	0.29	ng/ul	-0.02
14) Fluoranthene-d10	19.07	212	36423	0.27	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
Data File : BM025390.D
Acq On : 08 Mar 2020 17:58
Operator : CG/JU
Sample : L1617-06
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBDS0

Manual Integrations
APPROVED

mohammad
3/9/2020 3:03:37 PM

Quant Time: Mar 09 02:14:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

