

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
 Data File : BM025388.D
 Acq On : 08 Mar 2020 16:47
 Operator : CG/JU
 Sample : L1617-04
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDR8

Quant Time: Mar 09 01:15:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	5718	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.43	136	24366	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.29	164	17365	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.03	188	40861	0.40	ng/ul	-0.01
16) Chrysene-d12	21.22	240	33371	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	29021	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	4836	0.11	ng/ul	-0.02
14) Fluoranthene-d10	19.07	212	13583	0.10	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.08	178	2875	0.022	ng/ul	Ovalue 97




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
Data File : BM025388.D
Acq On : 08 Mar 2020 16:47
Operator : CG/JU
Sample : L1617-04
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBDR8

Quant Time: Mar 09 01:15:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

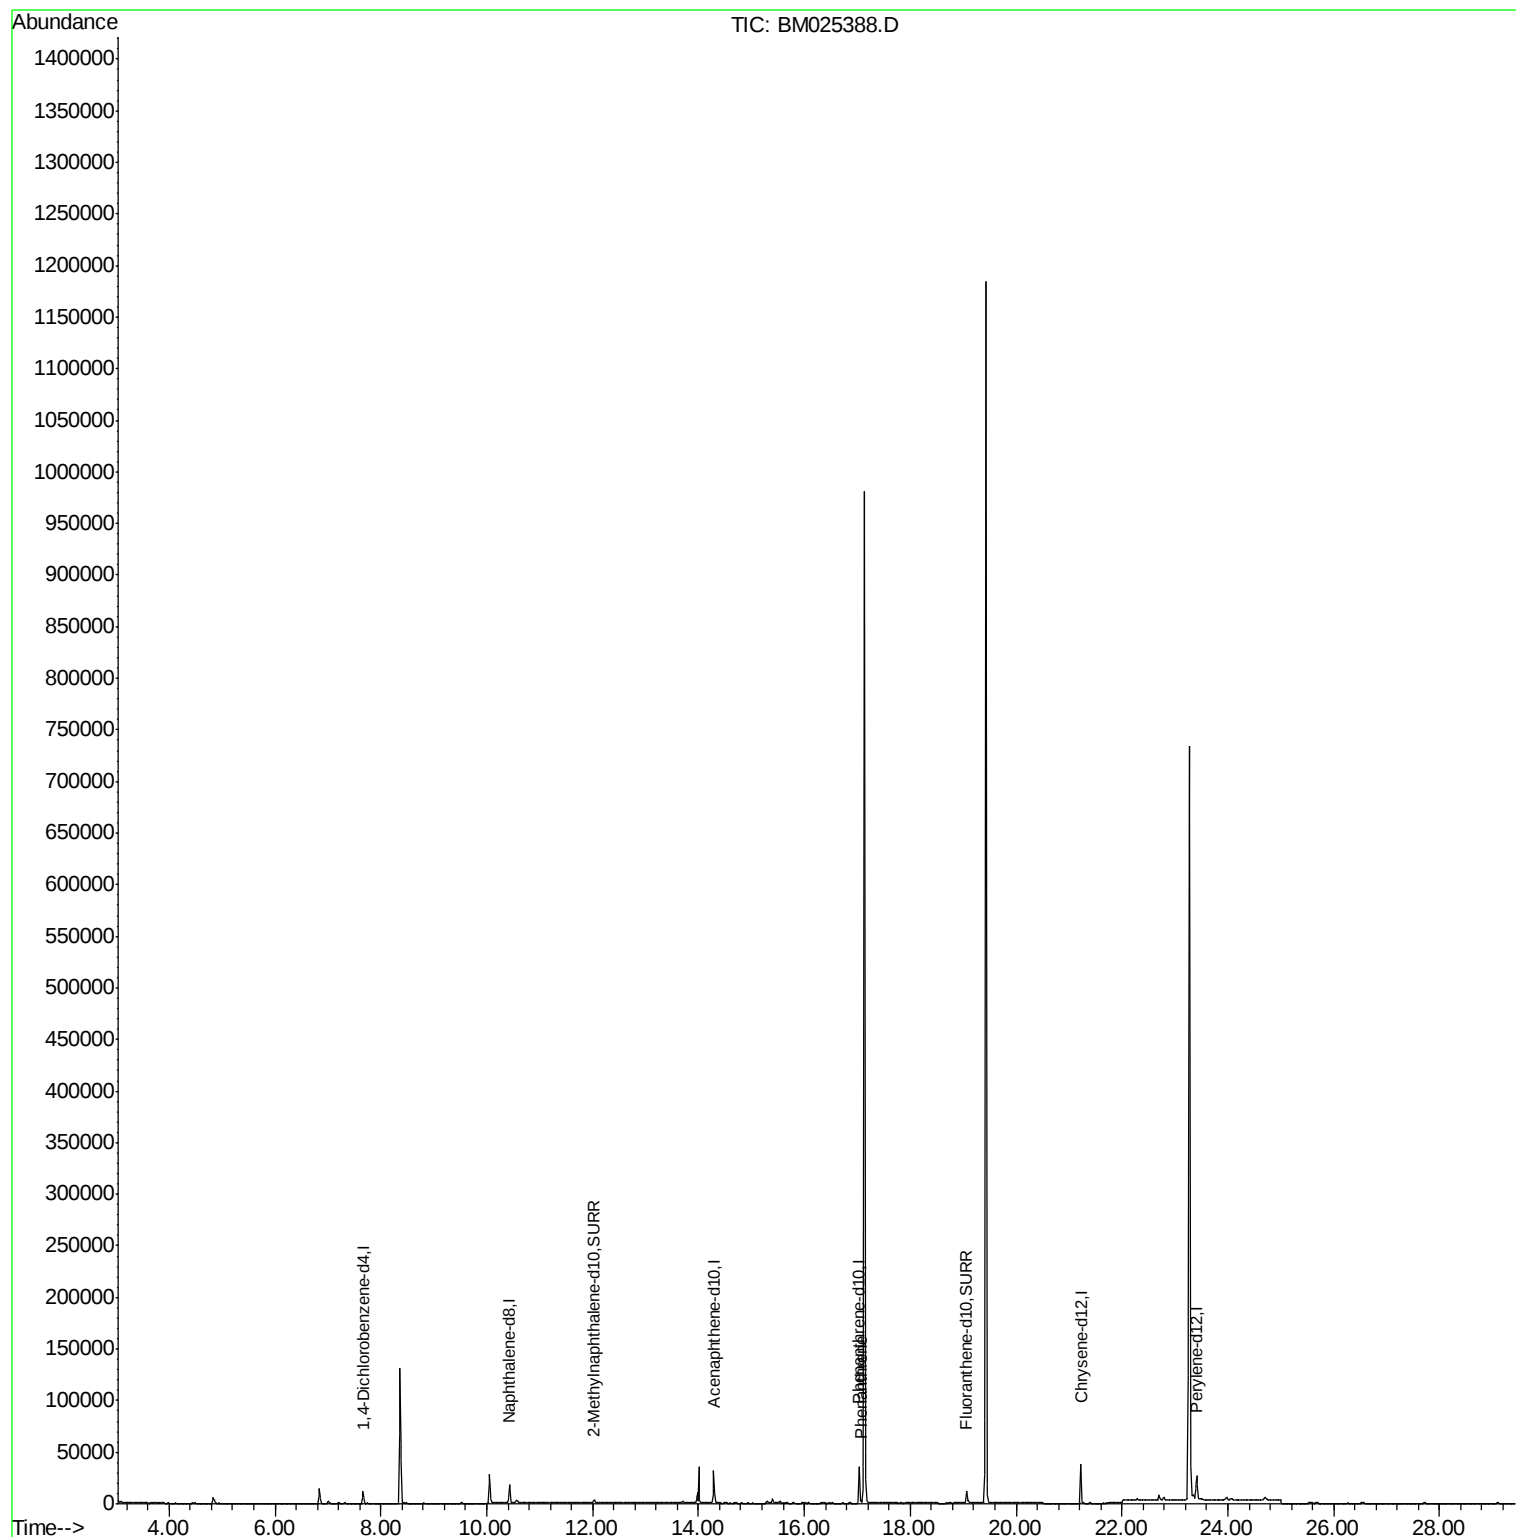

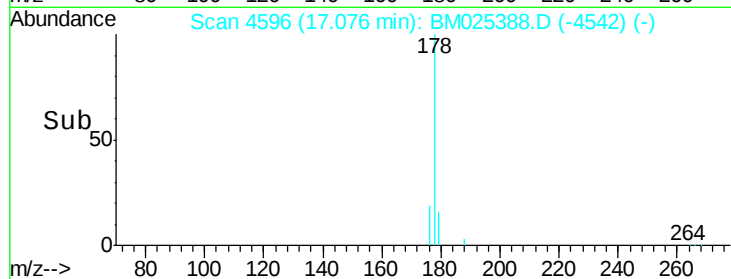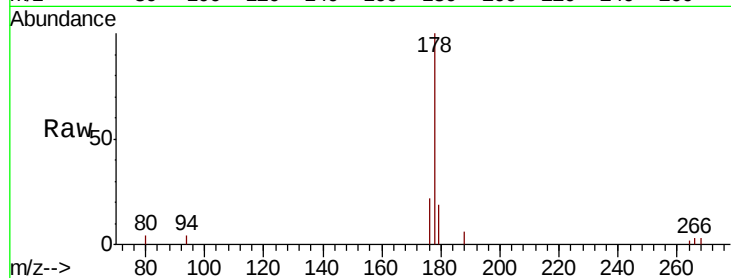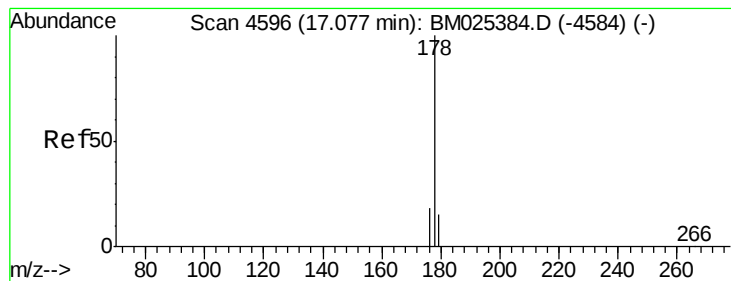

#12

Phenanthrene

Concen: 0.022 ng/ul

RT: 17.08 min Scan# 4596

Delta R.T. -0.01 min

Lab File: BM025388.D

Acq: 08 Mar 2020 16:47

Instrument :

BNA_M

ClientSampleId :

DBDR8

Tot Ion:178 Resp: 2875

Ion Ratio Lower Upper

178 100

179 19.3 14.0 21.0

176 21.5 16.6 24.8

