

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030819\
 Data File : BM019086.D
 Acq On : 08 Mar 2019 22:40
 Operator : JU/SJ
 Sample : K1807-35
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-11

Quant Time: Mar 09 01:00:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 05 03:36:13 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	164520	20.00	ng	-0.01
21) Naphthalene-d8	10.46	136	585476	20.00	ng	-0.01
39) Acenaphthene-d10	14.32	164	304868	20.00	ng	-0.01
64) Phenanthrene-d10	17.08	188	655582	20.00	ng	0.00
76) Chrysene-d12	21.27	240	737321	20.00	ng	-0.01
87) Perylene-d12	23.51	264	869439	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.27	112	1125572	112.10	ng	0.00
7) Phenol-d6	6.85	99	1494888	105.68	ng	-0.01
23) Nitrobenzene-d5	8.83	82	918297	72.52	ng	-0.02
42) 2,4,6-Tribromophenol	15.82	330	460676	104.83	ng	-0.01
45) 2-Fluorobiphenyl	12.93	172	1385992	60.35	ng	-0.02
79) Terphenyl-d14	19.71	244	2163268	60.52	ng	-0.02
Target Compounds						
50) Dimethylphthalate	13.79	163	120985	4.762	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030819\
Data File : BM019086.D
Acq On : 08 Mar 2019 22:40
Operator : JU/SJ
Sample : K1807-35
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-11

Quant Time: Mar 09 01:00:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 05 03:36:13 2019
Response via : Initial Calibration

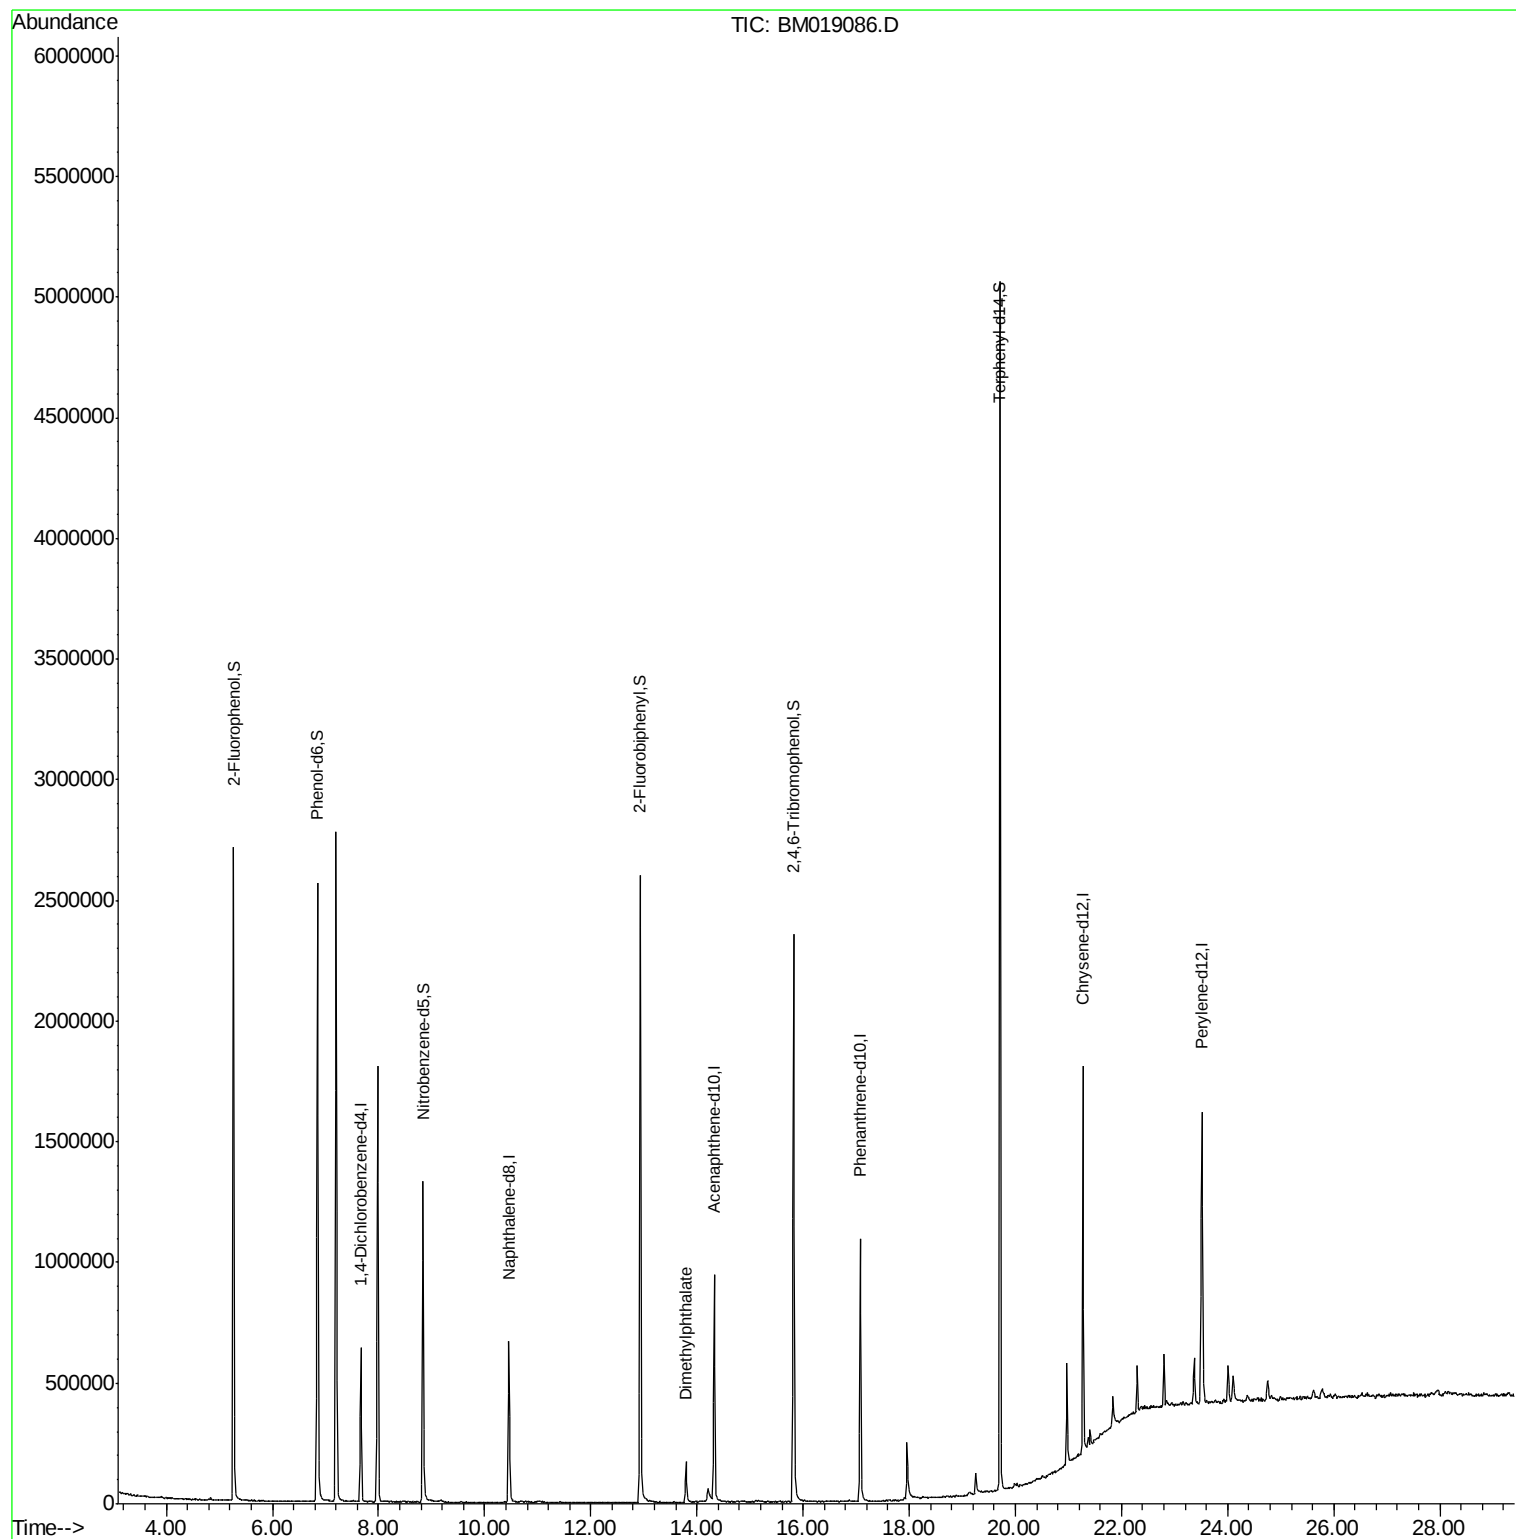

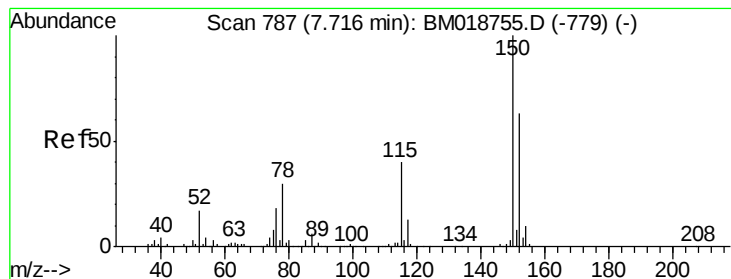


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.67 min Scan# 779
Delta R.T. -0.01 min
Lab File: BM019086.D
Acq: 08 Mar 2019 22:40

Instrument :
BNA_M
ClientSampleId :
TP-11

Tgt Ion:152 Resp: 164520
Ion Ratio Lower Upper
152 100
150 151.1 127.3 190.9
115 61.6 50.8 76.2

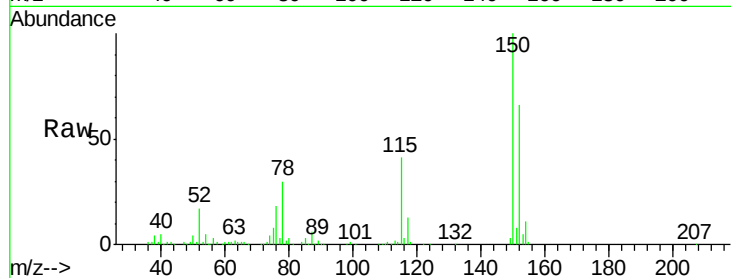


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

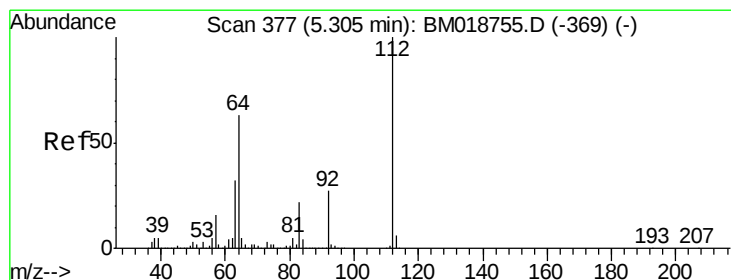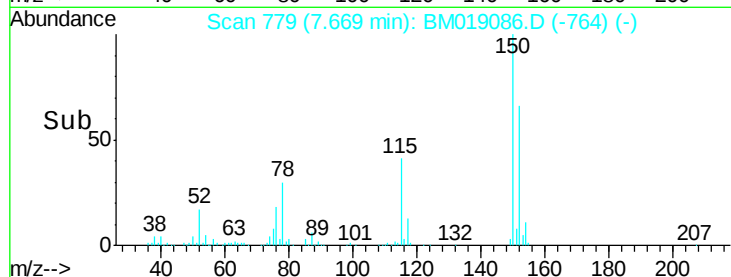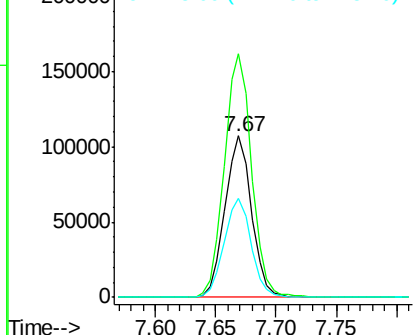



#5


2-Fluorophenol
Concen: 112.097 ng
RT: 5.27 min Scan# 371
Delta R.T. -0.01 min
Lab File: BM019086.D
Acq: 08 Mar 2019 22:40

Tgt Ion:112 Resp: 1125572
Ion Ratio Lower Upper
112 100
64 61.6 50.6 75.8
63 31.7 25.7 38.5

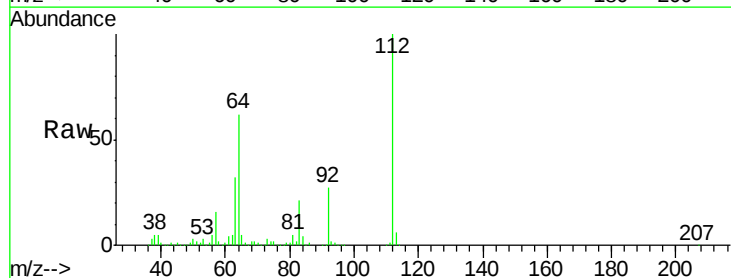

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

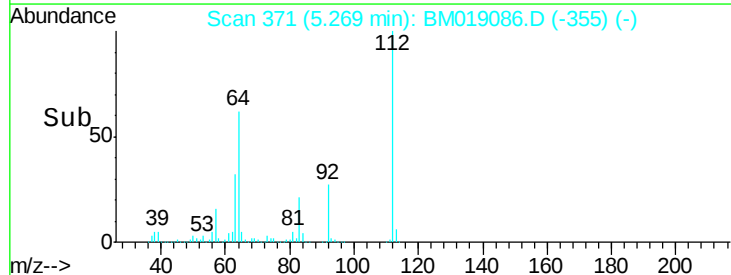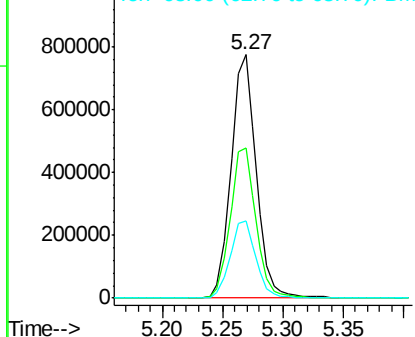

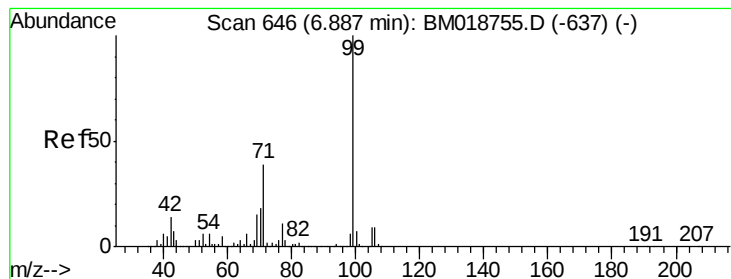

#7

Phenol-d6

Concen: 105.680 ng

RT: 6.85 min Scan# 639

Delta R.T. -0.01 min

Lab File: BM019086.D

Acq: 08 Mar 2019 22:40

Instrument :

BNA_M

ClientSampleId :

TP-11


Tgt Ion: 99 Resp: 1494888

Ion Ratio Lower Upper

99 100

42 14.1 11.0 16.6




71 38.4 31.3 46.9

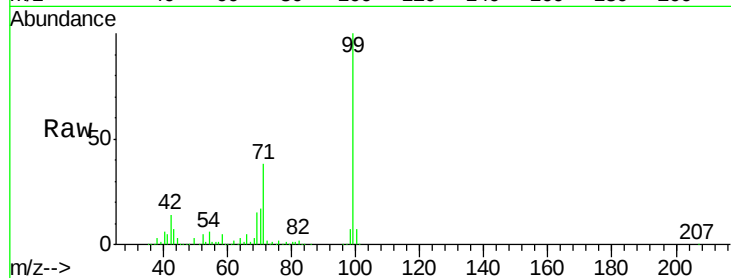

Abundance Ion 99.00 (98.70 to 99.70): BM018755.D (-637) (-)

Ion 42.00 (41.70 to 42.70): BM018755.D (-637) (-)

Ion 71.00 (70.70 to 71.70): BM018755.D (-637) (-)

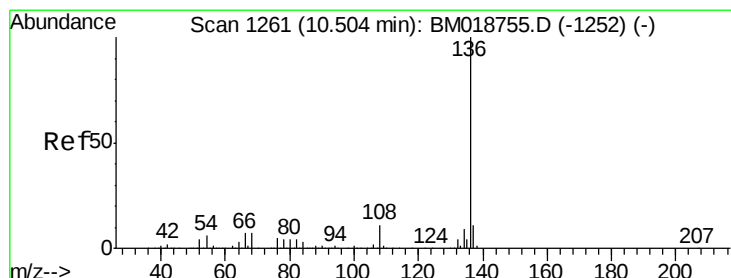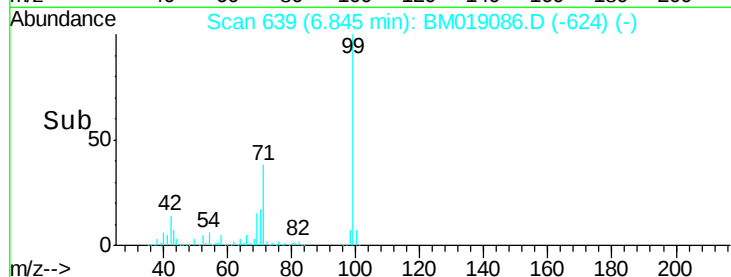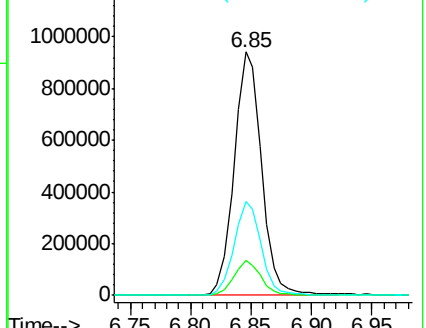

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.46 min Scan# 1253

Delta R.T. -0.01 min

Lab File: BM019086.D

Acq: 08 Mar 2019 22:40

Tgt Ion: 136 Resp: 585476


Ion Ratio Lower Upper

136 100

137 11.0 8.8 13.2

54 6.8 5.0 7.6

68 7.8 5.5 8.3


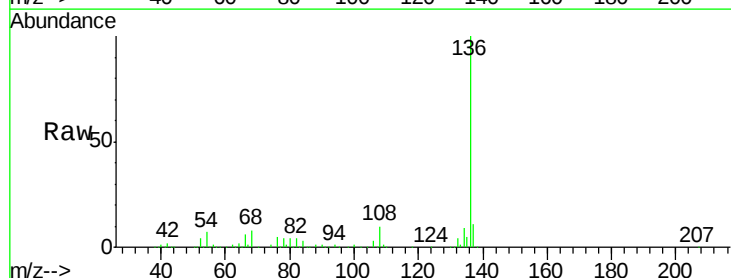


Abundance Ion 136.00 (135.70 to 136.70): BM018755.D (-1252) (-)

Ion 137.00 (136.70 to 137.70): BM018755.D (-1252) (-)

Ion 54.00 (53.70 to 54.70): BM018755.D (-1252) (-)

Ion 68.00 (67.70 to 68.70): BM018755.D (-1252) (-)



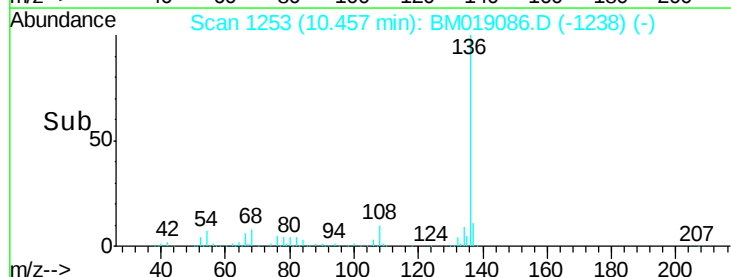
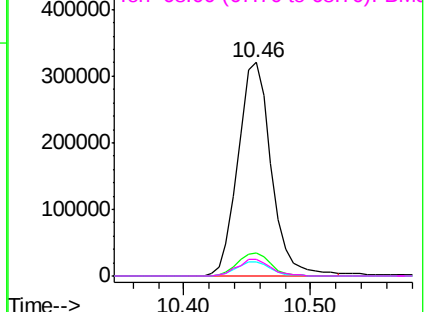




#23
 Nitrobenzene-d5
 Concen: 72.524 ng
 RT: 8.83 min Scan# 977
 Delta R.T. -0.02 min
 Lab File: BM019086.D
 Acq: 08 Mar 2019 22:40




Instrument :
 BNA_M
 ClientSampleId :
 TP-11

Tgt Ion	Ratio	Lower	Upper
82	100		
128	37.3	29.9	44.9
54	38.1	29.1	43.7

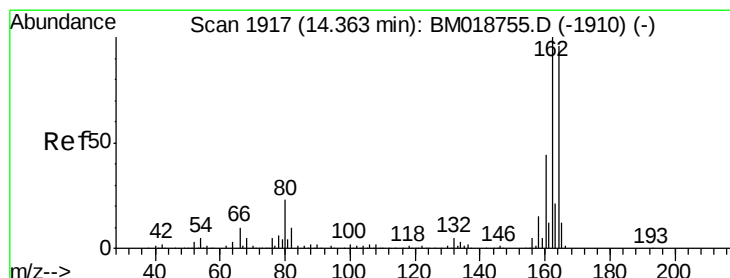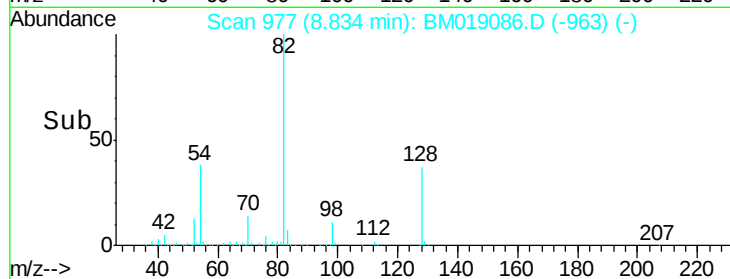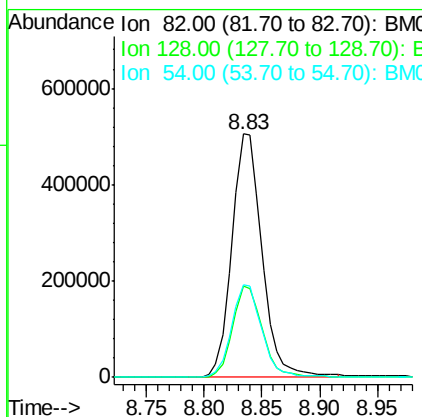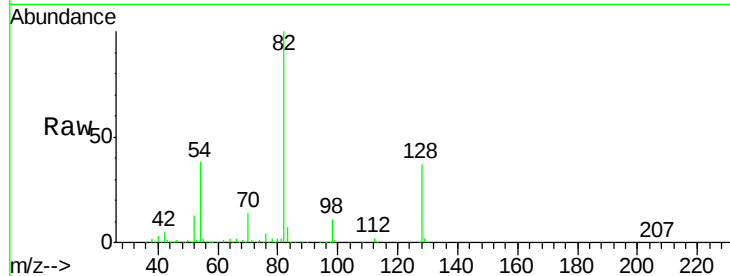

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.32 min Scan# 1910
 Delta R.T. -0.01 min
 Lab File: BM019086.D
 Acq: 08 Mar 2019 22:40

Tgt Ion	Ratio	Lower	Upper
164	100		
162	105.0	83.4	125.0
160	46.5	36.6	55.0

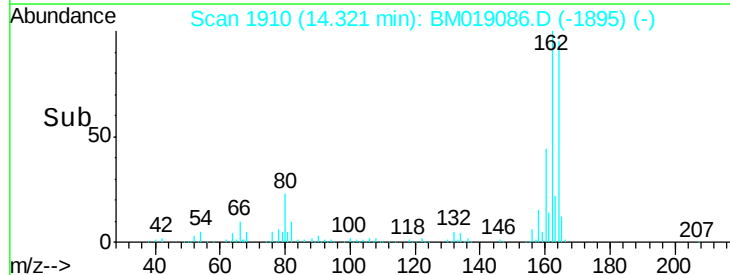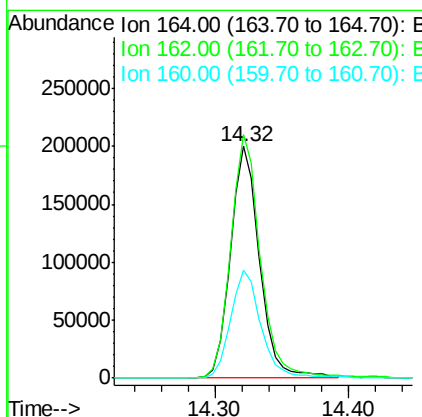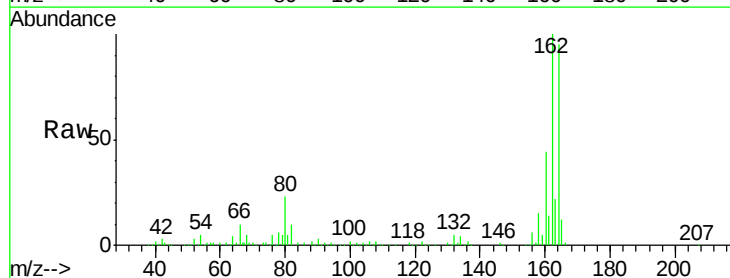







#42
 2,4,6-Tribromophenol
 Concen: 104.828 ng
 RT: 15.82 min Scan# 2165
 Delta R.T. -0.01 min
 Lab File: BM019086.D
 Acq: 08 Mar 2019 22:40

Instrument :
 BNA_M
 ClientSampleId :
 TP-11

Tgt Ion:330 Resp: 460676
 Ion Ratio Lower Upper
 330 100
 332 97.5 76.9 115.3
 141 35.4 28.7 43.1

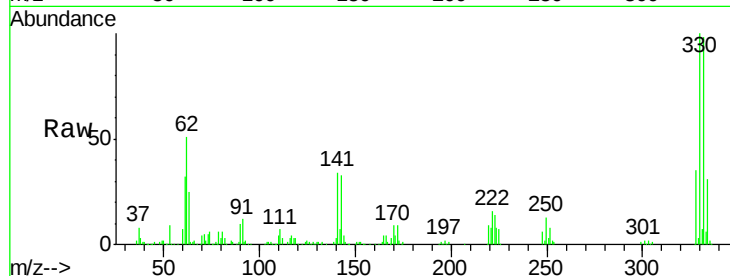


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

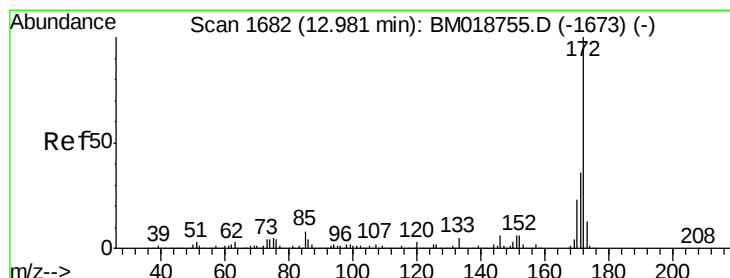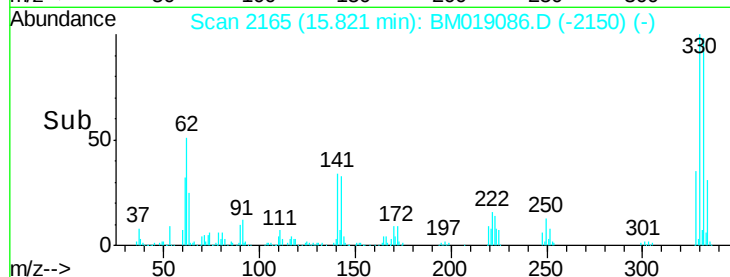
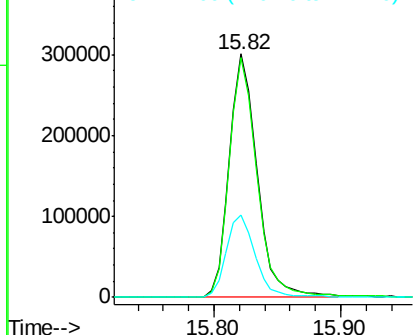



#45
 2-Fluorobiphenyl
 Concen: 60.350 ng
 RT: 12.93 min Scan# 1674
 Delta R.T. -0.02 min
 Lab File: BM019086.D
 Acq: 08 Mar 2019 22:40

Tgt Ion:172 Resp: 1385992
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.0 43.6
 170 23.1 18.6 28.0

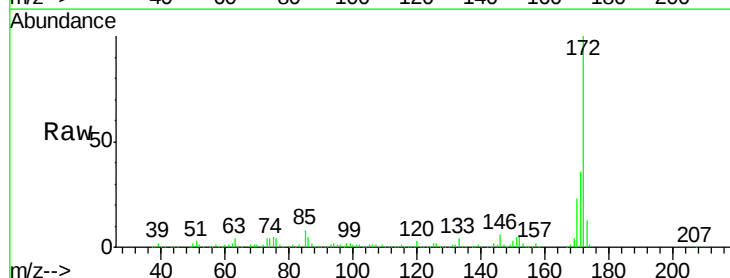

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

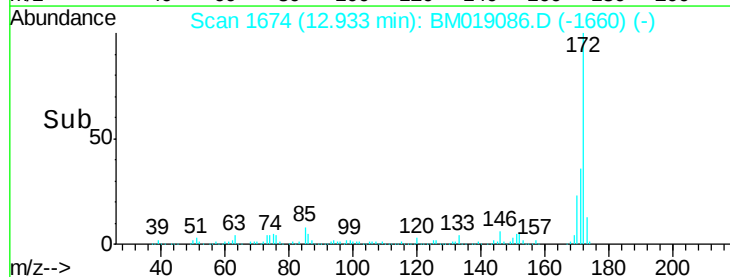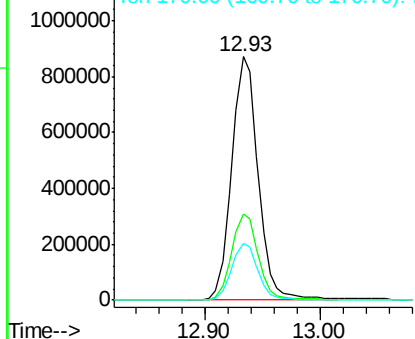


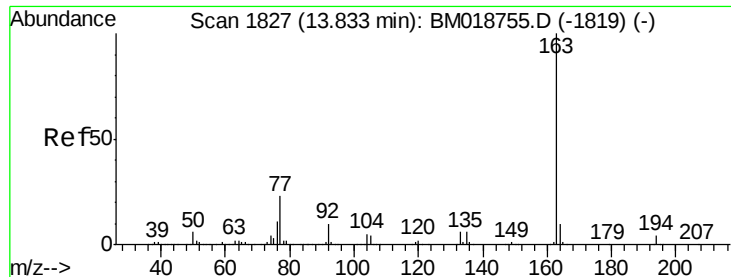




#50
Dimethylphthalate
Concen: 4.762 ng
RT: 13.79 min Scan# 1820
Delta R.T. -0.01 min
Lab File: BM019086.D
Acq: 08 Mar 2019 22:40

Instrument :
BNA_M
ClientSampleId :
TP-11

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.2	4.8
164	10.5	7.8	11.8

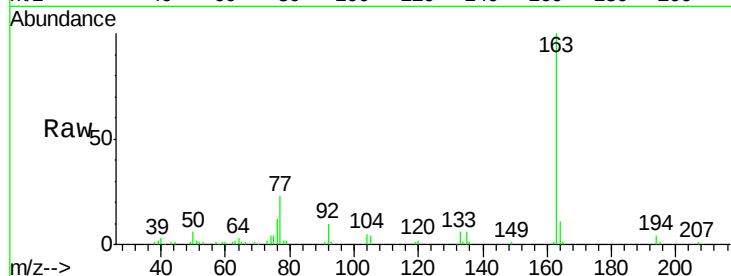


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

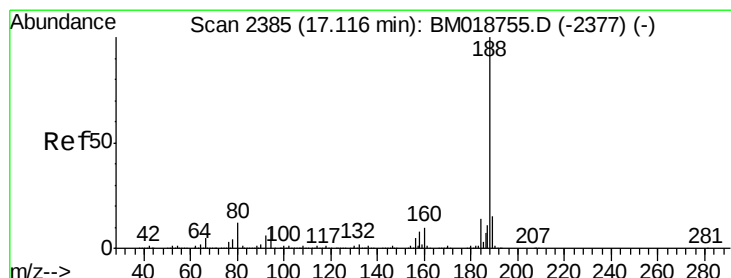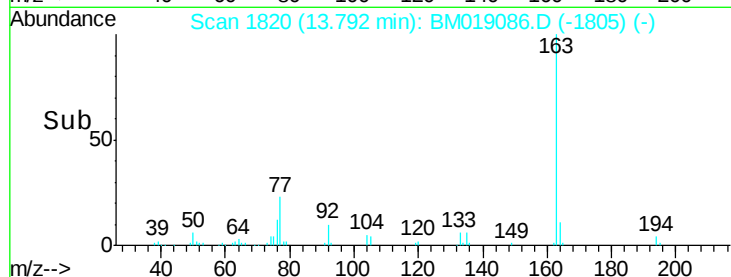
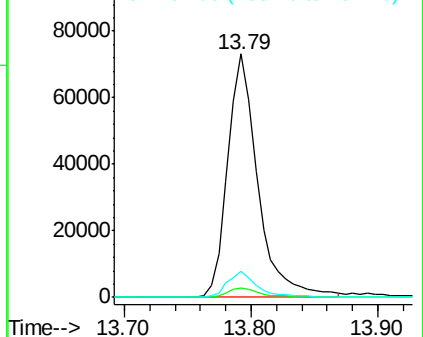



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.08 min Scan# 2379
Delta R.T. -0.01 min
Lab File: BM019086.D
Acq: 08 Mar 2019 22:40

Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.6	8.2	12.2
80	11.5	9.7	14.5

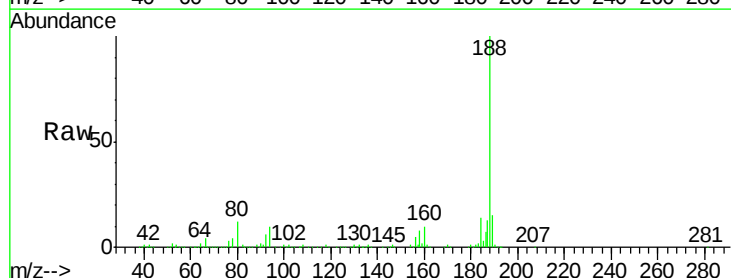

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM0
Ion 80.00 (79.70 to 80.70): BM0



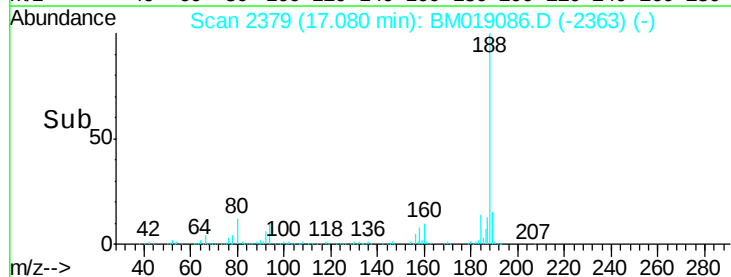
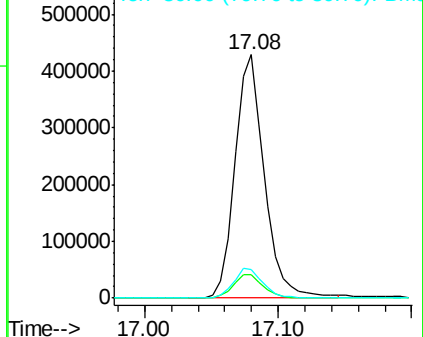


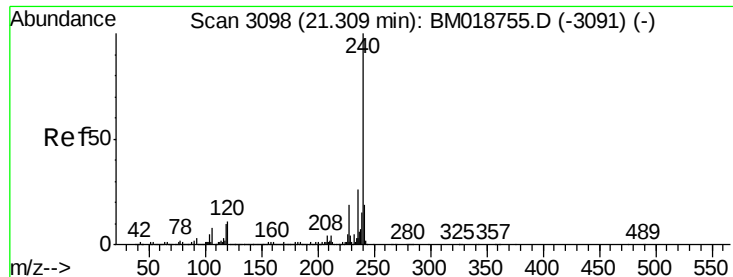

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.27 min Scan# 3092
Delta R.T. -0.01 min
Lab File: BM019086.D
Acq: 08 Mar 2019 22:40




Instrument :
BNA_M
ClientSampleId :
TP-11


Tgt Ion:240 Resp: 737321
Ion Ratio Lower Upper
240 100
120 11.3 8.9 13.3
236 25.6 20.9 31.3

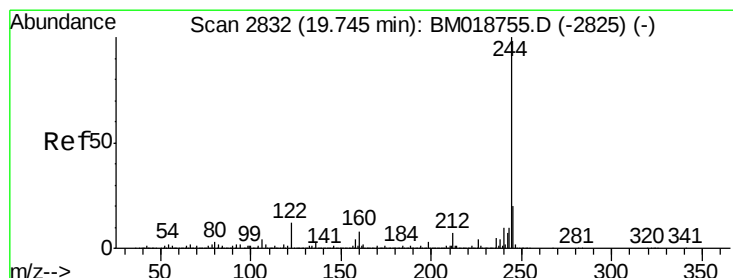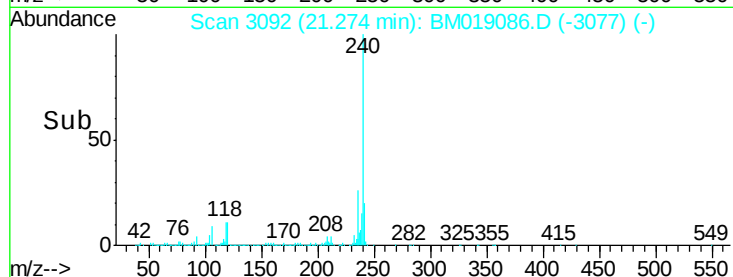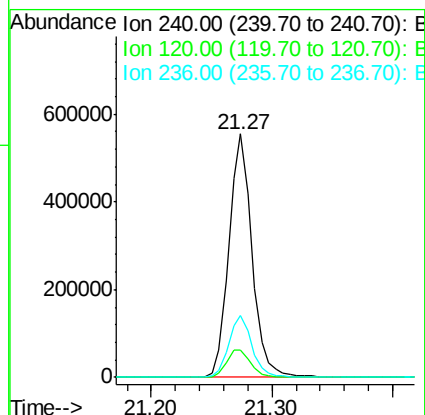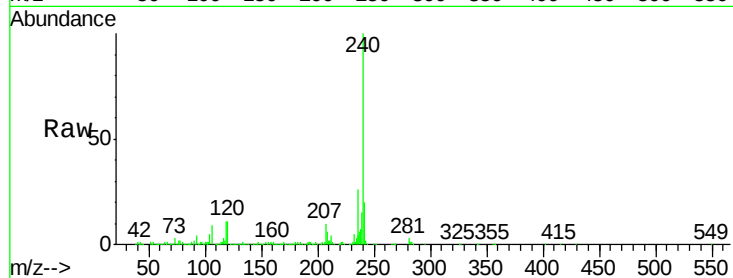

#79
Terphenyl-d14
Concen: 60.524 ng
RT: 19.71 min Scan# 2826
Delta R.T. -0.02 min
Lab File: BM019086.D
Acq: 08 Mar 2019 22:40

Tgt Ion:244 Resp: 2163268
Ion Ratio Lower Upper
244 100
212 7.0 5.6 8.4
122 11.5 9.3 13.9

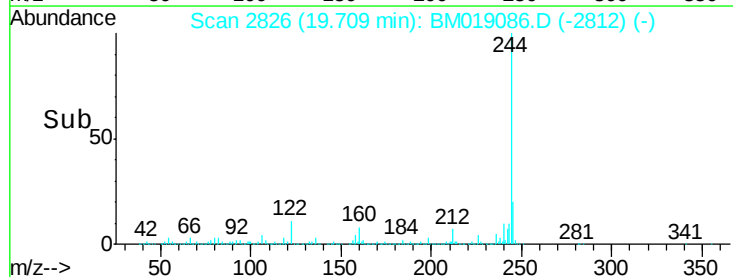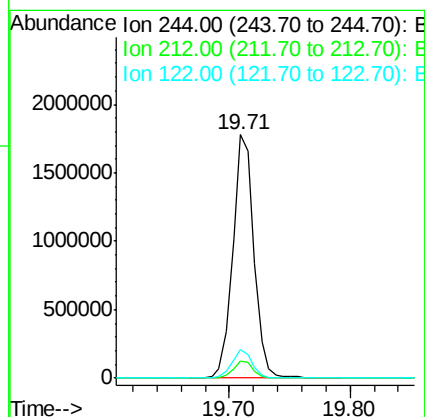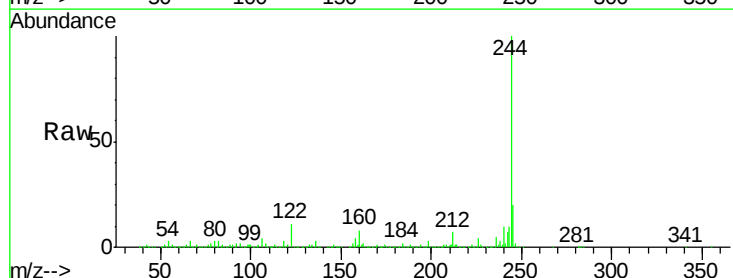

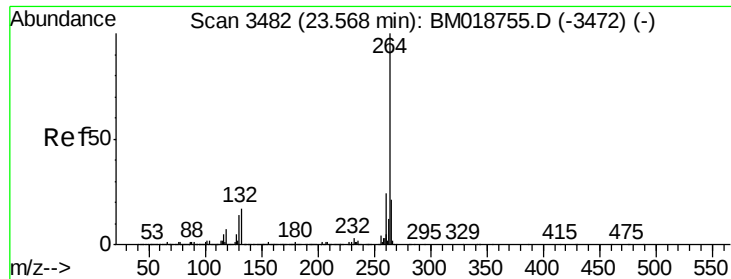

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.51 min Scan# 3473

Delta R.T. -0.02 min

Lab File: BM019086.D

Acq: 08 Mar 2019 22:40

Instrument :

BNA_M

ClientSampleId :

TP-11

Tgt Ion:264 Resp: 869439

Ion Ratio Lower Upper

264 100

260 23.7 18.9 28.3

265 22.5 17.3 25.9

