


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030819\
 Data File : BM019069.D
 Acq On : 08 Mar 2019 12:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 05 03:36:13 2019

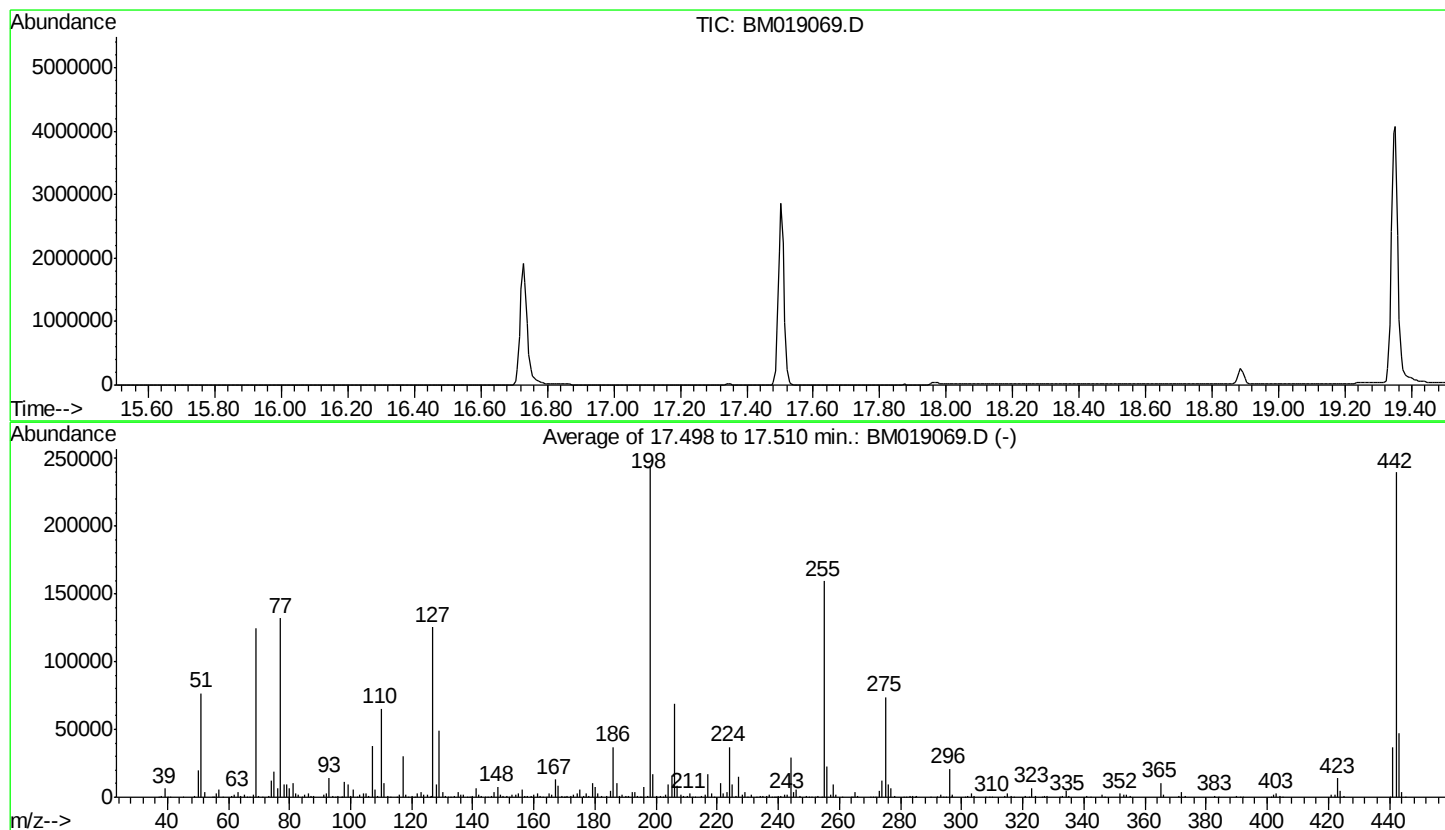

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	76885	PASS
68	69	0.00	2	1.9	2313	PASS
69	198	0.00	100	51.1	124845	PASS
70	69	0.00	2	0.6	701	PASS
127	198	10	80	51.2	125160	PASS
197	198	0.00	2	0.3	642	PASS
198	198	100	100	100.0	244501	PASS
199	198	5	9	6.8	16714	PASS
275	198	10	60	30.2	73778	PASS
365	198	1	100	4.4	10806	PASS
441	198	0.01	100	15.0	36680	PASS
442	198	50	100	97.9	239317	PASS
443	442	15	24	19.5	46752	PASS