




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034182.D
Acq On : 09 Mar 2022 12:44
Operator : CG/JU
Sample : N1775-12
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRU6

Manual IntegrationsAPPROVED

Quant Time: Mar 09 23:56:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 08 13:09:16 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/10/2022
Supervised By :Yogesh Patel 03/11/2022

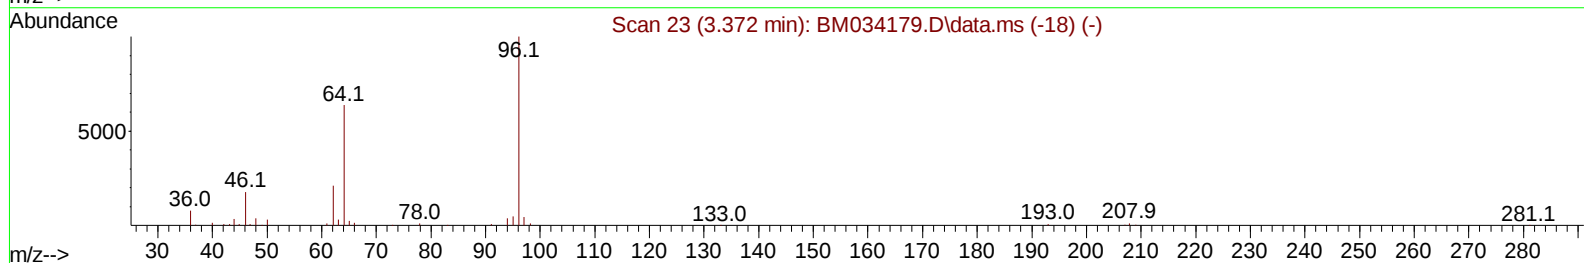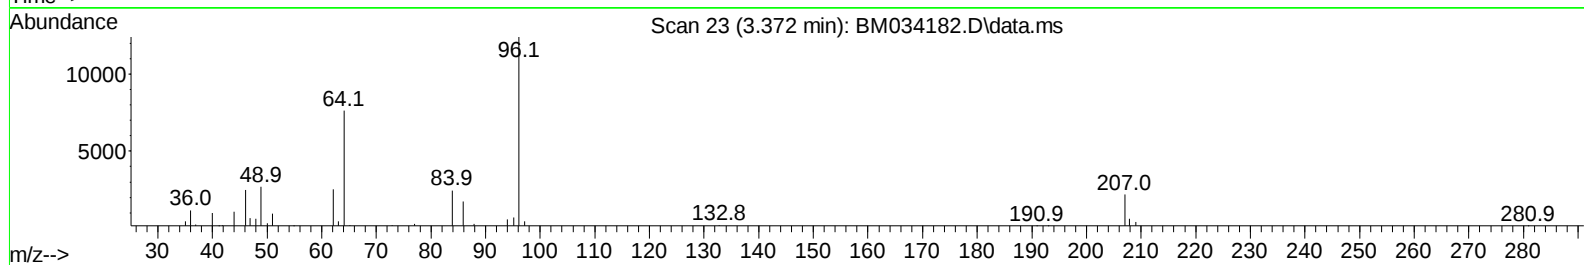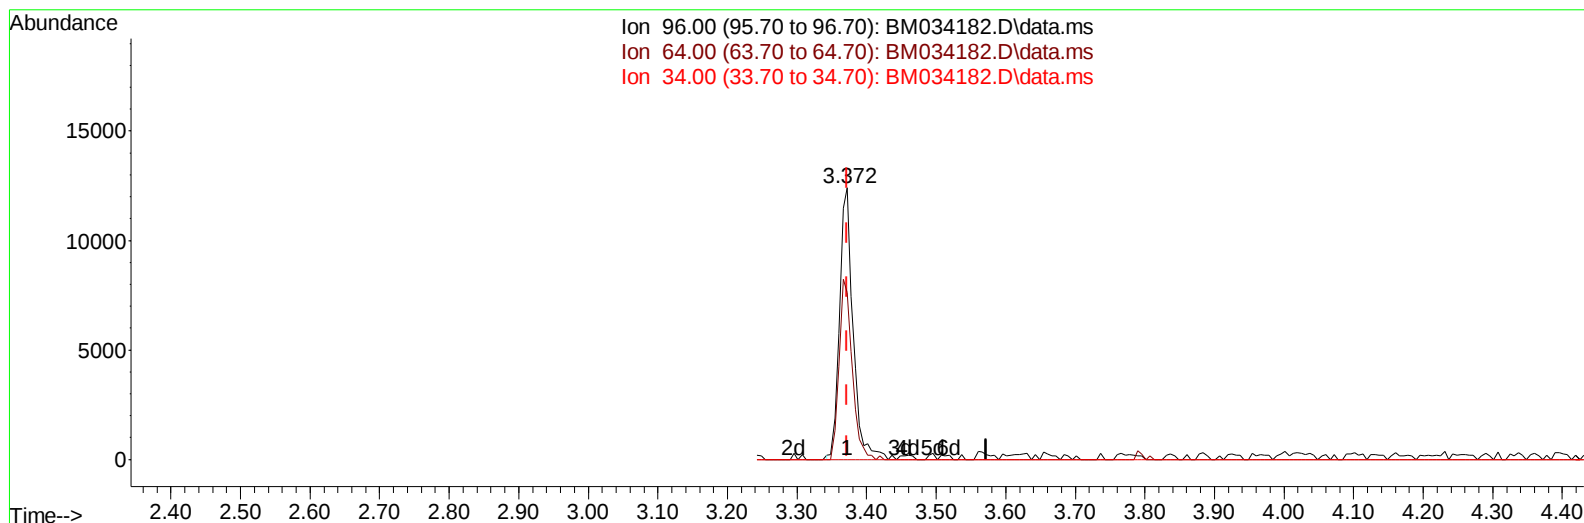

TIC: BM034182.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.372min (+ 0.000) 5.96 ng/uL

response 16791

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	61.46
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034182.D
 Acq On : 09 Mar 2022 12:44
 Operator : CG/JU
 Sample : N1775-12
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRU6

Manual IntegrationsAPPROVED

Quant Time: Mar 09 23:56:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 08 13:09:16 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/10/2022
 Supervised By :Yogesh Patel 03/11/2022

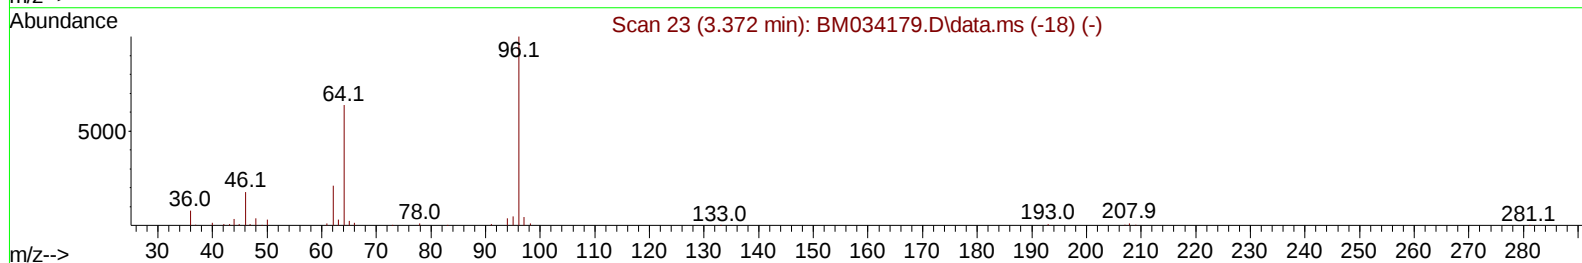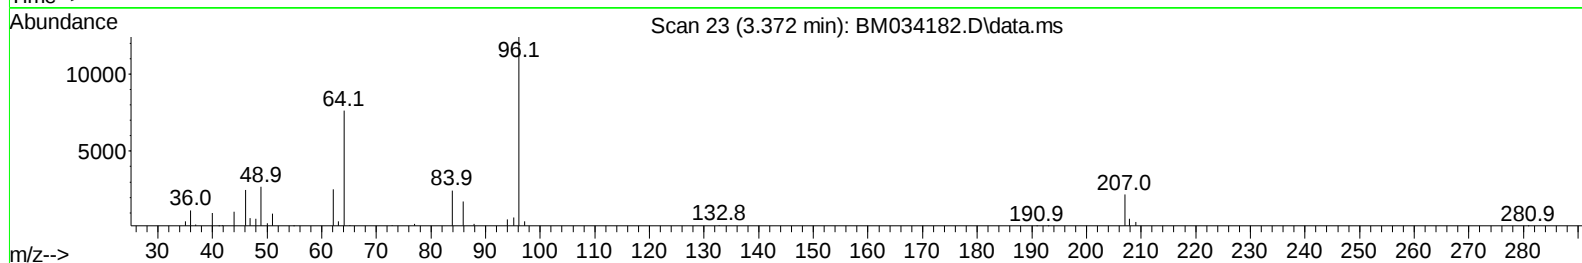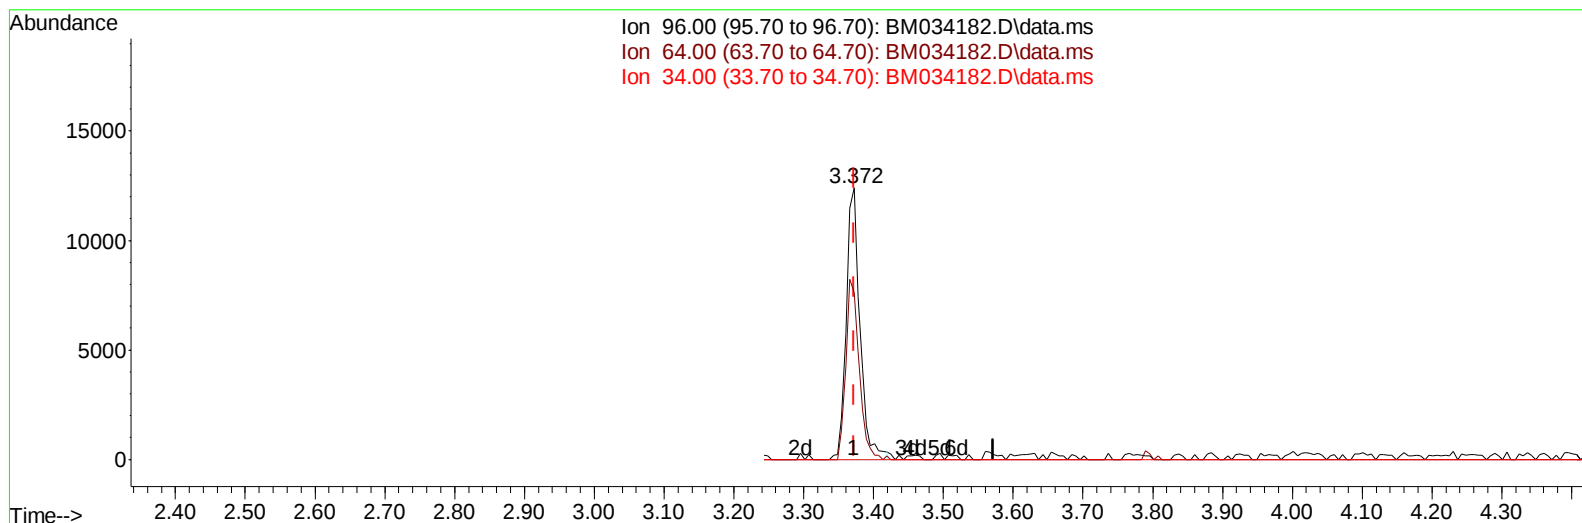

TIC: BM034182.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.372min (+ 0.000) 5.95 ng/uL m

response 16770

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	61.46
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034182.D
 Acq On : 09 Mar 2022 12:44
 Operator : CG/JU
 Sample : N1775-12
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRU6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/10/2022
 Supervised By :Yogesh Patel 03/11/2022

Quant Time: Mar 09 23:56:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 08 13:09:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.989	152	129657	20.000	ng/ul	0.00
20) Naphthalene-d8	10.801	136	526475	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.624	164	361117	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.365	188	767420	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.536	240	696846	20.000	ng/ul	# 0.00
88) Perylene-d12	23.977	264	690105	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	16770m	5.949	ng/uL	0.00
4) Pyridine-d5	3.790	84	192904	23.507	ng/ul	0.00
7) Phenol-d5	7.136	99	289476	28.493	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.307	67	170779	31.232	ng/ul	0.00
11) 2-Chlorophenol-d4	7.513	132	260364	30.917	ng/ul	0.00
15) 4-Methylphenol-d8	8.689	113	249684	29.331	ng/ul	0.00
21) Nitrobenzene-d5	9.148	128	127457	31.245	ng/ul	0.00
24) 2-Nitrophenol-d4	9.877	143	138627	31.289	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.419	165	273635	29.949	ng/ul	0.00
31) 4-Chloroaniline-d4	10.930	131	358414	28.712	ng/ul	0.00
46) Dimethylphthalate-d6	14.030	166	887316	32.380	ng/ul	0.00
49) Acenaphthylene-d8	14.318	160	1087365	31.732	ng/ul	0.00
54) 4-Nitrophenol-d4	14.801	143	118342	23.210	ng/ul	0.00
60) Fluorene-d10	15.612	176	776893	31.855	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.718	200	111873	22.590	ng/ul	0.00
73) Anthracene-d10	17.465	188	1216468	32.179	ng/ul	0.00
81) Pyrene-d10	19.747	212	1385736	36.178	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.824	264	1198089	32.727	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034182.D
Acq On : 09 Mar 2022 12:44
Operator : CG/JU
Sample : N1775-12
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRU6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/10/2022
Supervised By :Yogesh Patel 03/11/2022

Quant Time: Mar 09 23:56:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 08 13:09:16 2022
Response via : Initial Calibration

