




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034190.D
 Acq On : 09 Mar 2022 17:34
 Operator : CG/JU
 Sample : N1775-23
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSC6

Manual IntegrationsAPPROVED

Quant Time: Mar 10 00:00:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 08 13:09:16 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/10/2022
 Supervised By :Yogesh Patel 03/11/2022

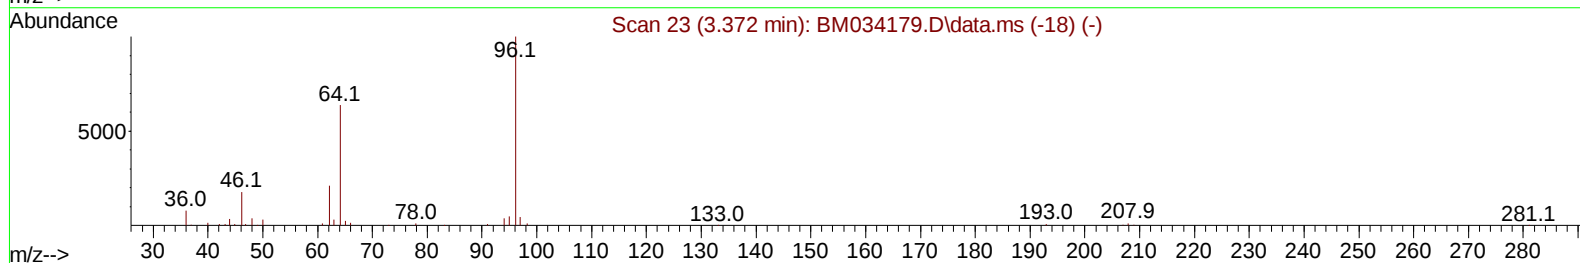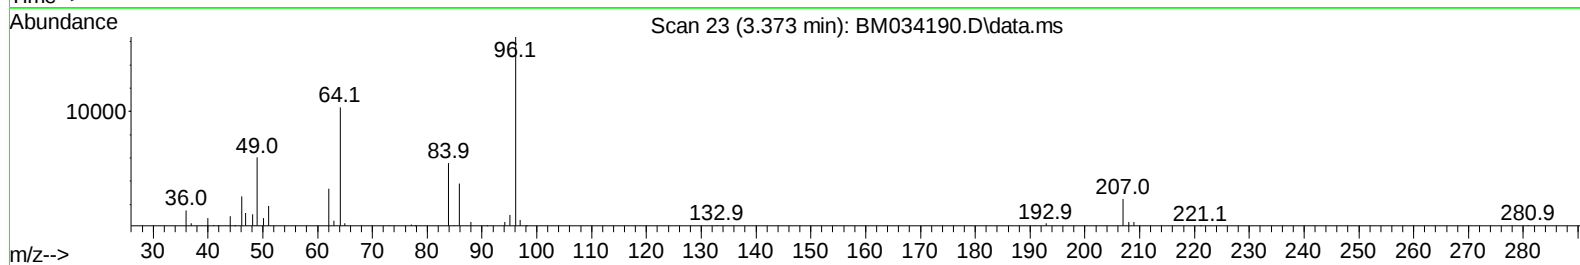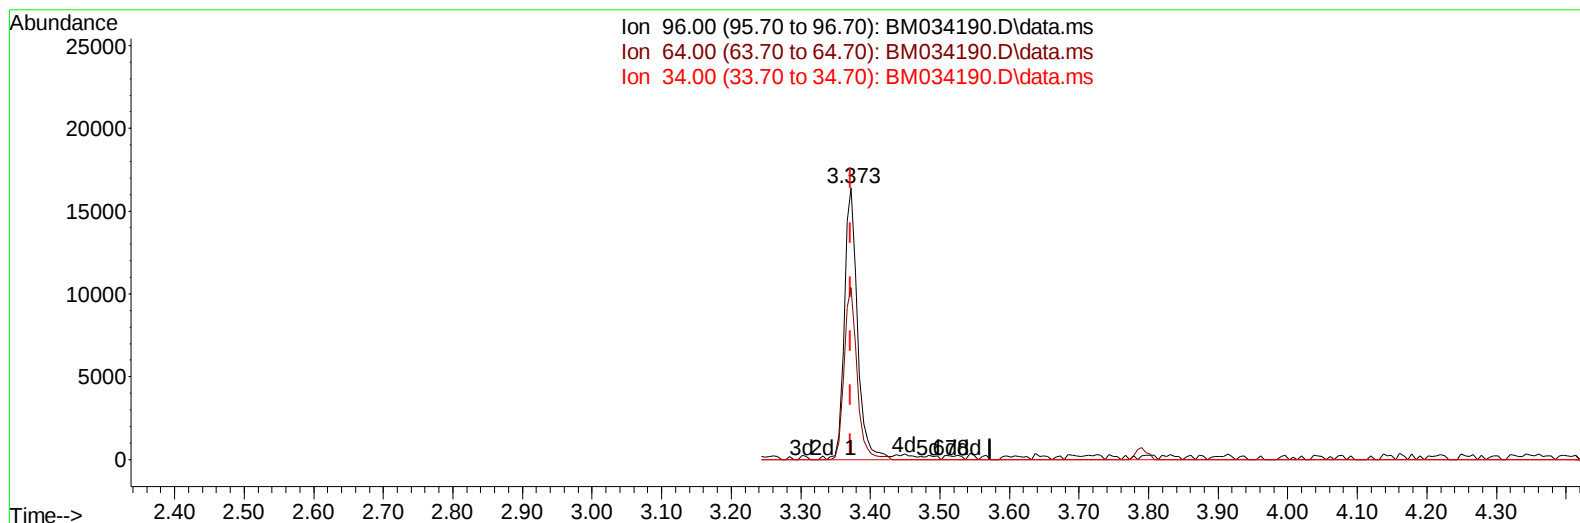

TIC: BM034190.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.373min (+ 0.001) 6.06 ng/uL

response 21427

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	63.24
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034190.D
 Acq On : 09 Mar 2022 17:34
 Operator : CG/JU
 Sample : N1775-23
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSC6

Manual IntegrationsAPPROVED

Quant Time: Mar 10 00:00:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 08 13:09:16 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/10/2022
 Supervised By :Yogesh Patel 03/11/2022

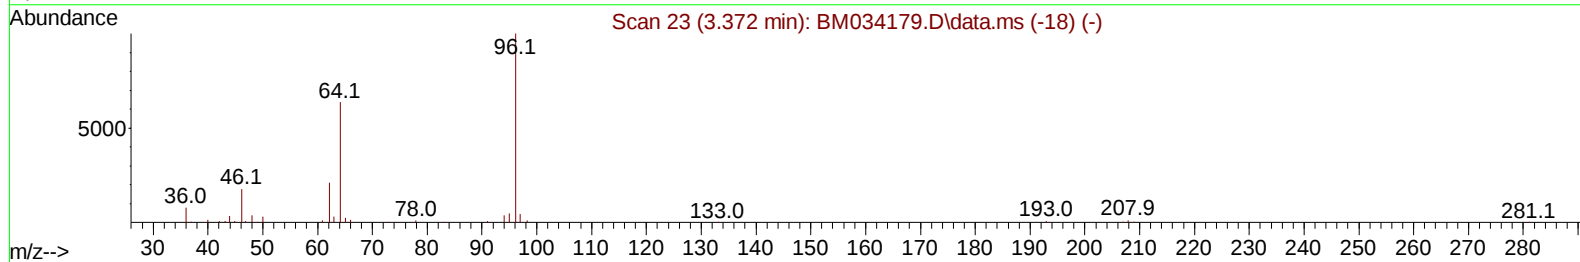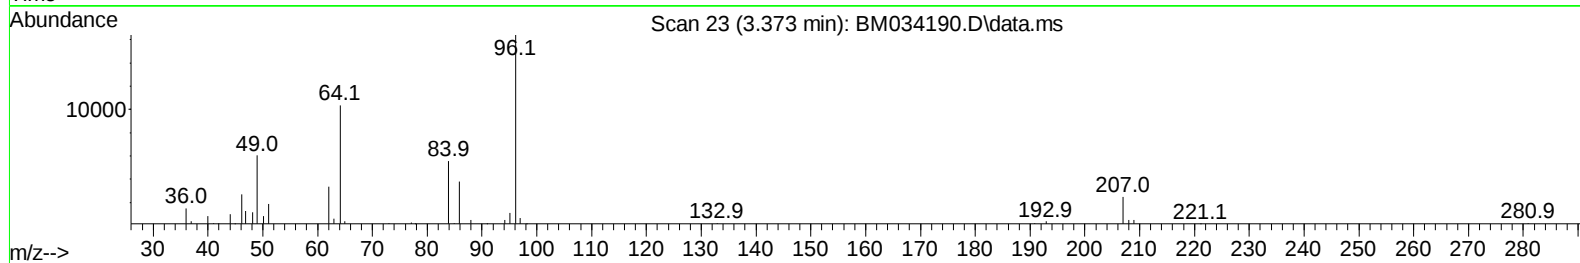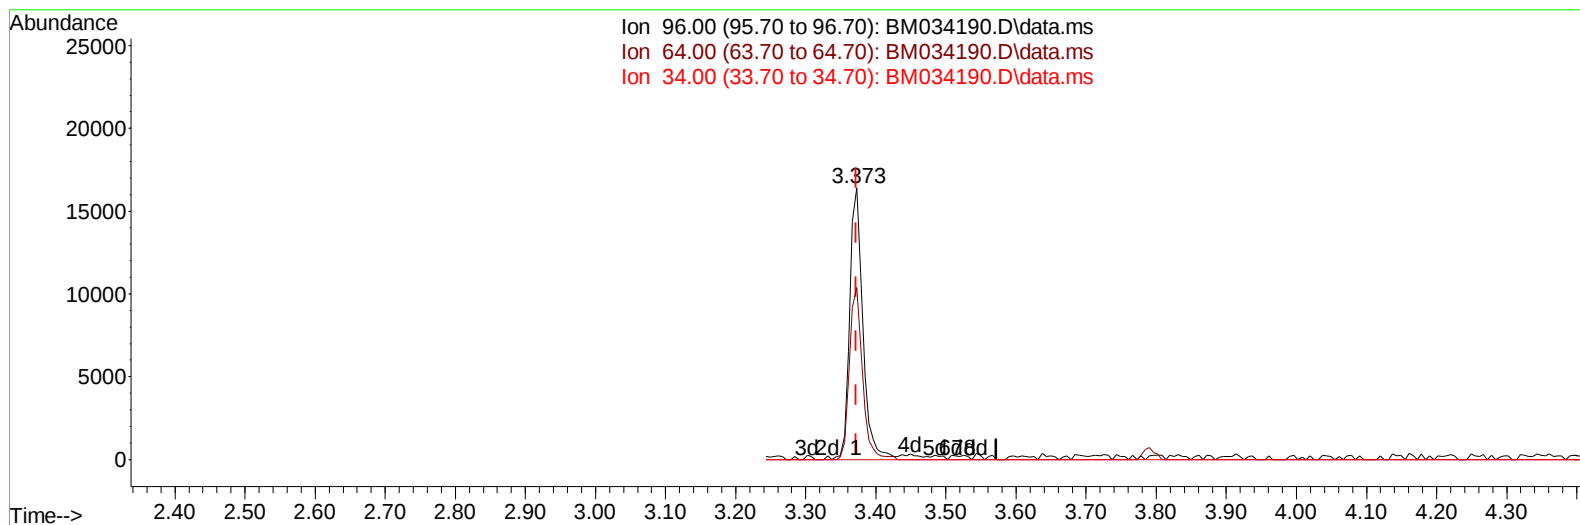

TIC: BM034190.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.373min (+ 0.001) 5.97 ng/uL m

response 21100

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	63.24
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034190.D
 Acq On : 09 Mar 2022 17:34
 Operator : CG/JU
 Sample : N1775-23
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSC6

Manual IntegrationsAPPROVED

Quant Time: Mar 10 00:00:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 08 13:09:16 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/10/2022
 Supervised By :Yogesh Patel 03/11/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.990	152		162589	20.000	ng/ul	0.00
20) Naphthalene-d8	10.802	136		606868	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.625	164		388017	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.366	188		800795	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.536	240		835726	20.000	ng/ul	# 0.00
88) Perylene-d12	23.983	264		940833	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.373	96		21100m	5.969	ng/uL	0.00
4) Pyridine-d5	3.790	84		269613	26.200	ng/ul	0.00
7) Phenol-d5	7.137	99		358766	28.161	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.308	67		204653	29.846	ng/ul	0.00
11) 2-Chlorophenol-d4	7.513	132		318149	30.126	ng/ul	0.00
15) 4-Methylphenol-d8	8.690	113		304384	28.514	ng/ul	0.00
21) Nitrobenzene-d5	9.149	128		155513	33.073	ng/ul	0.00
24) 2-Nitrophenol-d4	9.878	143		176217	34.505	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.413	165		330794	31.409	ng/ul	0.00
31) 4-Chloroaniline-d4	10.931	131		429119	29.822	ng/ul	0.00
46) Dimethylphthalate-d6	14.031	166		1006347	34.178	ng/ul	0.00
49) Acenaphthylene-d8	14.319	160		1254452	34.070	ng/ul	0.00
54) 4-Nitrophenol-d4	14.801	143		128987	23.544	ng/ul	0.00
60) Fluorene-d10	15.613	176		876693	33.455	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.719	200		120459	23.309	ng/ul	0.00
73) Anthracene-d10	17.466	188		1391201	35.268	ng/ul	0.00
81) Pyrene-d10	19.748	212		1612211	35.096	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.824	264		1742206	34.908	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034190.D
Acq On : 09 Mar 2022 17:34
Operator : CG/JU
Sample : N1775-23
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSC6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/10/2022
Supervised By :Yogesh Patel 03/11/2022

Quant Time: Mar 10 00:00:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 08 13:09:16 2022
Response via : Initial Calibration

