

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034157.D
 Acq On : 08 Mar 2022 20:28
 Operator : CG/JU
 Sample : N1733-25
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRU3

Quant Time: Mar 09 00:41:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 08 13:09:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.995	152	134083	20.000	ng/ul	0.00
20) Naphthalene-d8	10.807	136	525669	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.630	164	354204	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.365	188	718270	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.542	240	627613	20.000	ng/ul	# 0.00
88) Perylene-d12	23.989	264	639198	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	23181	7.952	ng/uL	0.00
4) Pyridine-d5	3.790	84	271796	32.027	ng/ul	0.00
7) Phenol-d5	7.143	99	392170	37.328	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.313	67	221111	39.101	ng/ul	0.00
11) 2-Chlorophenol-d4	7.519	132	348763	40.047	ng/ul	0.00
15) 4-Methylphenol-d8	8.695	113	331665	37.676	ng/ul	0.00
21) Nitrobenzene-d5	9.154	128	168962	41.484	ng/ul	0.00
24) 2-Nitrophenol-d4	9.884	143	193602	43.765	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.419	165	357381	39.175	ng/ul	0.00
31) 4-Chloroaniline-d4	10.937	131	458099	36.753	ng/ul	0.00
46) Dimethylphthalate-d6	14.036	166	1124804	41.848	ng/ul	0.00
49) Acenaphthylene-d8	14.325	160	1380065	41.060	ng/ul	0.00
54) 4-Nitrophenol-d4	14.801	143	166029	33.198	ng/ul	0.00
60) Fluorene-d10	15.619	176	973714	40.705	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.724	200	157592	33.999	ng/ul	0.00
73) Anthracene-d10	17.465	188	1489517	42.098	ng/ul	0.00
81) Pyrene-d10	19.754	212	1638349	47.491	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.830	264	1435109	42.324	ng/ul	0.00


Target Compounds					Qvalue	
8) Phenol	7.166	94	10801	1.016	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034157.D
Acq On : 08 Mar 2022 20:28
Operator : CG/JU
Sample : N1733-25
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRU3

Quant Time: Mar 09 00:41:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 08 13:09:16 2022
Response via : Initial Calibration

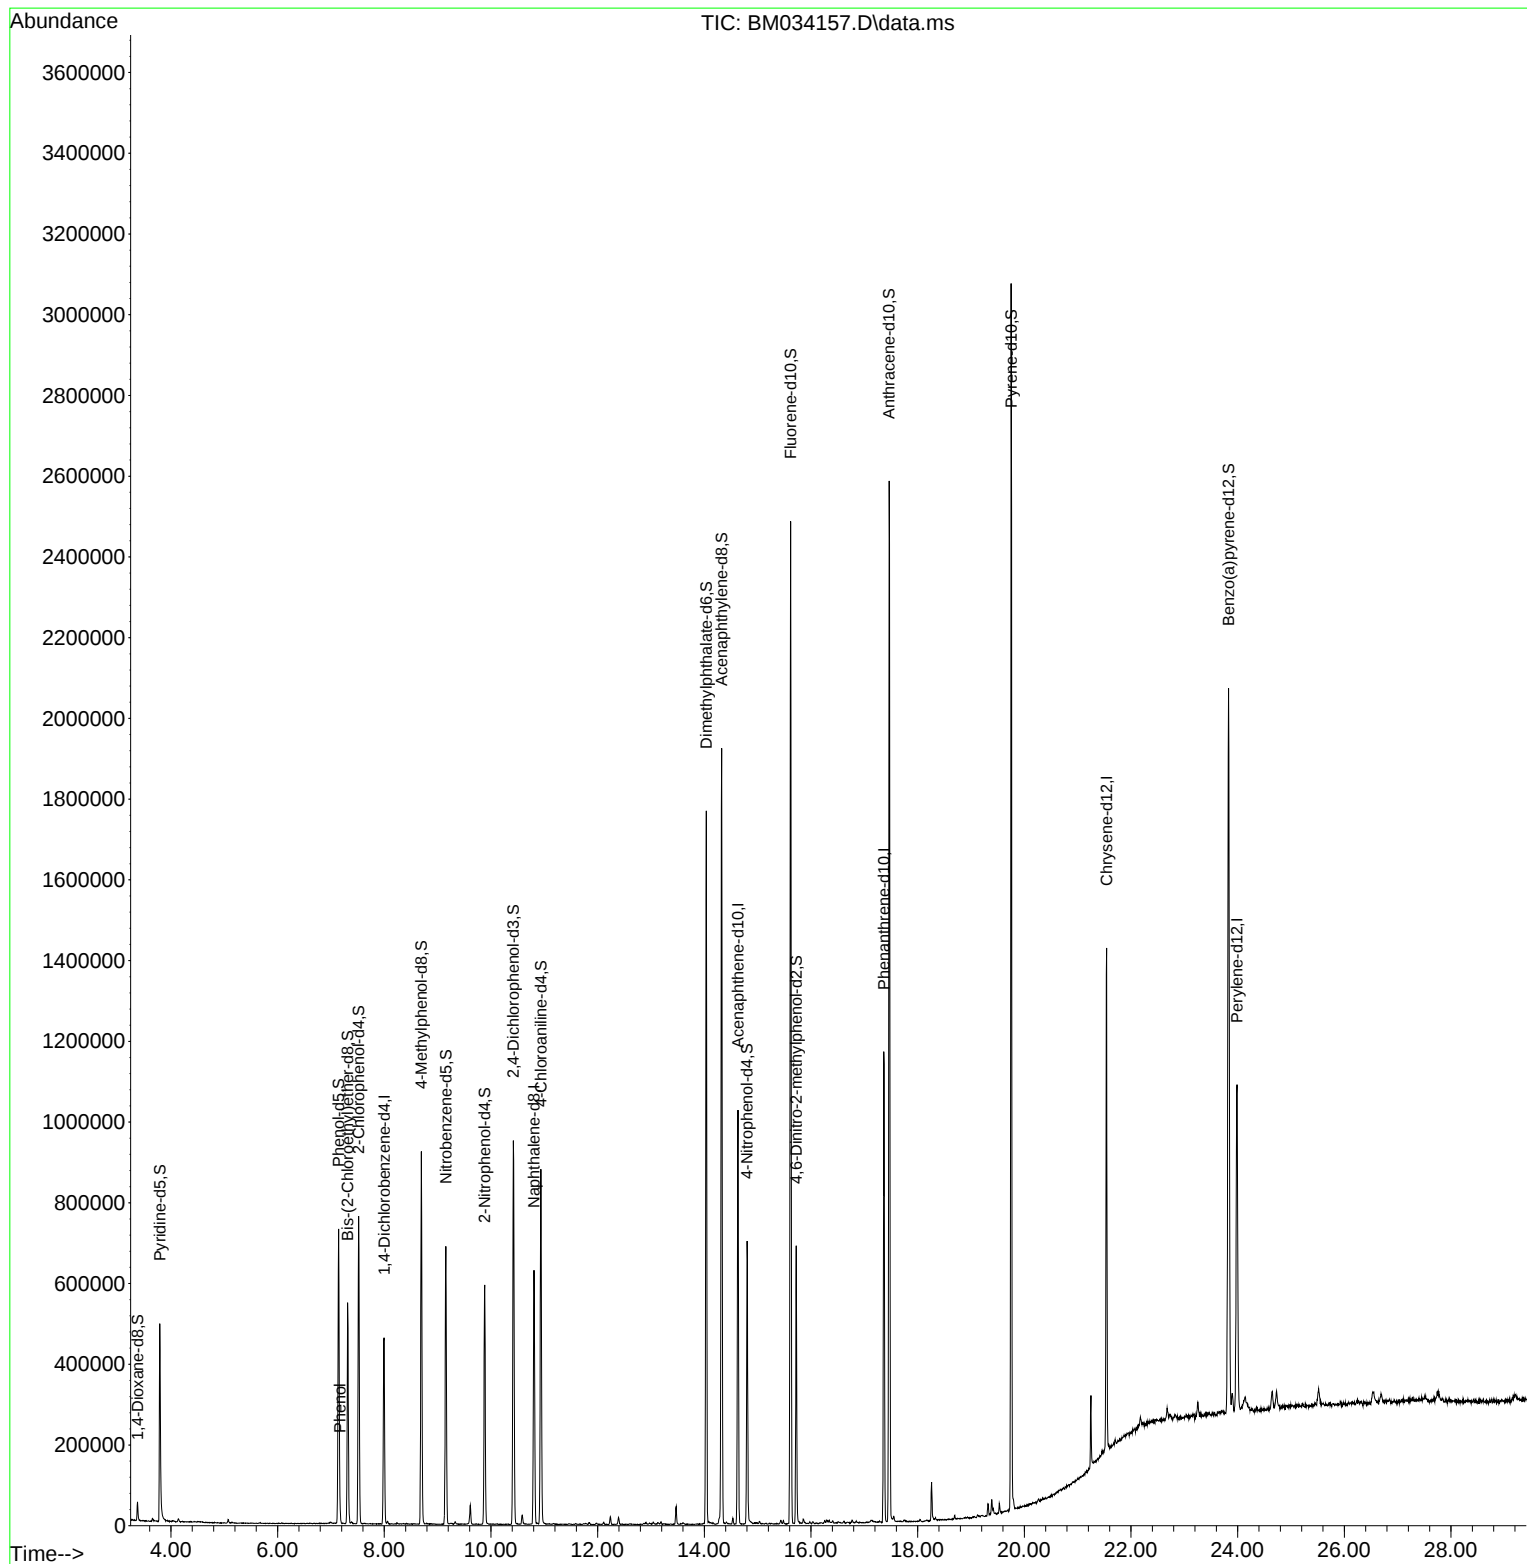

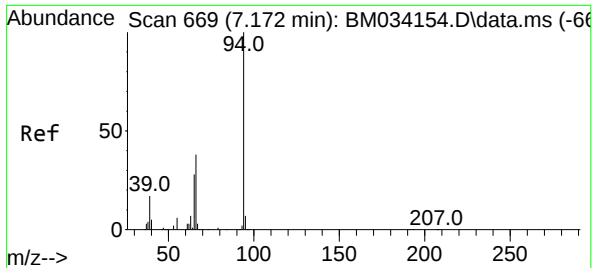

#8
Phenol
Concen: 1.016 ng/ul
RT: 7.166 min Scan# 60
Delta R.T. 0.000 min
Lab File: BM034157.D
Acq: 08 Mar 2022 20:28

Instrument :
BNA_M
ClientSampleId :
DBRU3

Tgt Ion: 94 Resp: 10801
Ion Ratio Lower Upper
94 100
65 31.0 31.7 47.5#
66 48.7 45.4 68.0

