

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034166.D
 Acq On : 09 Mar 2022 01:55
 Operator : CG/JU
 Sample : N1733-20
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRT8

Quant Time: Mar 09 02:32:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 08 13:09:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.989	152	126413	20.000	ng/ul	0.00
20) Naphthalene-d8	10.807	136	478247	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.624	164	294447	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.365	188	571997	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.536	240	573015	20.000	ng/ul	# 0.00
88) Perylene-d12	23.982	264	645427	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	22654	8.242	ng/uL	0.00
4) Pyridine-d5	3.790	84	299283	37.406	ng/ul	0.00
7) Phenol-d5	7.142	99	386622	39.032	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.313	67	216618	40.631	ng/ul	0.00
11) 2-Chlorophenol-d4	7.519	132	347998	42.383	ng/ul	0.00
15) 4-Methylphenol-d8	8.695	113	320293	38.591	ng/ul	0.00
21) Nitrobenzene-d5	9.154	128	162857	43.950	ng/ul	0.00
24) 2-Nitrophenol-d4	9.878	143	183958	45.708	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.419	165	341640	41.163	ng/ul	0.00
31) 4-Chloroaniline-d4	10.930	131	429195	37.849	ng/ul	0.00
46) Dimethylphthalate-d6	14.030	166	941655	42.144	ng/ul	0.00
49) Acenaphthylene-d8	14.318	160	1200997	42.984	ng/ul	0.00
54) 4-Nitrophenol-d4	14.801	143	127204	30.596	ng/ul	0.00
60) Fluorene-d10	15.618	176	822559	41.364	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.724	200	115301	31.236	ng/ul	0.00
73) Anthracene-d10	17.465	188	1222811	43.398	ng/ul	0.00
81) Pyrene-d10	19.753	212	1370044	43.497	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.824	264	1496584	43.711	ng/ul	0.00


Target Compounds					Qvalue	
8) Phenol	7.166	94	10168	1.015	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034166.D
Acq On : 09 Mar 2022 01:55
Operator : CG/JU
Sample : N1733-20
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRT8

Quant Time: Mar 09 02:32:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 08 13:09:16 2022
Response via : Initial Calibration

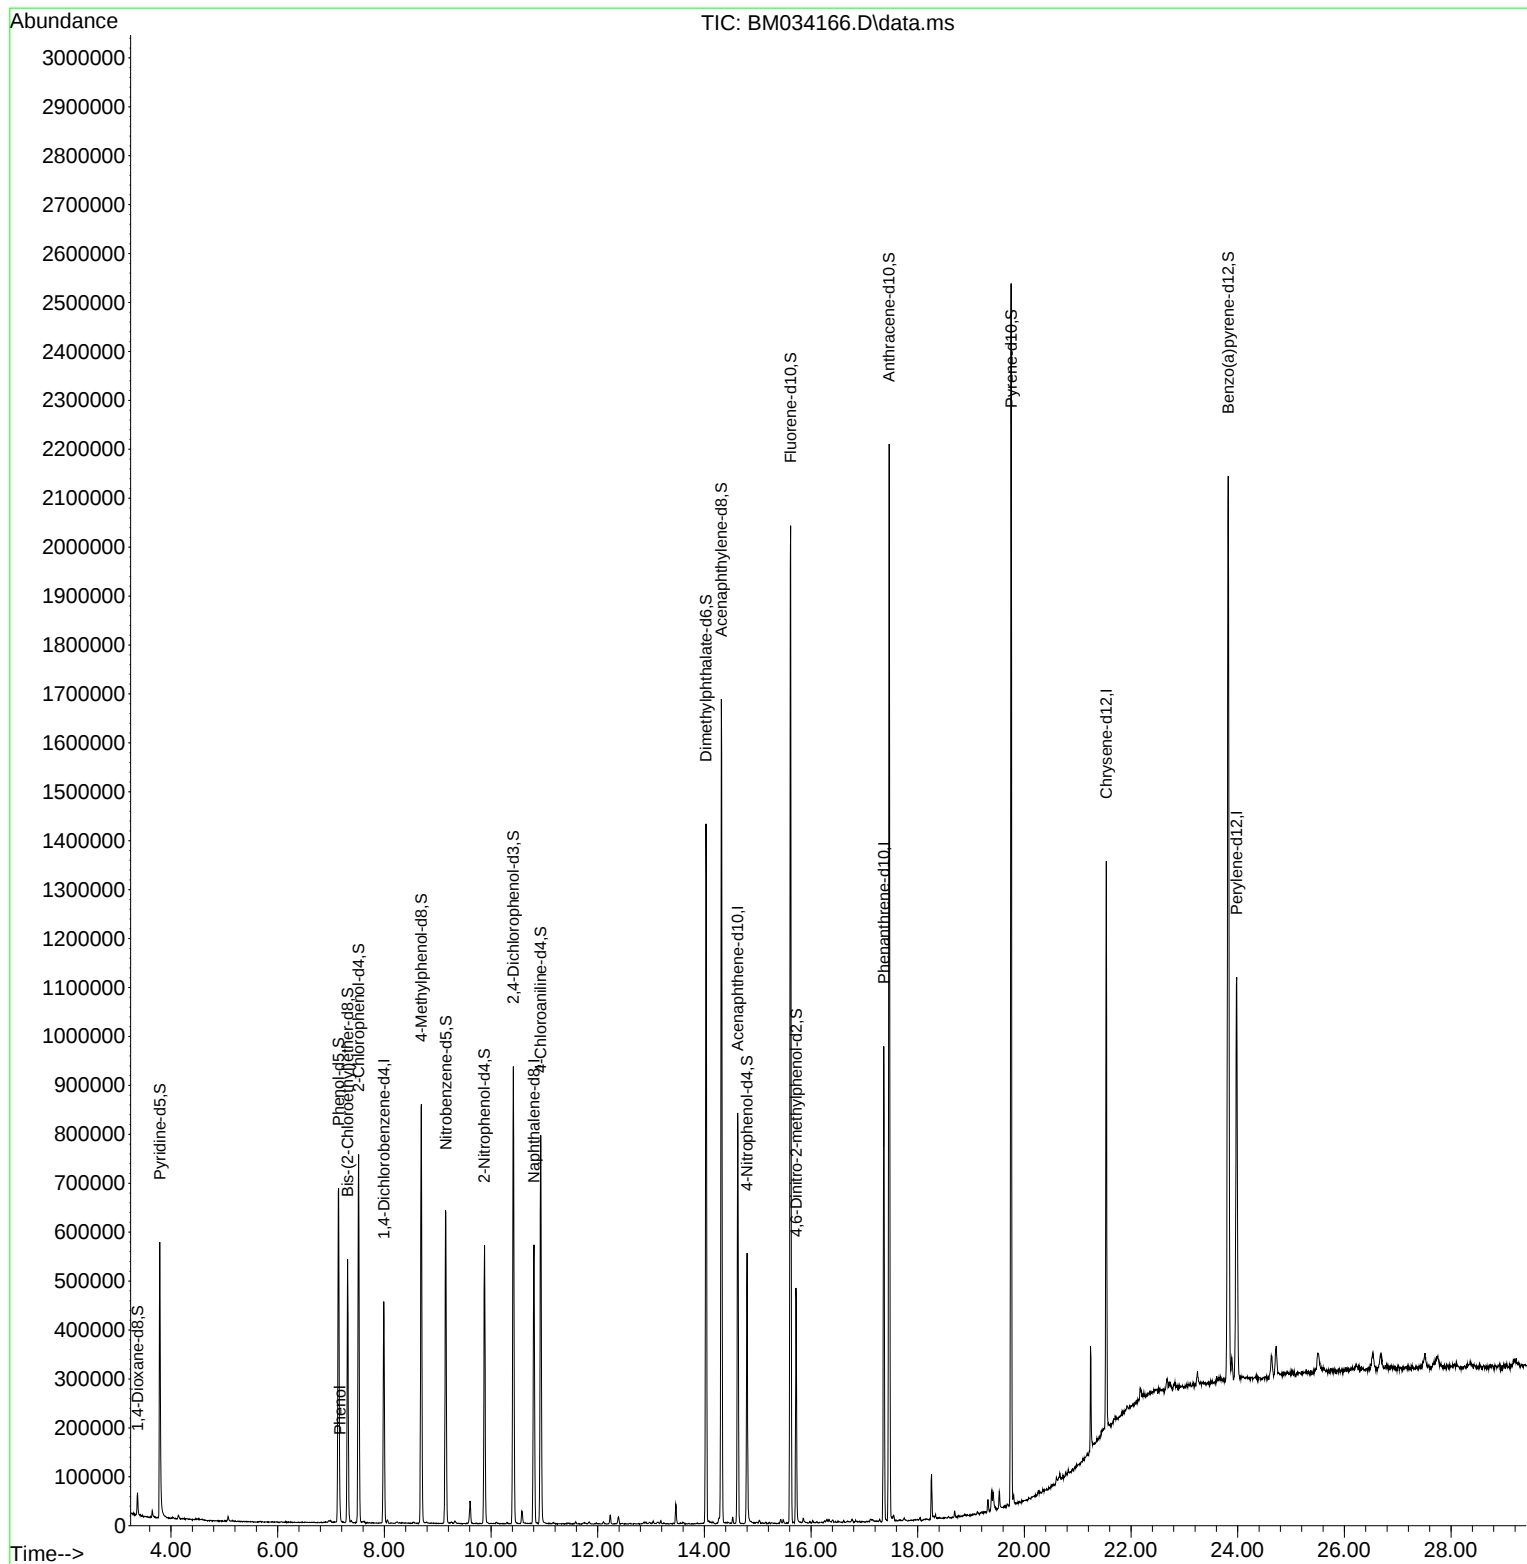

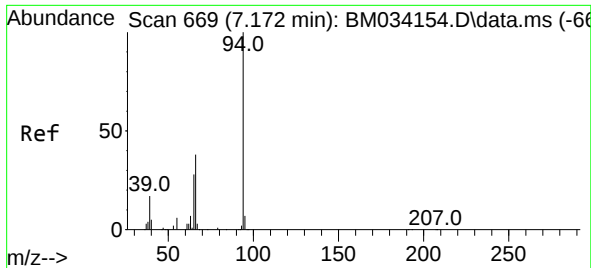

#8
Phenol
Concen: 1.015 ng/ul
RT: 7.166 min Scan# 66
Delta R.T. -0.000 min
Lab File: BM034166.D
Acq: 09 Mar 2022 01:55

Instrument :
BNA_M
ClientSampleId :
DBRT8

Tgt Ion: 94 Resp: 10168
Ion Ratio Lower Upper
94 100
65 28.3 31.7 47.5#
66 56.1 45.4 68.0

