

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034152.D
 Acq On : 08 Mar 2022 16:48
 Operator : CG/JU
 Sample : N1733-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034152.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	19	23	32	rVB	46777	62524	1.28%	0.129%
2	3.661	69	72	75	rBV3	4675	6292	0.13%	0.013%
3	3.790	90	94	108	rBV	565061	819206	16.75%	1.696%
4	4.137	149	153	159	rVB	10091	15340	0.31%	0.032%
5	5.072	308	312	318	rBV5	8799	13837	0.28%	0.029%
6	7.143	657	664	676	rVB	803424	1223335	25.01%	2.532%
7	7.313	685	693	703	rBV	599392	938987	19.20%	1.944%
8	7.519	721	728	737	rBV	827662	1276749	26.10%	2.643%
9	7.996	802	809	815	rBV	546720	873436	17.86%	1.808%
10	8.060	815	820	826	rVB4	7995	12952	0.26%	0.027%
11	8.237	845	850	853	rBV5	3124	4905	0.10%	0.010%
12	8.695	921	928	942	rBV	1035875	1605330	32.82%	3.323%
13	9.154	999	1006	1016	rVB	774051	1241615	25.39%	2.570%
14	9.331	1032	1036	1044	rVB7	5059	10082	0.21%	0.021%
15	9.613	1073	1084	1090	rVB	50858	83471	1.71%	0.173%
16	9.884	1120	1130	1141	rBV	648714	1066384	21.80%	2.207%
17	10.425	1213	1222	1230	rBV	1039595	1730767	35.39%	3.582%
18	10.584	1244	1249	1257	rBV	36998	61286	1.25%	0.127%
19	10.807	1280	1287	1295	rBV	746298	1243917	25.43%	2.575%
20	10.936	1300	1309	1326	rVV	998528	1673036	34.21%	3.463%
21	11.589	1416	1420	1424	rBV5	3884	6760	0.14%	0.014%
22	11.842	1460	1463	1468	rVB5	4812	8442	0.17%	0.017%
23	11.978	1482	1486	1490	rVB6	4786	6293	0.13%	0.013%
24	12.113	1503	1509	1514	rVB4	4836	7297	0.15%	0.015%
25	12.236	1525	1530	1536	rVB2	21761	31465	0.64%	0.065%
26	12.395	1548	1557	1563	rBV	17944	32152	0.66%	0.067%
27	12.878	1632	1639	1641	rBV7	3832	8360	0.17%	0.017%
28	12.907	1641	1644	1652	rVB6	4565	7675	0.16%	0.016%
29	13.042	1664	1667	1673	rBV3	6171	8273	0.17%	0.017%
30	13.130	1678	1682	1688	rVV7	4893	8315	0.17%	0.017%
31	13.189	1688	1692	1697	rVB3	6650	8486	0.17%	0.018%
32	13.472	1734	1740	1749	rBV2	47508	65858	1.35%	0.136%
33	13.601	1758	1762	1766	rVB6	4876	6313	0.13%	0.013%
34	14.036	1829	1836	1842	rBV	1959459	2678916	54.77%	5.545%
35	14.083	1842	1844	1849	rVV4	7759	11869	0.24%	0.025%
36	14.125	1849	1851	1854	rVV3	5099	5672	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034152.D
 Acq On : 08 Mar 2022 16:48
 Operator : CG/JU
 Sample : N1733-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

37	14.160	1854	1857	1865	rVB4	6243	11091	0.23%	0.023%
38	14.283	1873	1878	1879	rBV2	18278	25394	0.52%	0.053%
39	14.325	1879	1885	1896	rVV	2293983	3227540	65.99%	6.681%
40	14.419	1896	1901	1906	rVB6	4061	8828	0.18%	0.018%
41	14.536	1917	1921	1926	rBV2	14858	20441	0.42%	0.042%
42	14.630	1929	1937	1947	rVV	1232941	1787343	36.54%	3.700%
43	14.801	1959	1966	1976	rBV	728490	1062160	21.72%	2.199%
44	14.989	1994	1998	2002	rVV7	2922	5073	0.10%	0.011%
45	15.030	2003	2005	2011	rVB6	6459	8932	0.18%	0.018%
46	15.436	2069	2074	2078	rBV2	16400	23968	0.49%	0.050%
47	15.483	2078	2082	2086	rVB2	8604	10882	0.22%	0.023%
48	15.619	2099	2105	2112	rBV	2875595	3996465	81.71%	8.272%
49	15.724	2117	2123	2135	rBV	735944	1005531	20.56%	2.081%
50	15.860	2141	2146	2154	rVB5	14697	26466	0.54%	0.055%
51	15.983	2163	2167	2171	rVB5	4615	5557	0.11%	0.012%
52	16.036	2173	2176	2183	rBV6	6442	9898	0.20%	0.020%
53	16.189	2195	2202	2204	rBV5	3525	7391	0.15%	0.015%
54	16.260	2210	2214	2217	rBV4	7027	8861	0.18%	0.018%
55	16.301	2218	2221	2225	rVV5	9332	15525	0.32%	0.032%
56	16.342	2225	2228	2232	rVV6	6170	10412	0.21%	0.022%
57	16.413	2236	2240	2243	rVB5	7904	11842	0.24%	0.025%
58	16.518	2252	2258	2262	rBV6	4412	8857	0.18%	0.018%
59	16.618	2272	2275	2281	rVB7	4947	7229	0.15%	0.015%
60	16.689	2281	2287	2291	rBV9	3603	7897	0.16%	0.016%
61	16.771	2298	2301	2305	rVB5	8232	10615	0.22%	0.022%
62	16.848	2310	2314	2316	rVB5	5060	6029	0.12%	0.012%
63	17.124	2357	2361	2363	rBV3	5433	8126	0.17%	0.017%
64	17.295	2384	2390	2394	rVB7	6930	10941	0.22%	0.023%
65	17.371	2394	2403	2409	rBV	1539855	2119066	43.33%	4.386%
66	17.471	2413	2420	2431	rVV	2978814	4269025	87.28%	8.836%
67	17.554	2431	2434	2438	rVB5	11685	15568	0.32%	0.032%
68	17.748	2463	2467	2469	rBV4	6101	9010	0.18%	0.019%
69	18.042	2515	2517	2522	rVB5	7165	10785	0.22%	0.022%
70	18.265	2549	2555	2562	rBV2	67923	103152	2.11%	0.214%
71	18.336	2565	2567	2573	rVB2	8110	11285	0.23%	0.023%
72	18.695	2625	2628	2632	rBV6	7758	10197	0.21%	0.021%
73	19.324	2731	2735	2739	rBV3	36166	49451	1.01%	0.102%
74	19.395	2743	2747	2750	rVV	38447	44168	0.90%	0.091%
75	19.536	2768	2771	2778	rBV8	20421	31745	0.65%	0.066%
76	19.759	2802	2809	2819	rBV	3655949	4891044	100.00%	10.124%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034152.D
Acq On : 08 Mar 2022 16:48
Operator : CG/JU
Sample : N1733-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRR8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Title : SVOA CALIBRATION

77	21.253	3059	3063	3067	rBV2	108942	129267	2.64%	0.268%
78	21.542	3107	3112	3124	rBV	1592303	2178241	44.54%	4.509%
79	23.836	3495	3502	3510	rBV2	2131532	4172094	85.30%	8.636%
80	23.994	3522	3529	3540	rVB2	985862	2052907	41.97%	4.249%




Sum of corrected areas: 48311896

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034152.D
Acq On : 08 Mar 2022 16:48
Operator : CG/JU
Sample : N1733-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRR8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

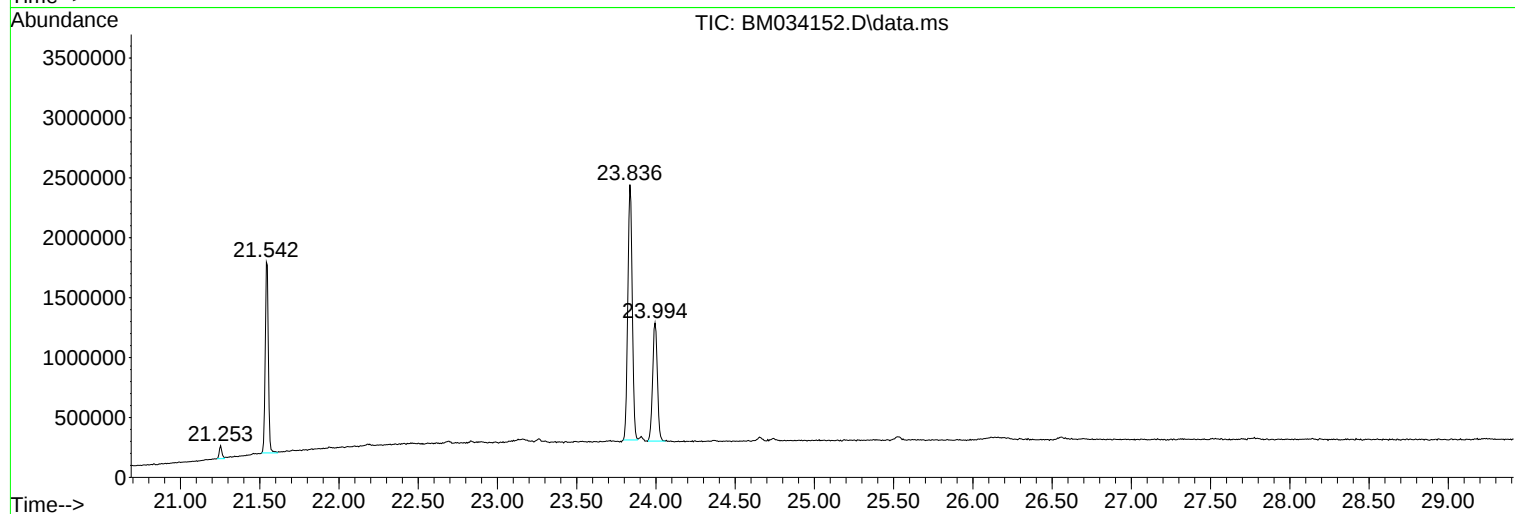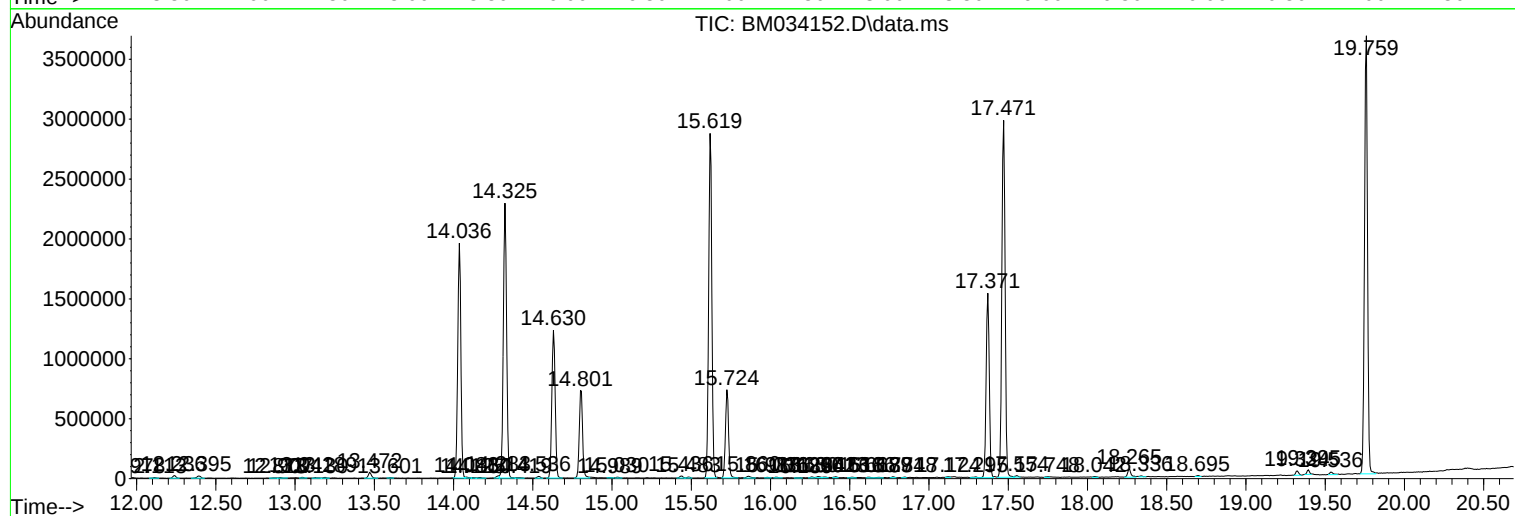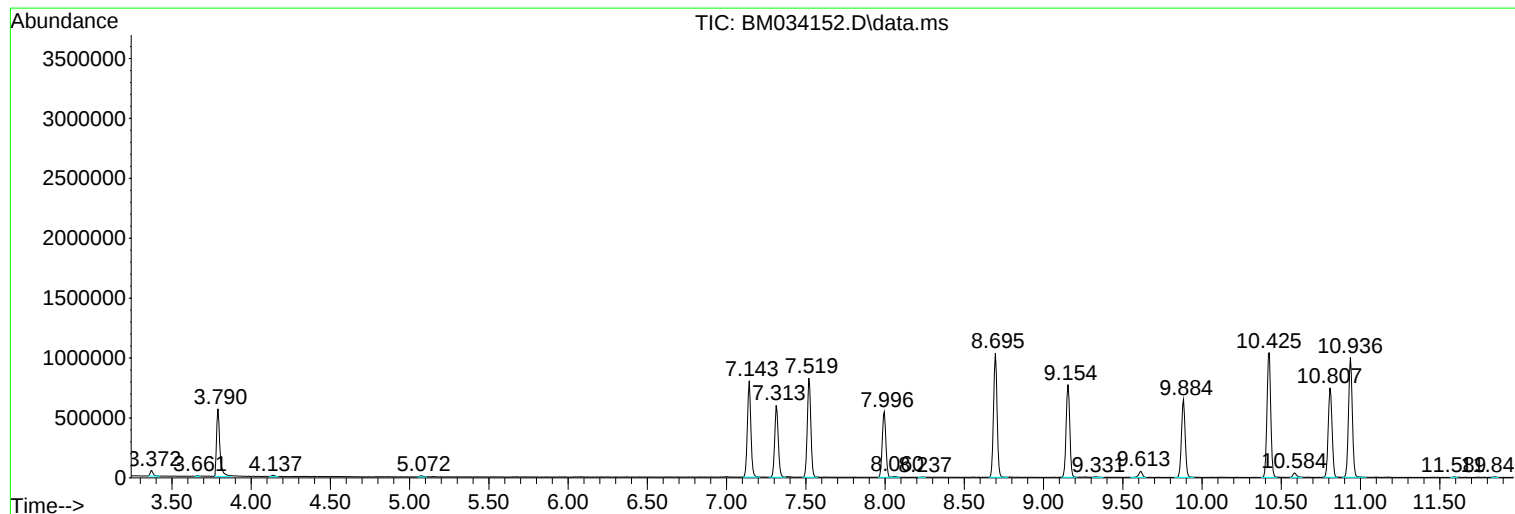

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034152.D
Acq On : 08 Mar 2022 16:48
Operator : CG/JU
Sample : N1733-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRR8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034152.D
Acq On : 08 Mar 2022 16:48
Operator : CG/JU
Sample : N1733-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRR8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------