

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034155.D
 Acq On : 08 Mar 2022 19:15
 Operator : CG/JU
 Sample : PB143121BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK121

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	19	23	29	rVB	34680	43521	1.31%	0.127%
2	3.790	90	94	118	rBV	422989	633967	19.06%	1.845%
3	4.137	150	153	158	rVB	8265	12295	0.37%	0.036%
4	4.366	188	192	196	rVB7	2296	3887	0.12%	0.011%
5	7.142	657	664	673	rVB	556904	843685	25.36%	2.455%
6	7.313	687	693	703	rVB	424000	656429	19.74%	1.910%
7	7.519	722	728	739	rBV	586989	909865	27.35%	2.647%
8	7.995	802	809	817	rVB	504370	787172	23.67%	2.290%
9	8.695	921	928	938	rBV	690151	1101905	33.13%	3.206%
10	9.154	998	1006	1016	rBV	533247	861959	25.91%	2.508%
11	9.883	1122	1130	1138	rBV	438752	733464	22.05%	2.134%
12	10.419	1214	1221	1235	rBV	726512	1200509	36.09%	3.493%
13	10.807	1280	1287	1296	rVB	664656	1097960	33.01%	3.195%
14	10.936	1300	1309	1318	rVV	690601	1162249	34.94%	3.382%
15	12.389	1552	1556	1561	rBV2	11154	18044	0.54%	0.052%
16	13.601	1758	1762	1768	rBV5	2495	4245	0.13%	0.012%
17	14.036	1828	1836	1842	rBV	1354765	1859264	55.90%	5.410%
18	14.324	1878	1885	1893	rBV	1488783	2154916	64.79%	6.270%
19	14.630	1929	1937	1945	rBV	1086968	1543102	46.39%	4.490%
20	14.801	1958	1966	1983	rBV	573466	825972	24.83%	2.403%
21	15.618	2098	2105	2112	rBV	1945321	2707164	81.39%	7.877%
22	15.724	2117	2123	2135	rVV	548305	730725	21.97%	2.126%
23	15.860	2141	2146	2151	rVB3	7659	12086	0.36%	0.035%
24	17.154	2363	2366	2369	rBV2	4485	5041	0.15%	0.015%
25	17.371	2396	2403	2411	rBV	1273098	1802312	54.19%	5.244%
26	17.465	2413	2419	2429	rBV2	2018262	2897171	87.10%	8.429%
27	18.259	2550	2554	2559	rBV8	5075	9350	0.28%	0.027%
28	19.324	2730	2735	2740	rVB3	24436	36418	1.09%	0.106%
29	19.389	2743	2746	2752	rBV2	23300	34047	1.02%	0.099%
30	19.689	2795	2797	2800	rBV4	5556	5349	0.16%	0.016%
31	19.753	2802	2808	2820	rVV	2507280	3326194	100.00%	9.678%
32	21.542	3107	3112	3119	rVB	1423239	1790553	53.83%	5.210%
33	23.830	3494	3501	3510	rBV2	1450741	2820296	84.79%	8.206%
34	23.988	3521	3528	3538	rVB2	844513	1738596	52.27%	5.059%

Sum of corrected areas: 34369712

Instrument :

BNA_M

ClientSampleId :




SBLK121

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034155.D
Acq On : 08 Mar 2022 19:15
Operator : CG/JU
Sample : PB143121BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

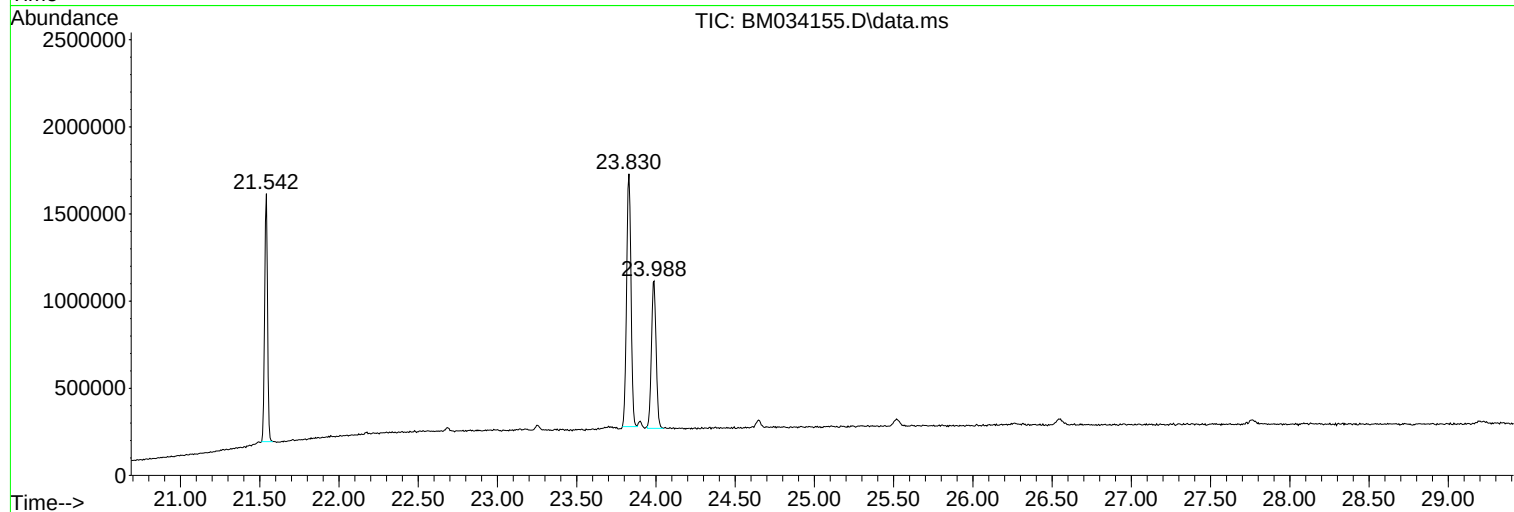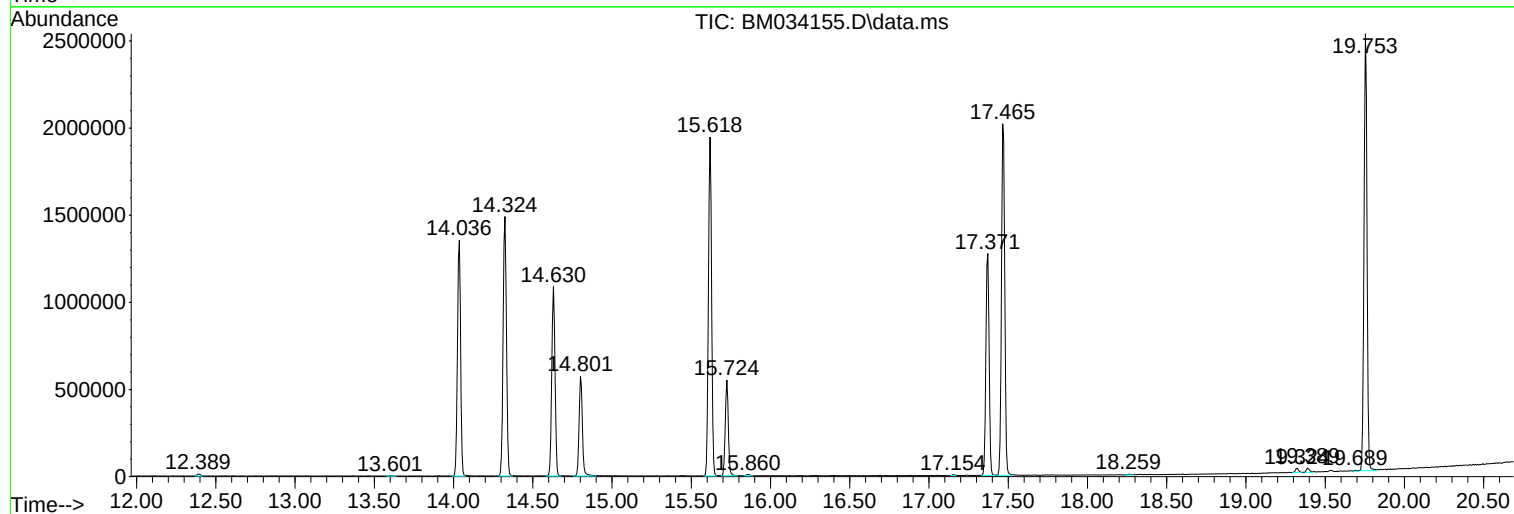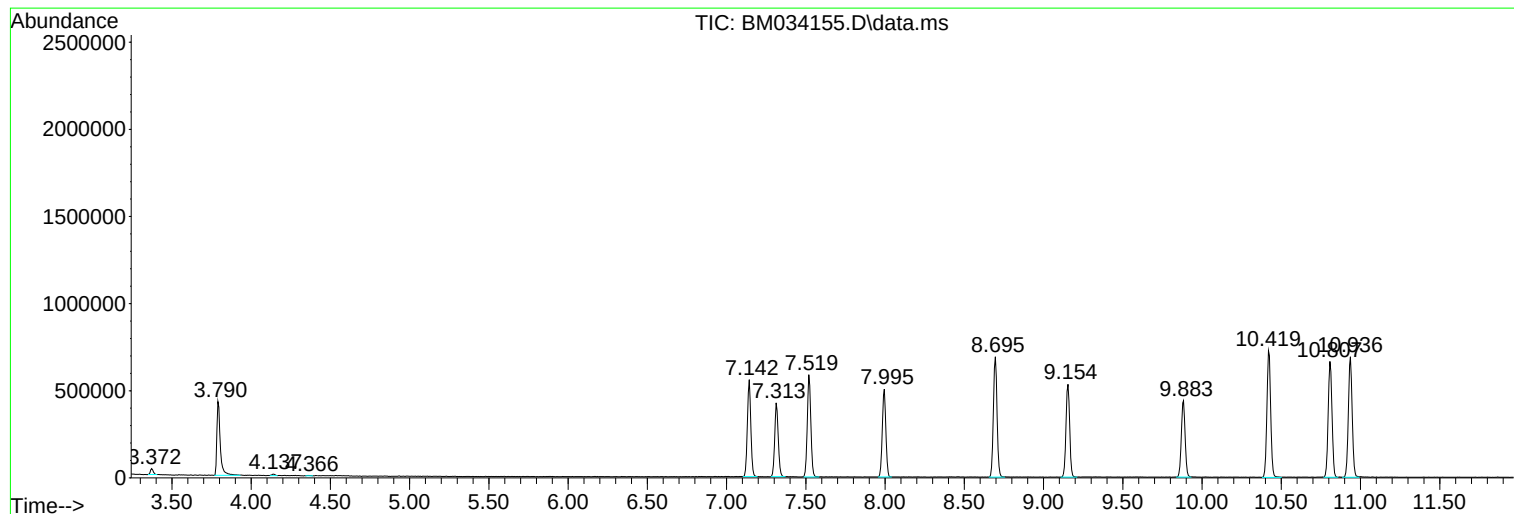

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034155.D
Acq On : 08 Mar 2022 19:15
Operator : CG/JU
Sample : PB143121BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034155.D
Acq On : 08 Mar 2022 19:15
Operator : CG/JU
Sample : PB143121BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------