

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034160.D
 Acq On : 08 Mar 2022 22:18
 Operator : CG/JU
 Sample : N1733-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034160.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	19	23	32	rVB	55202	70381	1.63%	0.156%
2	3.649	68	70	78	rBV2	11244	18883	0.44%	0.042%
3	3.790	90	94	107	rBV	587944	813640	18.83%	1.802%
4	4.137	149	153	158	rBV3	8825	13419	0.31%	0.030%
5	5.072	308	312	318	rBV2	10938	16526	0.38%	0.037%
6	7.142	657	664	674	rBV	846562	1308821	30.29%	2.899%
7	7.313	686	693	702	rBV	636034	978808	22.65%	2.168%
8	7.389	702	706	709	rVB	3990	6003	0.14%	0.013%
9	7.519	720	728	738	rBV	881606	1380630	31.95%	3.058%
10	7.989	802	808	816	rBV	550533	859159	19.88%	1.903%
11	8.054	816	819	827	rVB	8455	14636	0.34%	0.032%
12	8.695	919	928	938	rBV	1060028	1677297	38.82%	3.715%
13	9.154	998	1006	1015	rBV	787538	1288985	29.83%	2.855%
14	9.325	1031	1035	1042	rBV9	5978	10832	0.25%	0.024%
15	9.613	1077	1084	1091	rVB	48722	76338	1.77%	0.169%
16	9.878	1121	1129	1146	rBV	659805	1087315	25.16%	2.409%
17	10.419	1214	1221	1232	rBV	1114635	1797280	41.59%	3.981%
18	10.589	1245	1250	1254	rBV5	9436	15732	0.36%	0.035%
19	10.807	1279	1287	1294	rBV	700069	1160395	26.85%	2.570%
20	10.866	1294	1297	1301	rVB4	2807	4745	0.11%	0.011%
21	10.936	1301	1309	1320	rBV	970751	1672886	38.71%	3.706%
22	11.842	1459	1463	1467	rBV4	4421	7568	0.18%	0.017%
23	12.113	1504	1509	1511	rBV4	3546	4616	0.11%	0.010%
24	12.236	1525	1530	1536	rVB	23015	30899	0.72%	0.068%
25	12.389	1550	1556	1562	rVB	19455	31234	0.72%	0.069%
26	12.907	1640	1644	1647	rVV4	4502	6442	0.15%	0.014%
27	12.971	1651	1655	1659	rBV5	3948	5256	0.12%	0.012%
28	13.042	1662	1667	1672	rBV6	5802	9421	0.22%	0.021%
29	13.130	1677	1682	1685	rVV7	4622	6806	0.16%	0.015%
30	13.183	1688	1691	1699	rVB5	6835	10266	0.24%	0.023%
31	13.466	1735	1739	1747	rVB	45175	61430	1.42%	0.136%
32	13.595	1758	1761	1765	rBV3	3376	5145	0.12%	0.011%
33	14.036	1829	1836	1842	rBV	1747591	2409240	55.76%	5.337%
34	14.077	1842	1843	1848	rVV4	5783	8504	0.20%	0.019%
35	14.124	1848	1851	1854	rVV3	4157	5805	0.13%	0.013%
36	14.160	1854	1857	1863	rVB6	4890	6202	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034160.D
 Acq On : 08 Mar 2022 22:18
 Operator : CG/JU
 Sample : N1733-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

37	14.324	1873	1885	1895	rBV	2074412	3054020	70.68%	6.765%
38	14.536	1916	1921	1927	rVB	16161	22200	0.51%	0.049%
39	14.630	1929	1937	1946	rBV	1036969	1545644	35.77%	3.424%
40	14.801	1960	1966	1977	rBV	707233	989722	22.90%	2.192%
41	15.036	2002	2006	2010	rBV4	8180	11810	0.27%	0.026%
42	15.436	2068	2074	2078	rBV4	4961	8741	0.20%	0.019%
43	15.477	2078	2081	2085	rVB	9489	11934	0.28%	0.026%
44	15.618	2098	2105	2113	rBV	2633409	3634086	84.10%	8.050%
45	15.724	2116	2123	2131	rBV	611035	812961	18.81%	1.801%
46	15.860	2141	2146	2150	rBV3	12561	18330	0.42%	0.041%
47	16.036	2173	2176	2182	rVB6	4625	6604	0.15%	0.015%
48	16.259	2208	2214	2216	rBV7	4698	7811	0.18%	0.017%
49	16.295	2216	2220	2225	rVV7	5610	8996	0.21%	0.020%
50	16.336	2225	2227	2231	rVB4	4866	6329	0.15%	0.014%
51	16.401	2236	2238	2245	rVB5	5026	7147	0.17%	0.016%
52	16.518	2253	2258	2261	rVB6	3622	4928	0.11%	0.011%
53	16.618	2271	2275	2277	rBV3	5045	6057	0.14%	0.013%
54	16.771	2296	2301	2307	rVB6	7203	9653	0.22%	0.021%
55	17.365	2395	2402	2410	rBV	1172431	1691971	39.16%	3.748%
56	17.465	2413	2419	2429	rVV	2636986	3695264	85.52%	8.185%
57	17.548	2430	2433	2439	rVB7	10455	18767	0.43%	0.042%
58	17.748	2463	2467	2473	rBV6	5430	9471	0.22%	0.021%
59	18.042	2514	2517	2523	rVB5	6331	8752	0.20%	0.019%
60	18.259	2550	2554	2560	rBV	78977	106619	2.47%	0.236%
61	18.695	2624	2628	2634	rVB3	29907	33355	0.77%	0.074%
62	19.118	2698	2700	2704	rVB5	4758	5527	0.13%	0.012%
63	19.318	2729	2734	2738	rBV2	30082	45771	1.06%	0.101%
64	19.389	2742	2746	2749	rBV	41360	58269	1.35%	0.129%
65	19.530	2767	2770	2775	rBV4	26575	34290	0.79%	0.076%
66	19.753	2802	2808	2815	rBV	3067621	4048512	93.69%	8.968%
67	21.247	3058	3062	3070	rBV	248555	307763	7.12%	0.682%
68	21.536	3106	3111	3124	rBV	1306243	1773429	41.04%	3.928%
69	23.830	3493	3501	3509	rBV2	2157407	4321097	100.00%	9.572%
70	23.983	3521	3527	3537	rVB2	941748	1937017	44.83%	4.291%




Sum of corrected areas: 45144392

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034160.D
Acq On : 08 Mar 2022 22:18
Operator : CG/JU
Sample : N1733-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRS5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

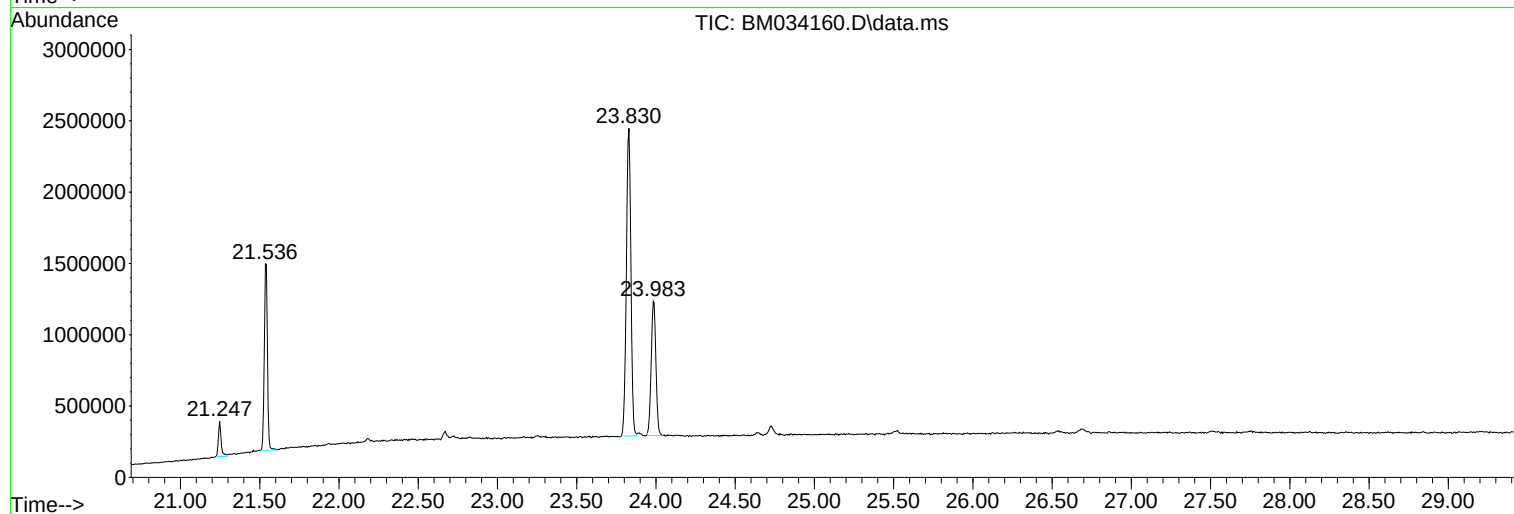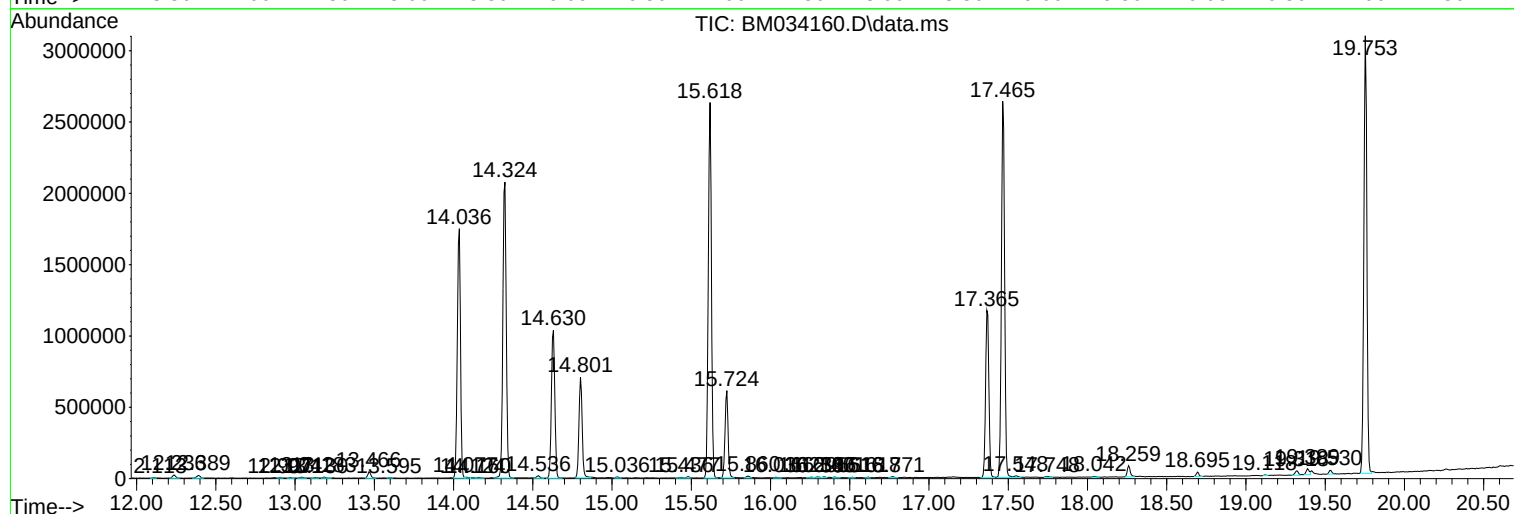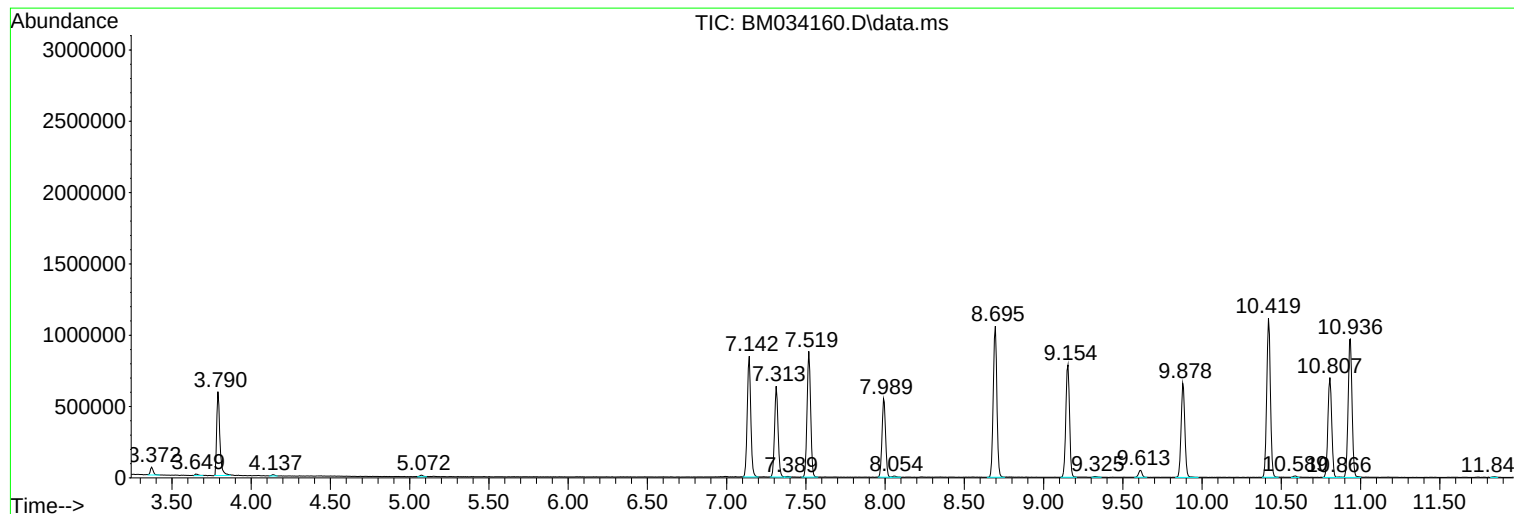

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034160.D
Acq On : 08 Mar 2022 22:18
Operator : CG/JU
Sample : N1733-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRS5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034160.D
Acq On : 08 Mar 2022 22:18
Operator : CG/JU
Sample : N1733-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRS5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc