

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034176.D
 Acq On : 09 Mar 2022 08:30
 Operator : CG/JU
 Sample : PB143058BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.302	7	11	17	rVB	869735	883703	46.94%	9.185%
2	3.425	29	32	35	rBV5	2806	3508	0.19%	0.036%
3	3.649	66	70	76	rVB	27493	33142	1.76%	0.344%
4	3.743	83	86	91	rVB5	3232	3815	0.20%	0.040%
5	4.131	146	152	158	rBV2	10358	14194	0.75%	0.148%
6	4.325	182	185	188	rVB3	2267	2684	0.14%	0.028%
7	4.431	200	203	207	rBV6	2862	4454	0.24%	0.046%
8	4.478	207	211	213	rVV4	3774	4782	0.25%	0.050%
9	4.896	279	282	285	rVB4	1330	1932	0.10%	0.020%
10	5.072	309	312	316	rVB4	2497	3129	0.17%	0.033%
11	6.025	471	474	479	rBV5	1665	1919	0.10%	0.020%
12	6.313	521	523	528	rBV5	1409	2639	0.14%	0.027%
13	6.619	570	575	579	rBV6	2136	4265	0.23%	0.044%
14	6.742	593	596	597	rBV3	2590	2487	0.13%	0.026%
15	6.925	625	627	630	rBV4	2096	2069	0.11%	0.022%
16	7.513	723	727	730	rBV5	1587	2044	0.11%	0.021%
17	7.984	800	807	817	rBV	604385	972859	51.68%	10.112%
18	8.548	900	903	906	rVB3	1715	1912	0.10%	0.020%
19	9.589	1078	1080	1085	rVB4	1411	2175	0.12%	0.023%
20	10.801	1276	1286	1296	rBV	737347	1198700	63.68%	12.459%
21	14.624	1928	1936	1944	rBV	1138906	1588634	84.39%	16.512%
22	14.677	1944	1945	1950	rVV5	1961	2473	0.13%	0.026%
23	16.048	2175	2178	2183	rVB5	1590	2061	0.11%	0.021%
24	16.618	2273	2275	2278	rBV3	1613	1957	0.10%	0.020%
25	17.154	2361	2366	2369	rVB	4145	5764	0.31%	0.060%
26	17.365	2395	2402	2412	rVV	1360573	1882468	100.00%	19.566%
27	17.459	2416	2418	2424	rVB2	4510	5898	0.31%	0.061%
28	17.777	2471	2472	2476	rVB4	1922	2048	0.11%	0.021%
29	18.253	2551	2553	2557	rVB4	2707	3273	0.17%	0.034%
30	18.489	2591	2593	2597	rBV4	2581	4208	0.22%	0.044%
31	18.548	2601	2603	2604	rBV2	2353	2184	0.12%	0.023%
32	19.530	2768	2770	2771	rBV2	4483	2230	0.12%	0.023%
33	21.536	3106	3111	3119	rBV	1184703	1488345	79.06%	15.470%
34	23.977	3520	3526	3536	rVB2	728283	1483048	78.78%	15.415%

Sum of corrected areas: 9621003

Instrument :

BNA_M

ClientSampleId :




SBLK058

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034176.D
Acq On : 09 Mar 2022 08:30
Operator : CG/JU
Sample : PB143058BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

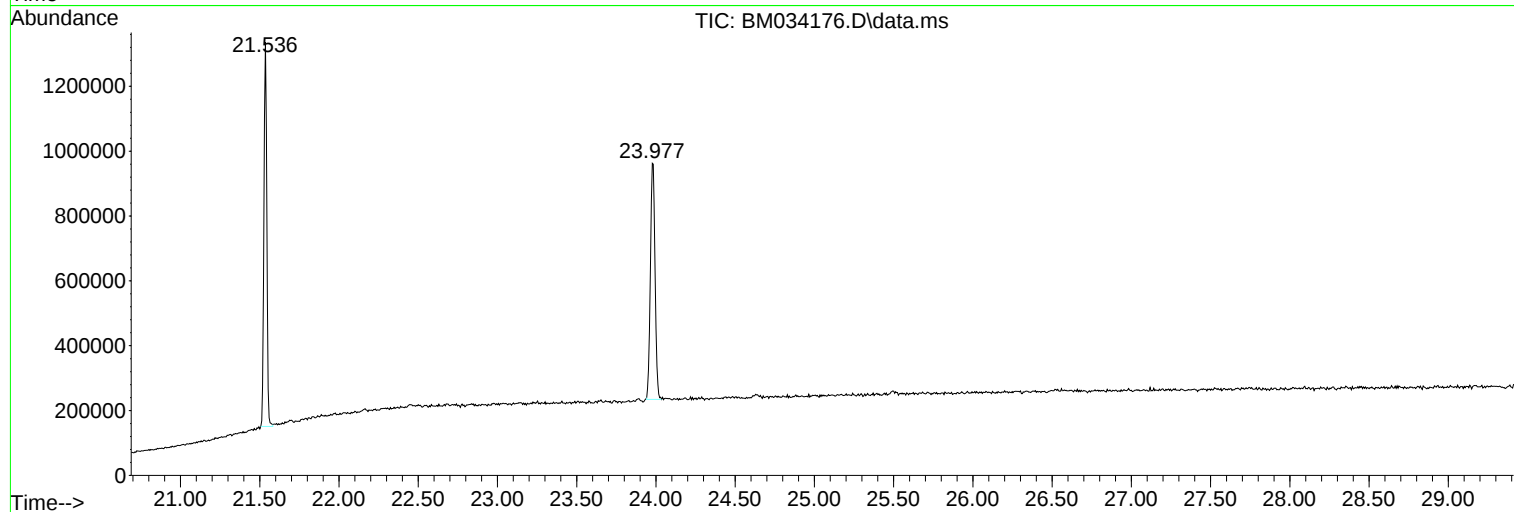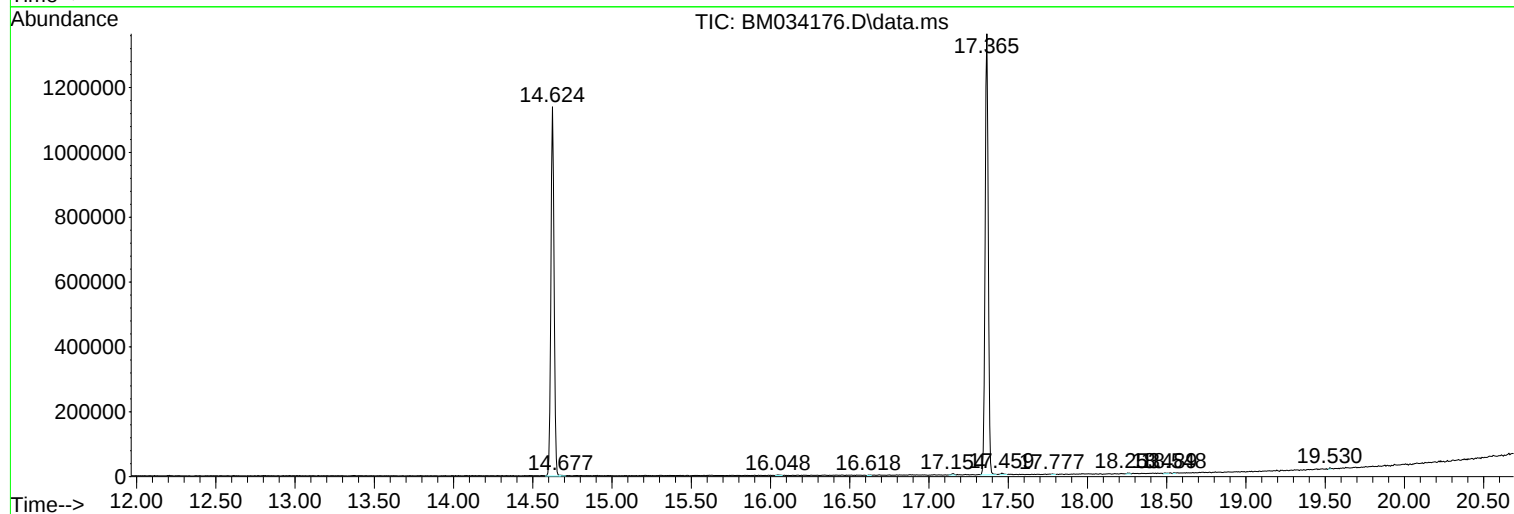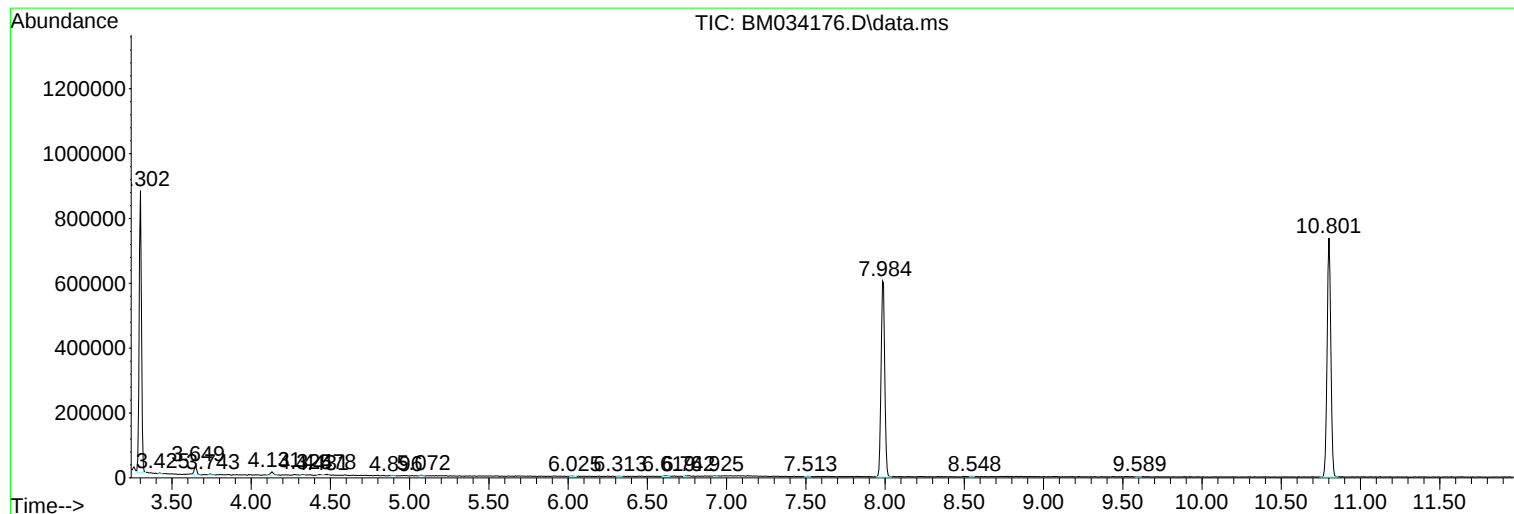

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034176.D
Acq On : 09 Mar 2022 08:30
Operator : CG/JU
Sample : PB143058BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK058










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.301	18.17 ng/ul	883703	1,4-Dichlorobenzene-d4	7.989

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane	100	C7H16	000142-82-5	91
2			Heptane	100	C7H16	000142-82-5	91
3			Heptane	100	C7H16	000142-82-5	87
4			Hydroxylamine, O-(2-methylpropyl)-	89	C4H11NO	005618-62-2	72
5			Heptane	100	C7H16	000142-82-5	58

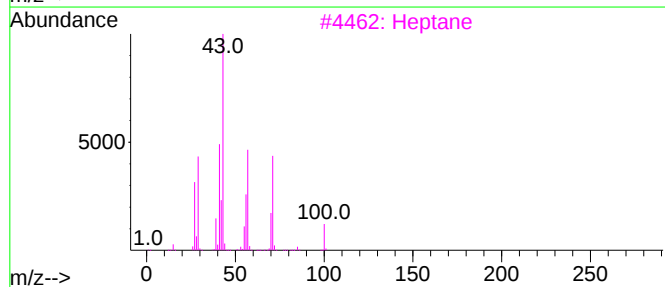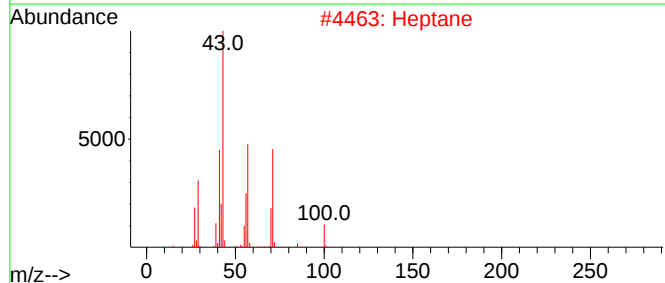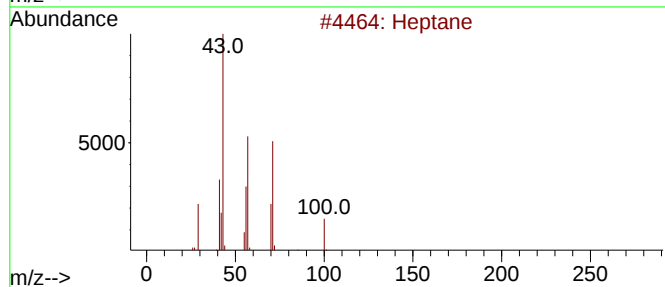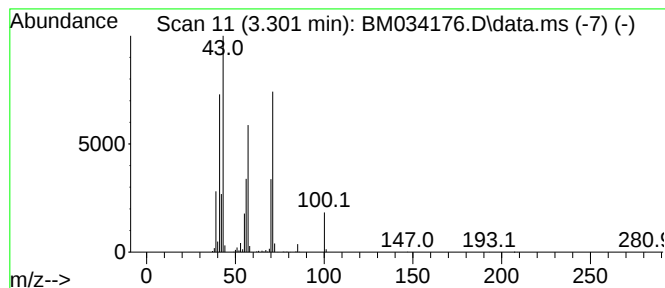

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034176.D
Acq On : 09 Mar 2022 08:30
Operator : CG/JU
Sample : PB143058BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.301	18.2	ng/u1	883703	1	7.989	972859	20.0