

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034180.D
 Acq On : 09 Mar 2022 11:31
 Operator : CG/JU
 Sample : PB143147BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK147

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.366	18	22	28	rBV	34358	45678	1.20%	0.122%
2	3.790	90	94	112	rBV	423163	629859	16.51%	1.684%
3	4.131	148	152	159	rBV3	8377	13943	0.37%	0.037%
4	7.137	656	663	674	rVB	563267	857146	22.47%	2.292%
5	7.307	686	692	701	rBV	418199	674635	17.69%	1.804%
6	7.513	721	727	738	rBV	568254	914507	23.98%	2.446%
7	7.989	800	808	816	rVB	524691	818949	21.47%	2.190%
8	8.689	919	927	938	rBV	725462	1130550	29.64%	3.023%
9	9.148	996	1005	1014	rBV	545598	877101	23.00%	2.346%
10	9.878	1121	1129	1138	rBV	457394	741221	19.43%	1.982%
11	10.419	1213	1221	1232	rBV	737696	1225459	32.13%	3.277%
12	10.742	1272	1276	1279	rBV4	1955	3924	0.10%	0.010%
13	10.801	1279	1286	1295	rVB	690605	1176998	30.86%	3.147%
14	10.930	1301	1308	1320	rBV	727534	1196733	31.38%	3.200%
15	12.389	1549	1556	1564	rBV	12807	20710	0.54%	0.055%
16	13.601	1758	1762	1767	rVB4	2614	3836	0.10%	0.010%
17	14.030	1829	1835	1841	rBV	1480538	1960097	51.39%	5.242%
18	14.318	1877	1884	1896	rBV	1605164	2275867	59.67%	6.086%
19	14.624	1927	1936	1945	rBV	1167036	1707243	44.76%	4.565%
20	14.801	1959	1966	1981	rBV	597790	869934	22.81%	2.326%
21	15.613	2098	2104	2111	rBV	2034793	2879009	75.49%	7.699%
22	15.718	2116	2122	2136	rVV	568051	784804	20.58%	2.099%
23	15.854	2141	2145	2152	rVB	8468	12685	0.33%	0.034%
24	16.289	2215	2219	2224	rVB5	3488	4506	0.12%	0.012%
25	17.148	2362	2365	2372	rVB3	5129	8980	0.24%	0.024%
26	17.365	2395	2402	2408	rBV	1501337	2062058	54.07%	5.514%
27	17.465	2412	2419	2433	rVV	2319219	3222338	84.49%	8.617%
28	19.318	2730	2734	2739	rBV3	27785	39485	1.04%	0.106%
29	19.389	2742	2746	2753	rVV	25821	37373	0.98%	0.100%
30	19.753	2801	2808	2818	rBV	2813455	3813992	100.00%	10.199%
31	21.536	3106	3111	3118	rVB	1751222	2199158	57.66%	5.881%
32	23.824	3493	3500	3507	rVB	1582627	3164463	82.97%	8.462%
33	23.977	3520	3526	3536	rVB2	994958	2021741	53.01%	5.406%




Sum of corrected areas: 37394982

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034180.D
Acq On : 09 Mar 2022 11:31
Operator : CG/JU
Sample : PB143147BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK147

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

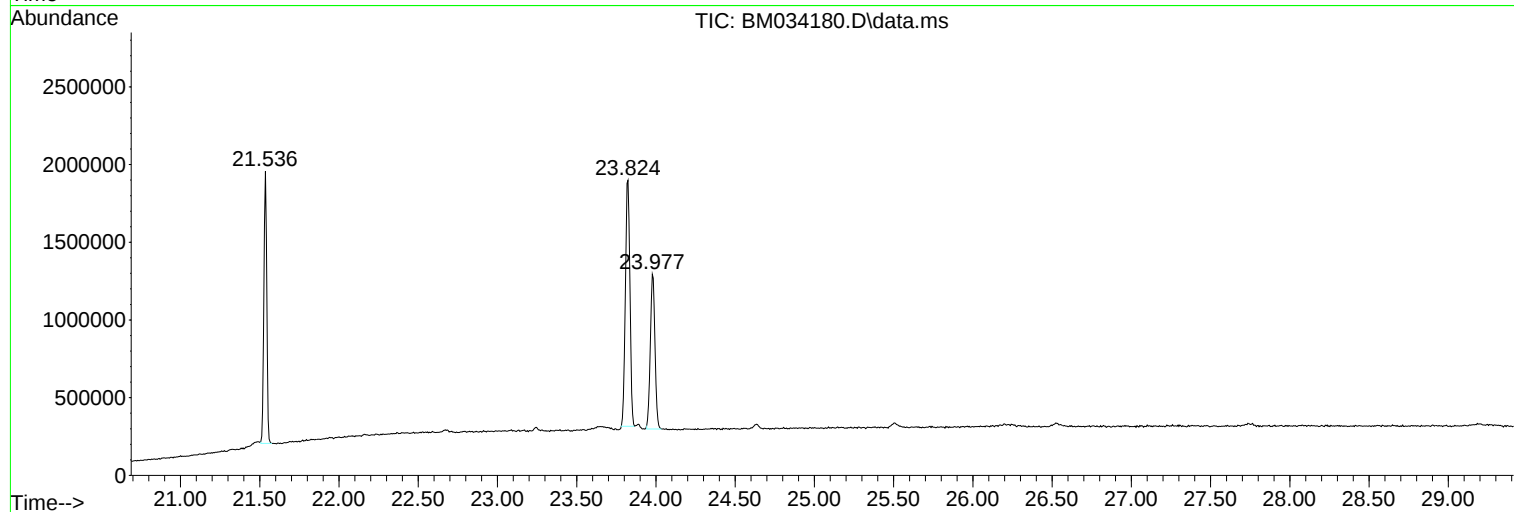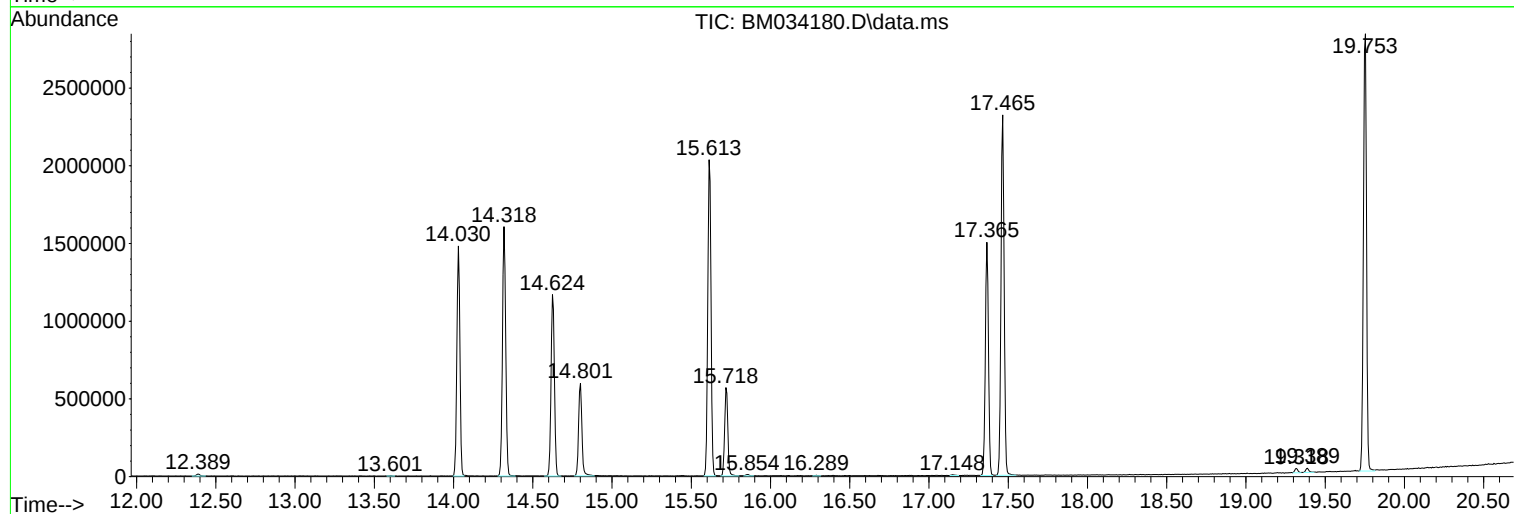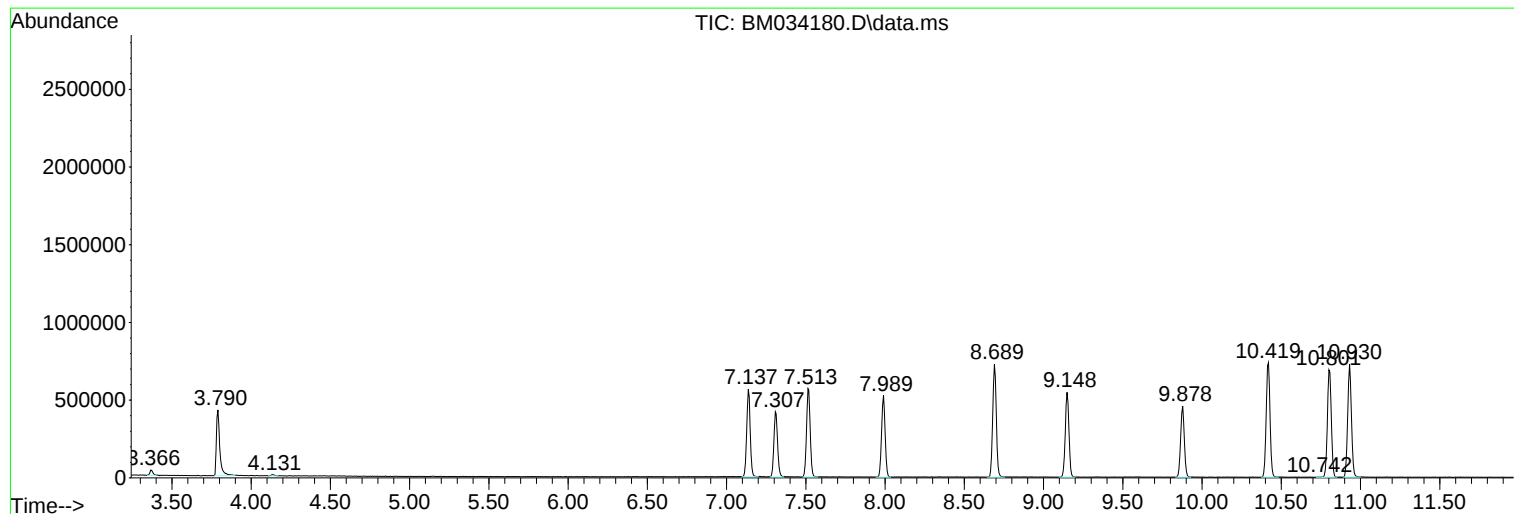

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034180.D
Acq On : 09 Mar 2022 11:31
Operator : CG/JU
Sample : PB143147BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK147

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034180.D
Acq On : 09 Mar 2022 11:31
Operator : CG/JU
Sample : PB143147BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK147

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------