

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034181.D
 Acq On : 09 Mar 2022 12:07
 Operator : CG/JU
 Sample : N1775-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRU7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034181.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.367	18	22	33	rBV	29505	46432	1.38%	0.132%
2	3.790	91	94	111	rBV	197723	306420	9.11%	0.870%
3	4.137	149	153	159	rVB2	9591	13938	0.41%	0.040%
4	5.067	305	311	315	rBV5	5228	9068	0.27%	0.026%
5	7.137	657	663	673	rVB	474958	751755	22.34%	2.134%
6	7.308	685	692	702	rBV	367549	583480	17.34%	1.656%
7	7.513	720	727	739	rBV	498809	792208	23.54%	2.249%
8	7.990	800	808	815	rBV	567770	877454	26.08%	2.491%
9	8.690	920	927	936	rBV	623918	977219	29.04%	2.774%
10	9.149	997	1005	1015	rVB	473650	766007	22.76%	2.174%
11	9.325	1029	1035	1038	rBV6	5867	8053	0.24%	0.023%
12	9.607	1078	1083	1089	rVB2	11114	17890	0.53%	0.051%
13	9.878	1122	1129	1138	rBV	364223	587445	17.46%	1.667%
14	10.413	1213	1220	1236	rBV	639206	1070990	31.83%	3.040%
15	10.584	1245	1249	1254	rBV4	8787	14612	0.43%	0.041%
16	10.802	1279	1286	1294	rVB	735284	1255871	37.32%	3.565%
17	10.931	1301	1308	1322	rBV	619362	1033162	30.70%	2.933%
18	12.113	1501	1509	1511	rBV4	2427	4860	0.14%	0.014%
19	12.237	1524	1530	1534	rVB3	4374	6416	0.19%	0.018%
20	12.390	1551	1556	1562	rVB2	10907	16772	0.50%	0.048%
21	13.001	1656	1660	1663	rBV5	2694	3676	0.11%	0.010%
22	13.243	1697	1701	1710	rVB6	4671	7788	0.23%	0.022%
23	13.466	1735	1739	1743	rBV2	11814	16807	0.50%	0.048%
24	13.595	1756	1761	1765	rBV6	3796	5423	0.16%	0.015%
25	14.031	1828	1835	1841	rBV	1224834	1615215	48.00%	4.585%
26	14.078	1841	1843	1847	rVV4	5380	7699	0.23%	0.022%
27	14.113	1847	1849	1853	rVV5	2826	3689	0.11%	0.010%
28	14.160	1853	1857	1861	rVB4	2817	4437	0.13%	0.013%
29	14.272	1871	1876	1878	rBV2	16808	23524	0.70%	0.067%
30	14.319	1878	1884	1891	rVB	1399589	1984888	58.99%	5.634%
31	14.531	1916	1920	1924	rBV3	7690	10257	0.30%	0.029%
32	14.625	1929	1936	1945	rVB	1276395	1829213	54.36%	5.192%
33	14.795	1957	1965	1977	rBV	409063	630238	18.73%	1.789%
34	14.872	1977	1978	1985	rVB6	5403	6060	0.18%	0.017%
35	15.025	2001	2004	2012	rVB7	4174	7009	0.21%	0.020%
36	15.260	2039	2044	2051	rBV2	7543	10593	0.31%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034181.D
 Acq On : 09 Mar 2022 12:07
 Operator : CG/JU
 Sample : N1775-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRU7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

37	15.431	2066	2073	2077	rBV3	16445	25997	0.77%	0.074%
38	15.484	2078	2082	2087	rVB5	7558	11499	0.34%	0.033%
39	15.613	2098	2104	2112	rBV	1816781	2553564	75.89%	7.248%
40	15.719	2117	2122	2131	rBV	361808	480179	14.27%	1.363%

41	15.854	2142	2145	2148	rBV2	8440	11706	0.35%	0.033%
42	15.978	2160	2166	2170	rBV7	4364	7621	0.23%	0.022%
43	16.036	2172	2176	2177	rVV3	4345	5548	0.16%	0.016%
44	16.054	2177	2179	2182	rVB3	3626	3597	0.11%	0.010%
45	16.160	2193	2197	2200	rBV6	2695	3387	0.10%	0.010%

46	16.254	2210	2213	2216	rBV5	4775	6578	0.20%	0.019%
47	16.295	2216	2220	2224	rVV5	8171	14895	0.44%	0.042%
48	16.336	2224	2227	2231	rVV5	8917	14237	0.42%	0.040%
49	16.407	2235	2239	2243	rVB6	5649	8112	0.24%	0.023%
50	16.507	2253	2256	2261	rVB3	8280	10688	0.32%	0.030%

51	16.683	2281	2286	2289	rBV6	3998	6232	0.19%	0.018%
52	16.754	2294	2298	2299	rBV3	2846	3843	0.11%	0.011%
53	16.848	2310	2314	2317	rBV6	5768	8449	0.25%	0.024%
54	17.054	2343	2349	2352	rBV9	2680	4824	0.14%	0.014%
55	17.083	2352	2354	2357	rBV4	2995	3476	0.10%	0.010%

56	17.131	2357	2362	2364	rBV4	9737	14315	0.43%	0.041%
57	17.183	2369	2371	2376	rVB5	5525	7324	0.22%	0.021%
58	17.289	2385	2389	2392	rVB5	12887	16260	0.48%	0.046%
59	17.366	2395	2402	2410	rBV	1628697	2250946	66.89%	6.389%
60	17.466	2412	2419	2429	rVV	1997060	2834728	84.24%	8.046%

61	17.554	2431	2434	2440	rVB8	11029	14796	0.44%	0.042%
62	17.736	2463	2465	2469	rVB5	4124	4238	0.13%	0.012%
63	17.872	2484	2488	2489	rBV3	4619	5187	0.15%	0.015%
64	18.042	2511	2517	2522	rVB5	11254	16666	0.50%	0.047%
65	18.260	2549	2554	2559	rBV2	34094	46512	1.38%	0.132%

66	18.336	2563	2567	2570	rVB	7073	9223	0.27%	0.026%
67	18.477	2588	2591	2593	rBV4	3144	3598	0.11%	0.010%
68	18.560	2603	2605	2609	rBV4	4401	5511	0.16%	0.016%
69	18.866	2654	2657	2659	rBV4	6249	7692	0.23%	0.022%
70	19.319	2730	2734	2738	rBV2	27389	39380	1.17%	0.112%

71	19.354	2738	2740	2742	rBV3	9107	8921	0.27%	0.025%
72	19.389	2742	2746	2749	rVV	26716	32863	0.98%	0.093%
73	19.530	2766	2770	2773	rBV6	15315	20052	0.60%	0.057%
74	19.754	2802	2808	2813	rBV	2495291	3364946	100.00%	9.551%
75	21.242	3058	3061	3067	rBV	148717	184749	5.49%	0.524%

76	21.536	3106	3111	3120	rBV	2011251	2516393	74.78%	7.143%
----	--------	------	------	------	-----	---------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034181.D
Acq On : 09 Mar 2022 12:07
Operator : CG/JU
Sample : N1775-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRU7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Title : SVOA CALIBRATION

77	23.824	3493	3500	3508	rBV2	1537451	2954154	87.79%	8.385%
78	23.983	3520	3527	3538	rVB2	1154289	2380735	70.75%	6.758%




Sum of corrected areas: 35230189

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034181.D
Acq On : 09 Mar 2022 12:07
Operator : CG/JU
Sample : N1775-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRU7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

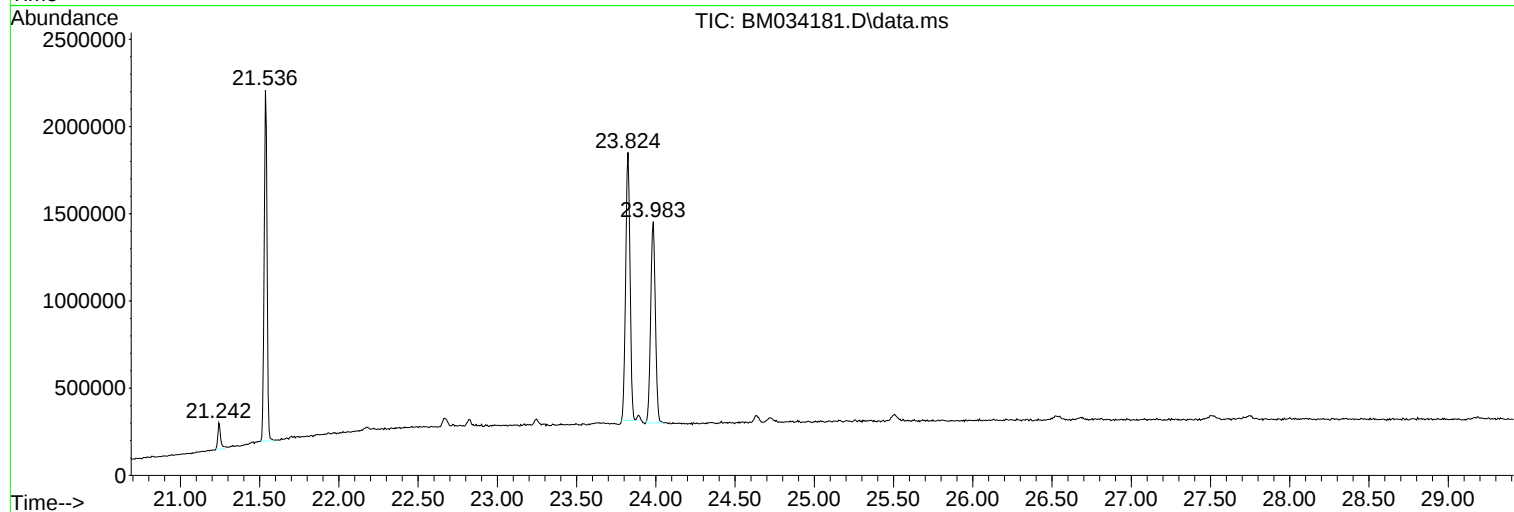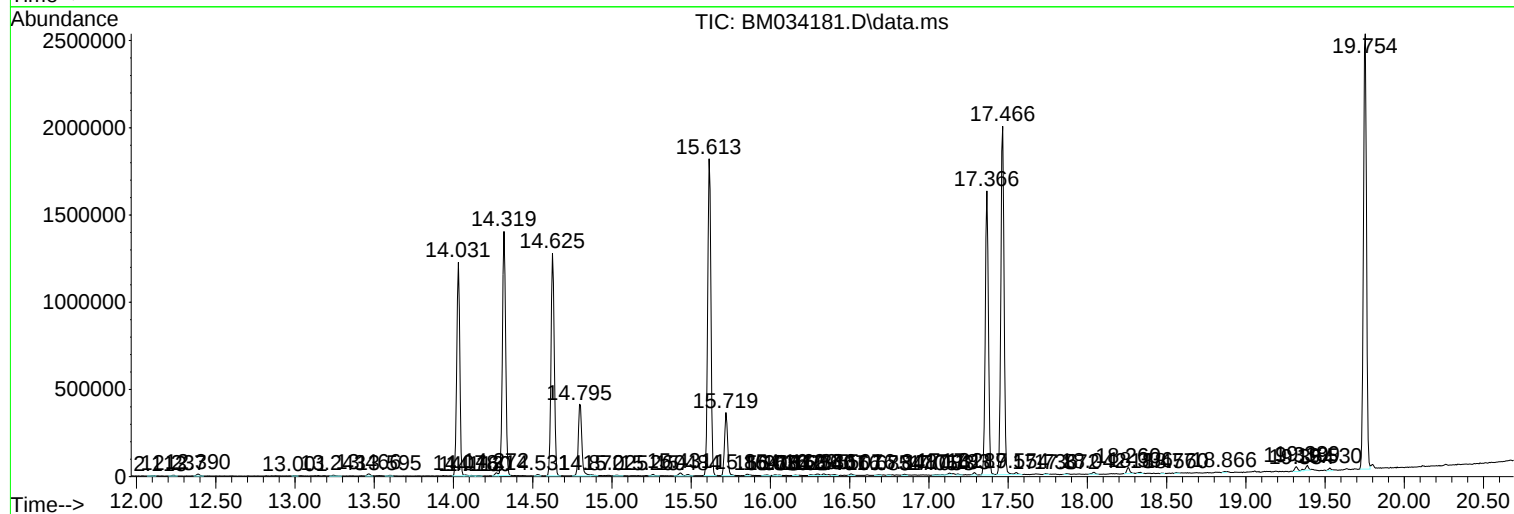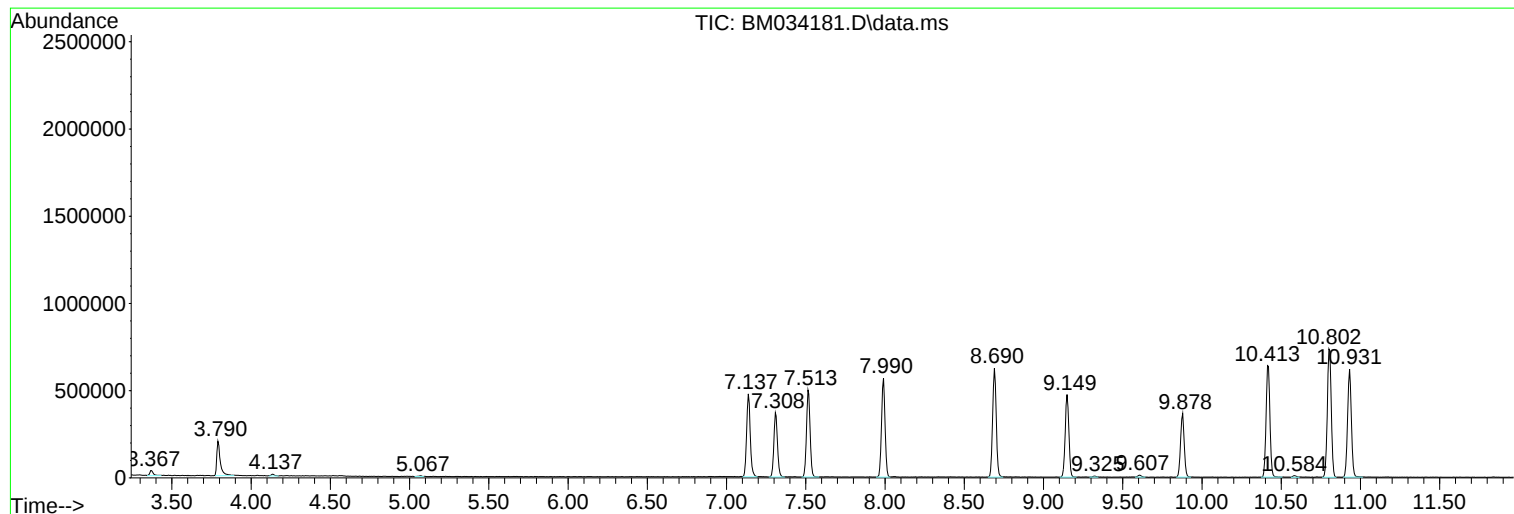

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034181.D
Acq On : 09 Mar 2022 12:07
Operator : CG/JU
Sample : N1775-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRU7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034181.D
Acq On : 09 Mar 2022 12:07
Operator : CG/JU
Sample : N1775-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRU7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc