

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM030822\  
 Data File : BM034186.D  
 Acq On : 09 Mar 2022 15:08  
 Operator : CG/JU  
 Sample : N1775-24  
 Misc :  
 ALS Vial : 45 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DBSC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM030822.M  
 Title : SVOA CALIBRATION

Signal : TIC: BM034186.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.372       | 19            | 23          | 28           | rVB3     | 6989           | 10545         | 0.35%           | 0.038%        |
| 2         | 3.802       | 93            | 96          | 104          | rBV      | 27733          | 44056         | 1.48%           | 0.158%        |
| 3         | 4.137       | 148           | 153         | 157          | rVB4     | 8195           | 12327         | 0.41%           | 0.044%        |
| 4         | 7.137       | 657           | 663         | 672          | rVB      | 159746         | 247565        | 8.31%           | 0.889%        |
| 5         | 7.307       | 686           | 692         | 702          | rVB      | 124107         | 196482        | 6.60%           | 0.705%        |
| 6         | 7.513       | 719           | 727         | 738          | rVB      | 142331         | 224445        | 7.53%           | 0.806%        |
| 7         | 7.990       | 800           | 808         | 816          | rBV      | 491195         | 780412        | 26.20%          | 2.801%        |
| 8         | 8.690       | 920           | 927         | 937          | rBV      | 288423         | 459575        | 15.43%          | 1.650%        |
| 9         | 9.148       | 998           | 1005        | 1012         | rBV      | 211514         | 345408        | 11.60%          | 1.240%        |
| 10        | 9.607       | 1079          | 1083        | 1088         | rVB4     | 6375           | 10241         | 0.34%           | 0.037%        |
| 11        | 9.878       | 1121          | 1129        | 1136         | rBV      | 185370         | 304673        | 10.23%          | 1.094%        |
| 12        | 10.419      | 1212          | 1221        | 1231         | rBV      | 330914         | 561889        | 18.86%          | 2.017%        |
| 13        | 10.584      | 1245          | 1249        | 1258         | rVB6     | 4345           | 7837          | 0.26%           | 0.028%        |
| 14        | 10.801      | 1279          | 1286        | 1295         | rVB      | 686711         | 1130895       | 37.96%          | 4.059%        |
| 15        | 10.931      | 1301          | 1308        | 1323         | rVB      | 383212         | 648095        | 21.76%          | 2.326%        |
| 16        | 11.213      | 1352          | 1356        | 1360         | rVB4     | 1869           | 3524          | 0.12%           | 0.013%        |
| 17        | 12.236      | 1527          | 1530        | 1533         | rVB4     | 3159           | 4031          | 0.14%           | 0.014%        |
| 18        | 12.389      | 1551          | 1556        | 1561         | rBV2     | 7361           | 11390         | 0.38%           | 0.041%        |
| 19        | 13.001      | 1655          | 1660        | 1663         | rBV5     | 1849           | 3381          | 0.11%           | 0.012%        |
| 20        | 13.042      | 1665          | 1667        | 1674         | rVB5     | 2657           | 3231          | 0.11%           | 0.012%        |
| 21        | 13.383      | 1721          | 1725        | 1729         | rBV3     | 3490           | 5624          | 0.19%           | 0.020%        |
| 22        | 13.466      | 1735          | 1739        | 1744         | rBV2     | 13581          | 18122         | 0.61%           | 0.065%        |
| 23        | 13.601      | 1760          | 1762        | 1767         | rVB5     | 2858           | 3324          | 0.11%           | 0.012%        |
| 24        | 14.030      | 1827          | 1835        | 1841         | rBV      | 1045348        | 1409340       | 47.31%          | 5.058%        |
| 25        | 14.072      | 1841          | 1842        | 1848         | rVB5     | 2375           | 3147          | 0.11%           | 0.011%        |
| 26        | 14.154      | 1853          | 1856        | 1860         | rVB5     | 2423           | 3116          | 0.10%           | 0.011%        |
| 27        | 14.272      | 1873          | 1876        | 1877         | rBV3     | 5532           | 5495          | 0.18%           | 0.020%        |
| 28        | 14.319      | 1878          | 1884        | 1891         | rVB      | 1145484        | 1615919       | 54.25%          | 5.800%        |
| 29        | 14.536      | 1915          | 1921        | 1924         | rVB2     | 7020           | 10969         | 0.37%           | 0.039%        |
| 30        | 14.625      | 1928          | 1936        | 1946         | rVB      | 1149986        | 1675661       | 56.25%          | 6.014%        |
| 31        | 14.795      | 1959          | 1965        | 1976         | rBV      | 345413         | 522755        | 17.55%          | 1.876%        |
| 32        | 14.977      | 1993          | 1996        | 2001         | rVB7     | 3444           | 5321          | 0.18%           | 0.019%        |
| 33        | 15.030      | 2001          | 2005        | 2009         | rBV6     | 4333           | 6702          | 0.22%           | 0.024%        |
| 34        | 15.166      | 2022          | 2028        | 2029         | rBV5     | 4214           | 6090          | 0.20%           | 0.022%        |
| 35        | 15.260      | 2040          | 2044        | 2047         | rBV6     | 3193           | 4823          | 0.16%           | 0.017%        |
| 36        | 15.430      | 2065          | 2073        | 2078         | rBV6     | 8054           | 15639         | 0.53%           | 0.056%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM030822\  
 Data File : BM034186.D  
 Acq On : 09 Mar 2022 15:08  
 Operator : CG/JU  
 Sample : N1775-24  
 Misc :  
 ALS Vial : 45 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DBSC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM030822.M  
 Title : SVOA CALIBRATION

|    |        |      |      |      |      |         |         |         |         |
|----|--------|------|------|------|------|---------|---------|---------|---------|
| 37 | 15.477 | 2078 | 2081 | 2085 | rVB2 | 4489    | 5075    | 0.17%   | 0.018%  |
| 38 | 15.613 | 2097 | 2104 | 2116 | rVB  | 1584741 | 2217781 | 74.45%  | 7.960%  |
| 39 | 15.719 | 2116 | 2122 | 2132 | rBV  | 315526  | 432304  | 14.51%  | 1.552%  |
| 40 | 15.854 | 2139 | 2145 | 2149 | rBV3 | 9274    | 14385   | 0.48%   | 0.052%  |
| 41 | 15.977 | 2164 | 2166 | 2171 | rVB5 | 3067    | 3762    | 0.13%   | 0.014%  |
| 42 | 16.042 | 2171 | 2177 | 2178 | rBV6 | 2789    | 5278    | 0.18%   | 0.019%  |
| 43 | 16.166 | 2194 | 2198 | 2204 | rBV8 | 2425    | 5529    | 0.19%   | 0.020%  |
| 44 | 16.295 | 2216 | 2220 | 2223 | rVV5 | 4638    | 6422    | 0.22%   | 0.023%  |
| 45 | 16.336 | 2223 | 2227 | 2230 | rVB6 | 2811    | 4577    | 0.15%   | 0.016%  |
| 46 | 16.401 | 2236 | 2238 | 2242 | rVB5 | 3395    | 4089    | 0.14%   | 0.015%  |
| 47 | 16.513 | 2252 | 2257 | 2260 | rBV4 | 2943    | 5316    | 0.18%   | 0.019%  |
| 48 | 16.601 | 2271 | 2272 | 2278 | rVB6 | 2118    | 3717    | 0.12%   | 0.013%  |
| 49 | 16.683 | 2282 | 2286 | 2289 | rVB5 | 2527    | 3292    | 0.11%   | 0.012%  |
| 50 | 16.766 | 2297 | 2300 | 2304 | rVB6 | 2837    | 4230    | 0.14%   | 0.015%  |
| 51 | 16.842 | 2309 | 2313 | 2315 | rVV5 | 2733    | 3818    | 0.13%   | 0.014%  |
| 52 | 17.154 | 2357 | 2366 | 2368 | rBV5 | 6101    | 13234   | 0.44%   | 0.047%  |
| 53 | 17.289 | 2385 | 2389 | 2393 | rVB7 | 6681    | 9534    | 0.32%   | 0.034%  |
| 54 | 17.366 | 2395 | 2402 | 2408 | rBV  | 1506654 | 2052798 | 68.91%  | 7.368%  |
| 55 | 17.466 | 2412 | 2419 | 2429 | rVV  | 1768136 | 2500660 | 83.95%  | 8.975%  |
| 56 | 17.542 | 2430 | 2432 | 2438 | rVB7 | 7634    | 12749   | 0.43%   | 0.046%  |
| 57 | 17.736 | 2463 | 2465 | 2468 | rBV3 | 3549    | 3510    | 0.12%   | 0.013%  |
| 58 | 18.042 | 2512 | 2517 | 2520 | rVV4 | 12270   | 17473   | 0.59%   | 0.063%  |
| 59 | 18.254 | 2549 | 2553 | 2561 | rBV3 | 43890   | 66815   | 2.24%   | 0.240%  |
| 60 | 19.212 | 2713 | 2716 | 2720 | rVB5 | 7081    | 6980    | 0.23%   | 0.025%  |
| 61 | 19.318 | 2730 | 2734 | 2738 | rBV4 | 22322   | 32289   | 1.08%   | 0.116%  |
| 62 | 19.389 | 2742 | 2746 | 2748 | rBV  | 26646   | 35380   | 1.19%   | 0.127%  |
| 63 | 19.530 | 2767 | 2770 | 2772 | rBV2 | 13598   | 14899   | 0.50%   | 0.053%  |
| 64 | 19.748 | 2801 | 2807 | 2813 | rBV  | 2164834 | 2978791 | 100.00% | 10.691% |
| 65 | 21.242 | 3058 | 3061 | 3067 | rBV2 | 108329  | 135766  | 4.56%   | 0.487%  |
| 66 | 21.536 | 3106 | 3111 | 3117 | rBV  | 1820891 | 2262734 | 75.96%  | 8.121%  |
| 67 | 23.824 | 3493 | 3500 | 3507 | rBV  | 1318580 | 2541011 | 85.30%  | 9.120%  |
| 68 | 23.983 | 3520 | 3527 | 3539 | rVB  | 1056878 | 2135091 | 71.68%  | 7.663%  |




Sum of corrected areas: 27861338

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM030822\  
Data File : BM034186.D  
Acq On : 09 Mar 2022 15:08  
Operator : CG/JU  
Sample : N1775-24  
Misc :  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DBSC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM030822.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

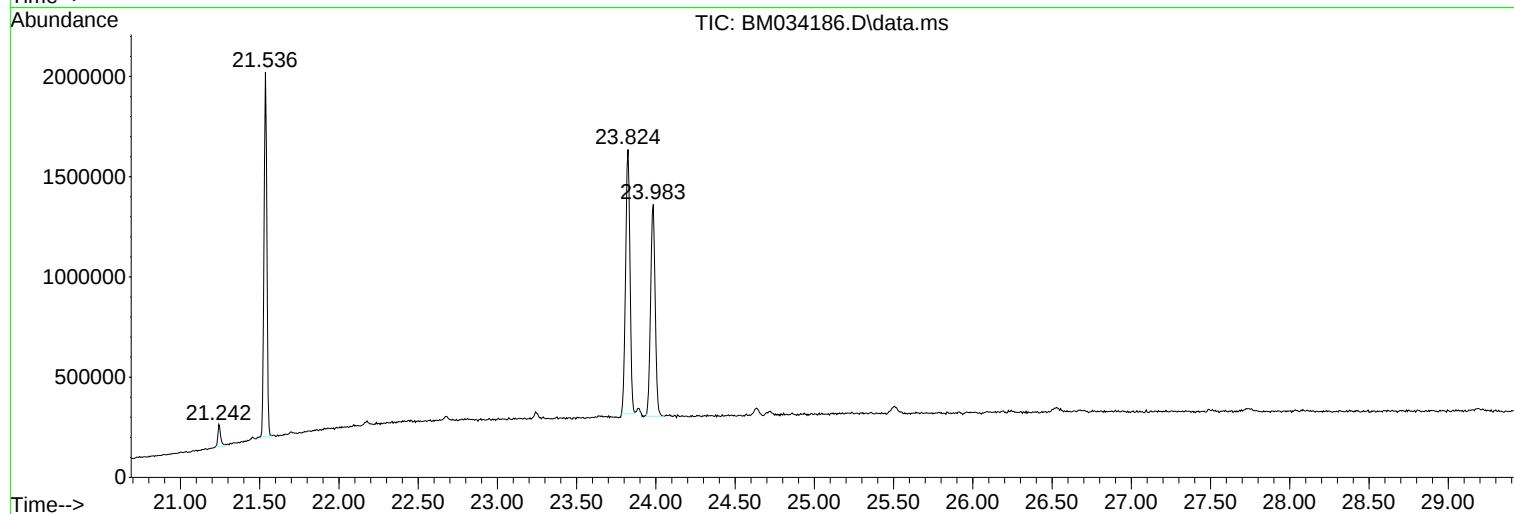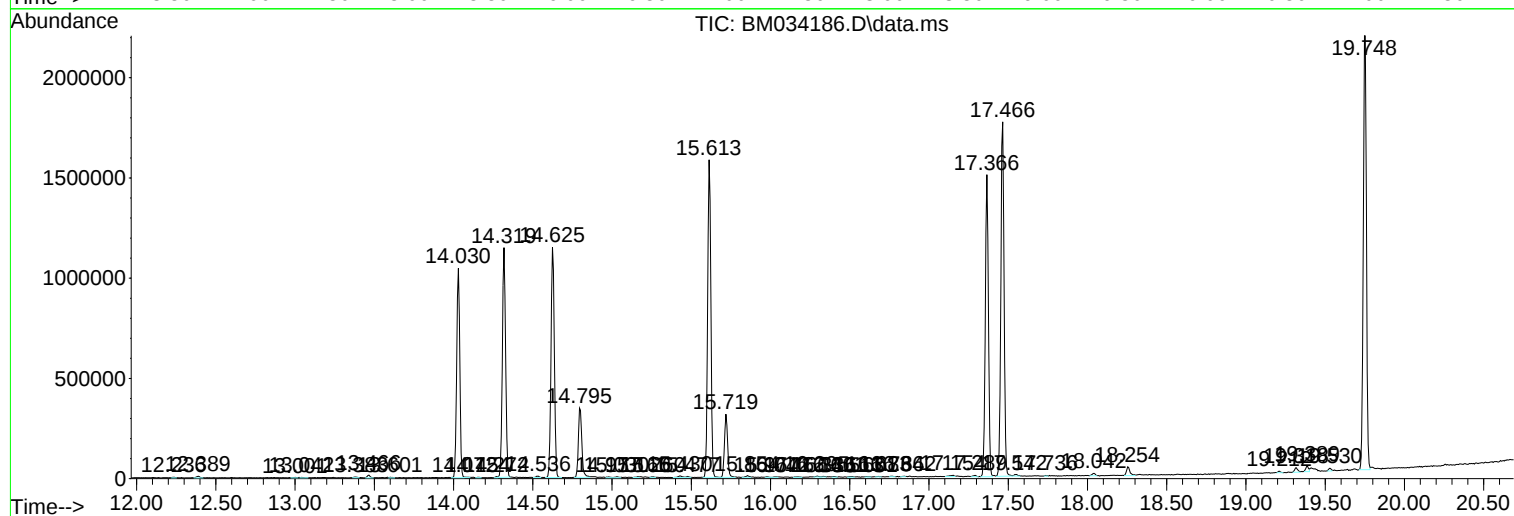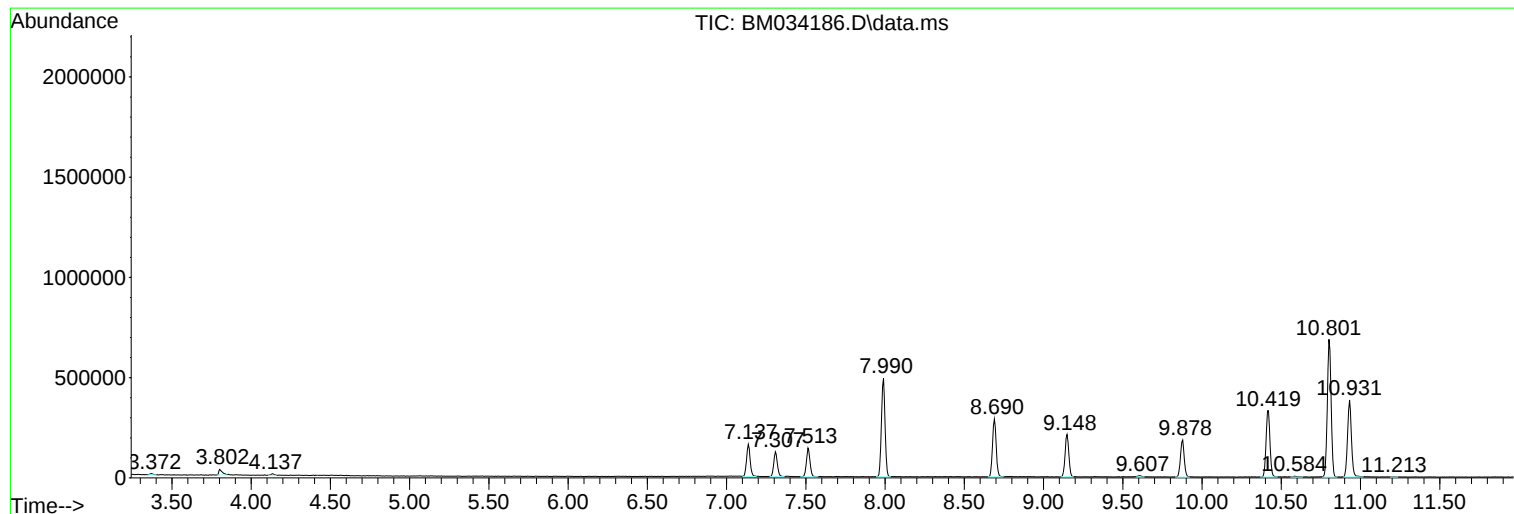

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM030822\  
Data File : BM034186.D  
Acq On : 09 Mar 2022 15:08  
Operator : CG/JU  
Sample : N1775-24  
Misc :  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DBSC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM030822.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM030822\  
Data File : BM034186.D  
Acq On : 09 Mar 2022 15:08  
Operator : CG/JU  
Sample : N1775-24  
Misc :  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DBSC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM030822.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |