

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034187.D
 Acq On : 09 Mar 2022 15:45
 Operator : CG/JU
 Sample : N1775-03
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRU9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.366	18	22	30	rVB	33952	47037	1.41%	0.131%
2	3.790	90	94	107	rBV	410278	601583	18.02%	1.670%
3	4.137	150	153	157	rVB	9319	12542	0.38%	0.035%
4	5.060	307	310	311	rBV2	5226	4641	0.14%	0.013%
5	5.660	408	412	416	rBV6	2537	4257	0.13%	0.012%
6	6.160	494	497	502	rBV6	2289	3812	0.11%	0.011%
7	7.137	656	663	675	rVB	551789	875965	26.24%	2.432%
8	7.307	685	692	703	rBV	420326	658572	19.73%	1.828%
9	7.513	720	727	738	rVB	582880	904251	27.09%	2.511%
10	7.989	800	808	815	rBV	497435	780749	23.39%	2.168%
11	8.054	816	819	824	rVB5	3296	5354	0.16%	0.015%
12	8.689	920	927	935	rBV	716862	1137342	34.07%	3.158%
13	9.148	998	1005	1014	rVB	541458	866853	25.97%	2.407%
14	9.319	1029	1034	1041	rBV7	9246	16393	0.49%	0.046%
15	9.601	1075	1082	1088	rVB3	16337	25843	0.77%	0.072%
16	9.878	1121	1129	1140	rVB	451508	744003	22.29%	2.066%
17	10.289	1195	1199	1204	rBV4	3794	6201	0.19%	0.017%
18	10.419	1213	1221	1230	rBV	747450	1245054	37.29%	3.457%
19	10.583	1243	1249	1257	rBV2	15336	27394	0.82%	0.076%
20	10.801	1279	1286	1294	rVB	676269	1113669	33.36%	3.092%
21	10.930	1299	1308	1319	rBV	689728	1168583	35.00%	3.245%
22	12.107	1500	1508	1513	rBV2	12736	20985	0.63%	0.058%
23	12.230	1524	1529	1534	rVB4	4413	6840	0.20%	0.019%
24	12.389	1550	1556	1561	rBV2	12758	20666	0.62%	0.057%
25	13.177	1688	1690	1694	rVB5	3197	3371	0.10%	0.009%
26	13.242	1694	1701	1705	rBV3	4354	7208	0.22%	0.020%
27	13.466	1733	1739	1743	rBV	14002	17825	0.53%	0.049%
28	13.530	1746	1750	1753	rBV5	3531	4999	0.15%	0.014%
29	13.595	1758	1761	1763	rBV3	3985	4956	0.15%	0.014%
30	13.913	1810	1815	1821	rBV9	4305	6653	0.20%	0.018%
31	14.030	1829	1835	1841	rBV	1394961	1909781	57.20%	5.302%
32	14.077	1841	1843	1847	rVV3	10392	12675	0.38%	0.035%
33	14.107	1847	1848	1852	rVV4	2620	3360	0.10%	0.009%
34	14.154	1855	1856	1863	rVB6	3011	4594	0.14%	0.013%
35	14.271	1871	1876	1878	rBV2	18295	25815	0.77%	0.072%
36	14.318	1878	1884	1894	rVB	1615631	2259695	67.69%	6.274%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034187.D
 Acq On : 09 Mar 2022 15:45
 Operator : CG/JU
 Sample : N1775-03
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRU9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

37	14.530	1916	1920	1925	rVB5	10083	15428	0.46%	0.043%
38	14.624	1930	1936	1947	rVB	1126297	1625991	48.70%	4.514%
39	14.801	1958	1966	1979	rBV	487198	728161	21.81%	2.022%
40	15.030	2001	2005	2011	rVB5	8217	12298	0.37%	0.034%
41	15.213	2033	2036	2040	rBV6	2995	4521	0.14%	0.013%
42	15.260	2040	2044	2049	rVB	8641	11265	0.34%	0.031%
43	15.430	2066	2073	2077	rBV2	18220	30011	0.90%	0.083%
44	15.477	2077	2081	2085	rVB3	11162	13401	0.40%	0.037%
45	15.612	2097	2104	2112	rBV	2047735	2853532	85.47%	7.923%
46	15.718	2116	2122	2136	rVB	495975	650069	19.47%	1.805%
47	15.854	2142	2145	2149	rBV3	10383	12934	0.39%	0.036%
48	15.971	2162	2165	2171	rVB7	4863	5743	0.17%	0.016%
49	16.030	2171	2175	2178	rBV4	4992	6993	0.21%	0.019%
50	16.101	2182	2187	2193	rVB8	2925	4808	0.14%	0.013%
51	16.160	2193	2197	2199	rBV3	3143	5103	0.15%	0.014%
52	16.254	2209	2213	2217	rBV5	5787	8583	0.26%	0.024%
53	16.295	2217	2220	2225	rVV5	9130	15220	0.46%	0.042%
54	16.336	2225	2227	2230	rVV4	10857	12028	0.36%	0.033%
55	16.360	2230	2231	2234	rVV3	5706	5887	0.18%	0.016%
56	16.401	2236	2238	2245	rVB6	5314	7133	0.21%	0.020%
57	16.507	2253	2256	2261	rVB3	7606	10395	0.31%	0.029%
58	16.618	2272	2275	2278	rVB5	3655	3711	0.11%	0.010%
59	16.689	2281	2287	2288	rBV6	3962	7235	0.22%	0.020%
60	16.848	2310	2314	2316	rBV5	7823	9624	0.29%	0.027%
61	16.907	2321	2324	2329	rVV7	3094	4216	0.13%	0.012%
62	17.136	2357	2363	2364	rBV3	8264	13074	0.39%	0.036%
63	17.183	2369	2371	2376	rVB6	7494	8447	0.25%	0.023%
64	17.289	2385	2389	2393	rVB4	16167	19654	0.59%	0.055%
65	17.365	2396	2402	2410	rBV	1373967	1911762	57.26%	5.308%
66	17.465	2412	2419	2429	rVV	2114606	3028908	90.73%	8.410%
67	17.548	2429	2433	2439	rVB6	15583	25406	0.76%	0.071%
68	17.677	2449	2455	2462	rBV10	5871	12929	0.39%	0.036%
69	17.742	2462	2466	2468	rBV4	3443	5589	0.17%	0.016%
70	17.871	2486	2488	2491	rVB3	4413	3758	0.11%	0.010%
71	18.042	2510	2517	2521	rBV5	11246	17342	0.52%	0.048%
72	18.253	2549	2553	2561	rBV	62648	91069	2.73%	0.253%
73	18.559	2603	2605	2608	rBV4	5156	6238	0.19%	0.017%
74	19.118	2697	2700	2701	rBV2	5869	5345	0.16%	0.015%
75	19.318	2729	2734	2737	rBV3	30805	44496	1.33%	0.124%
76	19.353	2737	2740	2742	rBV3	8027	9581	0.29%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034187.D
 Acq On : 09 Mar 2022 15:45
 Operator : CG/JU
 Sample : N1775-03
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRU9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

77	19.383	2742	2745	2749	rBV2	40309	56645	1.70%	0.157%
78	19.530	2766	2770	2774	rBV6	23218	32973	0.99%	0.092%
79	19.683	2794	2796	2799	rVB4	11435	11731	0.35%	0.033%
80	19.753	2801	2808	2813	rVV	2454652	3338527	100.00%	9.269%
81	19.800	2813	2816	2821	rVB3	26697	34644	1.04%	0.096%
82	21.242	3058	3061	3067	rBV	172551	233646	7.00%	0.649%
83	21.536	3106	3111	3120	rBV	1457506	1817474	54.44%	5.046%
84	23.824	3493	3500	3508	rBV2	1514774	2877602	86.19%	7.990%
85	23.983	3520	3527	3534	rVB	866004	1786553	53.51%	4.960%


Sum of corrected areas: 36017204

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034187.D
Acq On : 09 Mar 2022 15:45
Operator : CG/JU
Sample : N1775-03
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRU9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

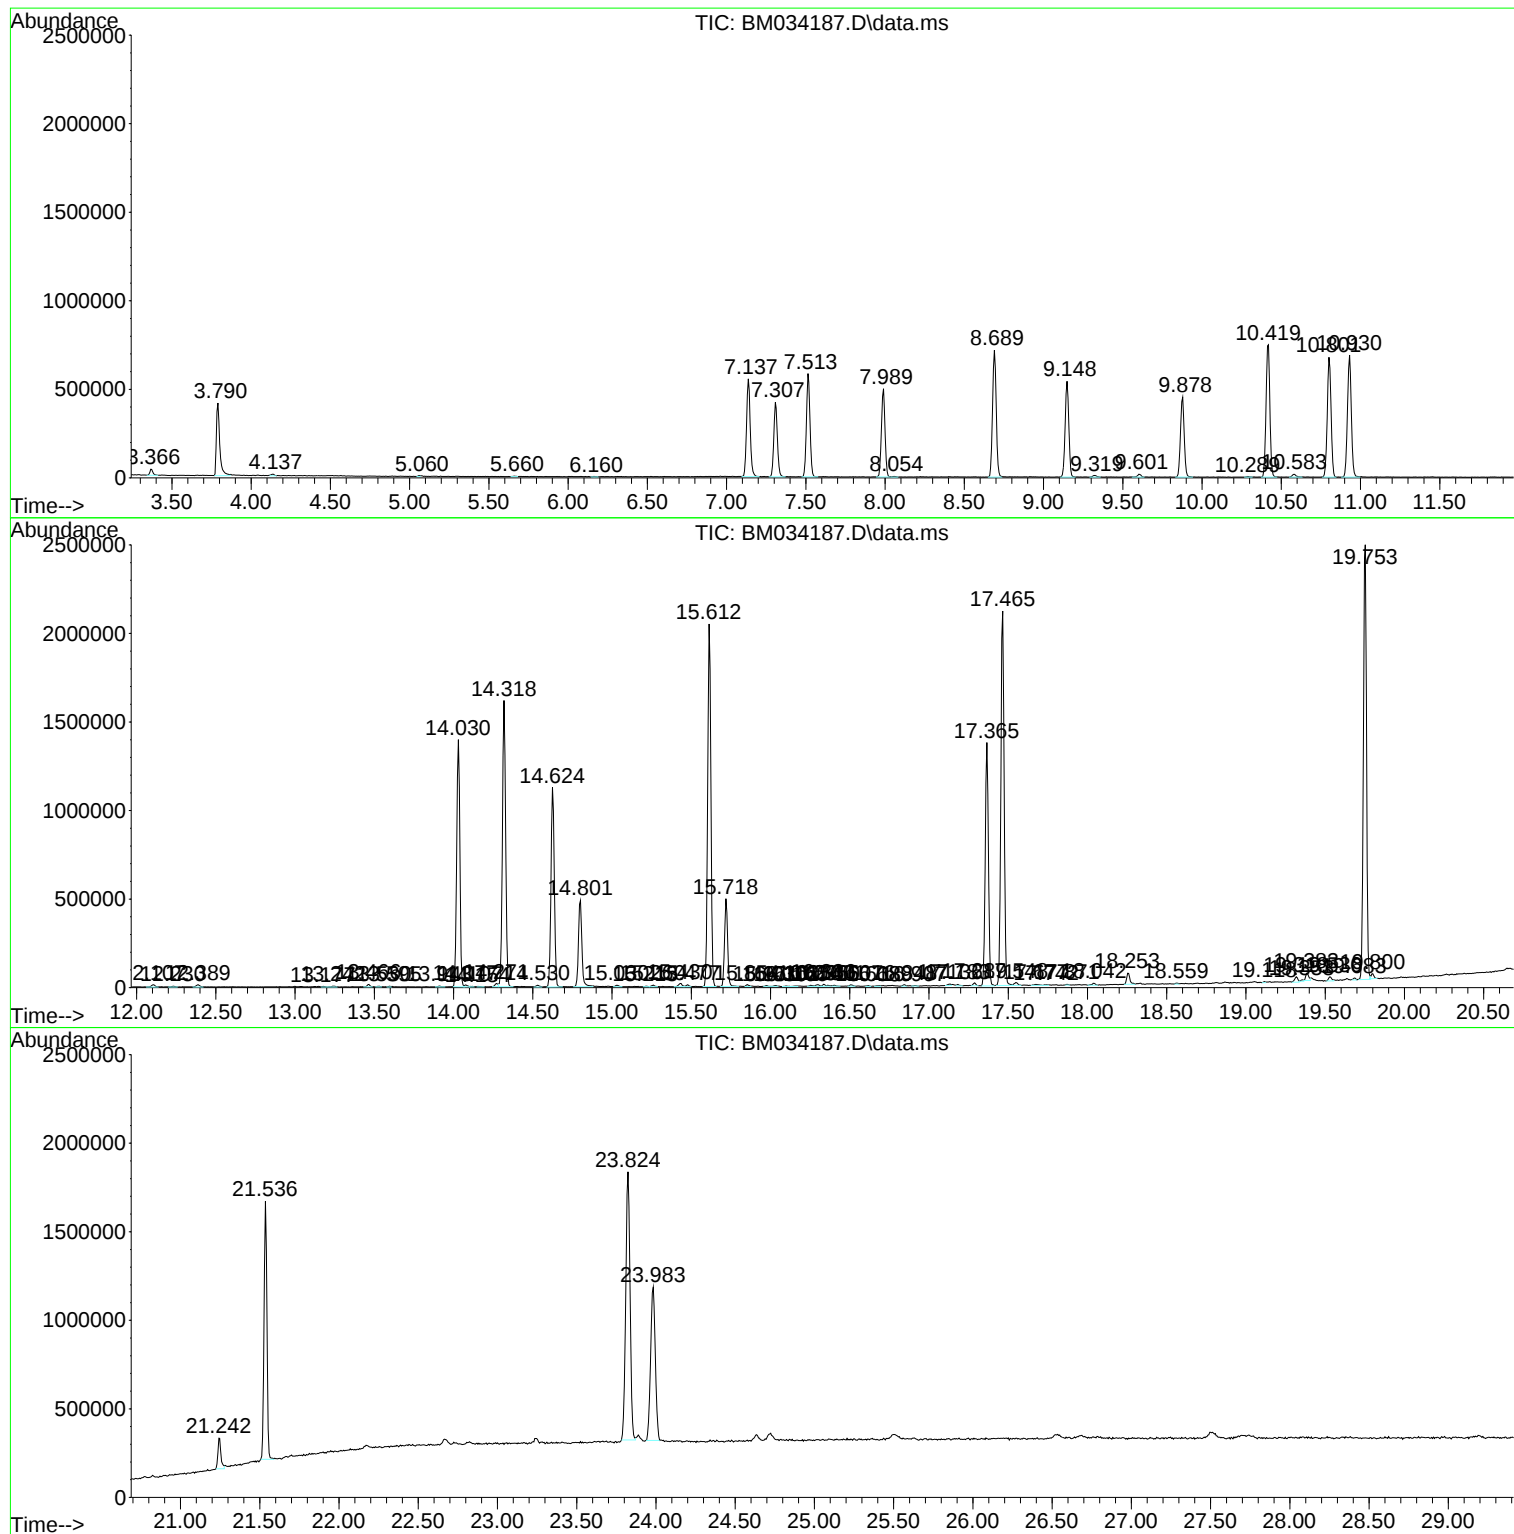

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034187.D
Acq On : 09 Mar 2022 15:45
Operator : CG/JU
Sample : N1775-03
Misc :
ALS Vial : 46 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
DBRU9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.241	2.57 ng/ul	233646	Chrysene-d12		21.536	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Nonadecene		266	C19H38	018435-45-5	98
2	n-Tetracosanol-1		354	C24H50O	000506-51-4	95
3	1-Heneicosanol		312	C21H44O	015594-90-8	95
4	Behenic alcohol		326	C22H46O	000661-19-8	95
5	Trifluoroacetic acid, pentadecyl...		324	C17H31F3O2	959010-23-2	94

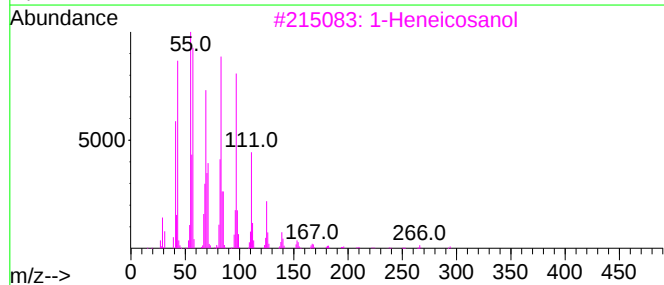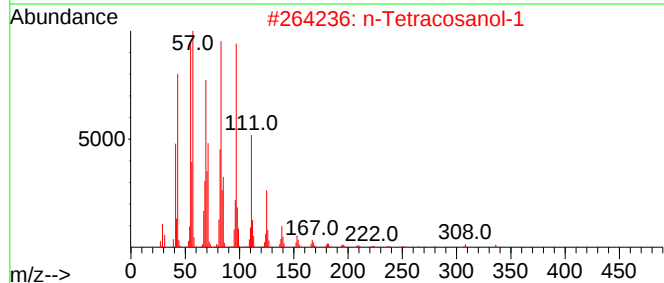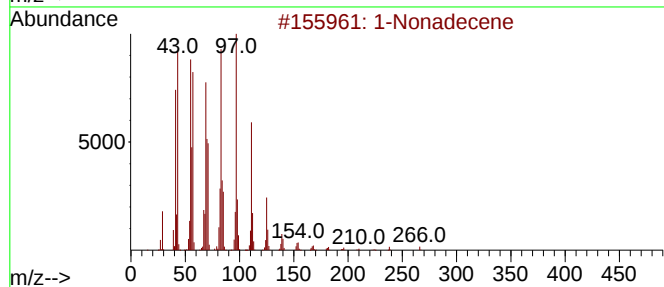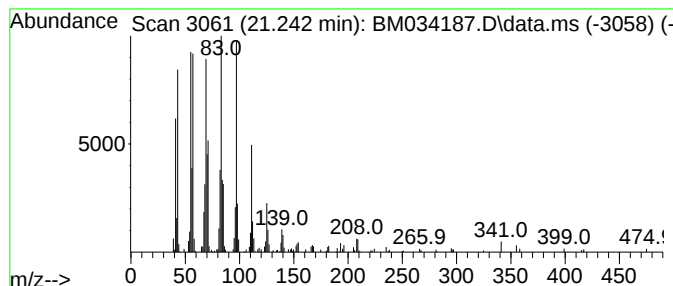

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034187.D
Acq On : 09 Mar 2022 15:45
Operator : CG/JU
Sample : N1775-03
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRU9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.241	2.6	ng/u1	233646	5	21.536	1817470	20.0