

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034189.D
 Acq On : 09 Mar 2022 16:57
 Operator : CG/JU
 Sample : N1775-06
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRV2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	19	23	28	rBV	19970	26299	1.28%	0.109%
2	3.796	92	95	108	rBV	73768	118419	5.76%	0.490%
3	4.090	143	145	147	rBV2	2641	2570	0.12%	0.011%
4	4.137	149	153	158	rVB	8420	13618	0.66%	0.056%
5	4.302	178	181	182	rBV2	1688	2110	0.10%	0.009%
6	4.760	256	259	261	rBV3	2273	2515	0.12%	0.010%
7	5.054	308	309	312	rBV3	2084	2291	0.11%	0.009%
8	5.284	344	348	349	rBV3	2077	2069	0.10%	0.009%
9	5.849	441	444	450	rBV5	1423	2251	0.11%	0.009%
10	6.684	584	586	590	rBV4	1468	2193	0.11%	0.009%
11	6.843	611	613	617	rBV5	2046	2494	0.12%	0.010%
12	7.137	656	663	676	rVB	325816	500004	24.31%	2.067%
13	7.219	676	677	683	rVB6	1850	2143	0.10%	0.009%
14	7.307	686	692	701	rBV	248133	392199	19.07%	1.621%
15	7.513	721	727	734	rBV	335293	527705	25.66%	2.181%
16	7.625	744	746	751	rVB2	1925	2528	0.12%	0.010%
17	7.660	751	752	755	rBV3	1779	2061	0.10%	0.009%
18	7.990	799	808	816	rBV	495940	796591	38.73%	3.293%
19	8.054	816	819	825	rVB5	2444	3800	0.18%	0.016%
20	8.690	920	927	936	rBV	415184	648341	31.52%	2.680%
21	8.754	936	938	941	rVB3	1849	2140	0.10%	0.009%
22	9.148	998	1005	1014	rVV	322598	522749	25.42%	2.161%
23	9.607	1077	1083	1088	rVB4	9124	16590	0.81%	0.069%
24	9.878	1122	1129	1137	rVB	212639	356022	17.31%	1.472%
25	10.413	1213	1220	1231	rBV	423349	709502	34.50%	2.933%
26	10.801	1278	1286	1293	rBV	676552	1134547	55.16%	4.690%
27	10.931	1300	1308	1320	rBV	399738	680800	33.10%	2.814%
28	11.842	1461	1463	1468	rVV4	1601	2324	0.11%	0.010%
29	12.230	1525	1529	1533	rBV3	5547	7080	0.34%	0.029%
30	12.389	1550	1556	1565	rVB5	8445	14092	0.69%	0.058%
31	12.972	1651	1655	1660	rBV4	1207	2561	0.12%	0.011%
32	13.036	1663	1666	1671	rVB6	1801	2189	0.11%	0.009%
33	13.119	1678	1680	1685	rVB5	1753	2177	0.11%	0.009%
34	13.466	1733	1739	1745	rBV2	13106	19118	0.93%	0.079%
35	13.595	1757	1761	1765	rBV6	2405	3388	0.16%	0.014%
36	14.030	1829	1835	1841	rVV	788973	1059573	51.52%	4.380%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034189.D
 Acq On : 09 Mar 2022 16:57
 Operator : CG/JU
 Sample : N1775-06
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRV2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

37	14.077	1841	1843	1845	rVV3	4037	3954	0.19%	0.016%
38	14.107	1845	1848	1852	rVB5	2149	3827	0.19%	0.016%
39	14.272	1873	1876	1877	rBV2	3486	3057	0.15%	0.013%
40	14.319	1877	1884	1891	rVV	974805	1384536	67.32%	5.723%
41	14.530	1912	1920	1924	rBV5	5331	9340	0.45%	0.039%
42	14.624	1929	1936	1946	rVB	1163772	1674979	81.44%	6.924%
43	14.795	1957	1965	1976	rBV	217209	342175	16.64%	1.414%
44	15.419	2067	2071	2072	rBV4	1753	2096	0.10%	0.009%
45	15.436	2072	2074	2077	rVV3	4074	4700	0.23%	0.019%
46	15.471	2077	2080	2085	rVB6	3238	4618	0.22%	0.019%
47	15.613	2098	2104	2112	rVB	1286318	1789000	86.98%	7.395%
48	15.718	2117	2122	2132	rBV	167705	233728	11.36%	0.966%
49	15.854	2142	2145	2149	rVB4	5635	7662	0.37%	0.032%
50	16.254	2209	2213	2216	rBV5	1285	2103	0.10%	0.009%
51	16.289	2216	2219	2221	rBV4	1832	2066	0.10%	0.009%
52	16.618	2270	2275	2277	rBV5	1729	3089	0.15%	0.013%
53	16.771	2298	2301	2304	rVB5	3138	3789	0.18%	0.016%
54	16.836	2310	2312	2317	rVB6	2392	3019	0.15%	0.012%
55	17.148	2363	2365	2370	rVB3	4263	5746	0.28%	0.024%
56	17.236	2376	2380	2384	rBV5	2524	4196	0.20%	0.017%
57	17.365	2395	2402	2408	rBV	1422759	1956994	95.15%	8.090%
58	17.465	2412	2419	2428	rVV	1311578	1897676	92.27%	7.845%
59	17.554	2431	2434	2436	rVB3	5141	5456	0.27%	0.023%
60	17.683	2454	2456	2459	rBV4	2393	2607	0.13%	0.011%
61	17.830	2478	2481	2484	rBV5	1415	2508	0.12%	0.010%
62	18.254	2550	2553	2560	rVB8	16781	23925	1.16%	0.099%
63	18.883	2659	2660	2665	rVB5	2888	3046	0.15%	0.013%
64	19.118	2698	2700	2702	rBV2	3504	3032	0.15%	0.013%
65	19.318	2730	2734	2738	rBV4	15083	20428	0.99%	0.084%
66	19.383	2743	2745	2748	rVV2	14058	15448	0.75%	0.064%
67	19.748	2801	2807	2814	rBV	1522335	2056708	100.00%	8.502%
68	21.242	3058	3061	3066	rBV3	63001	77564	3.77%	0.321%
69	21.536	3106	3111	3120	rBV	1384835	1751447	85.16%	7.240%
70	23.824	3493	3500	3507	rVB	818021	1611548	78.36%	6.662%
71	23.977	3520	3526	3536	rVB2	816725	1687997	82.07%	6.978%




Sum of corrected areas: 24191117

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034189.D
Acq On : 09 Mar 2022 16:57
Operator : CG/JU
Sample : N1775-06
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRV2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

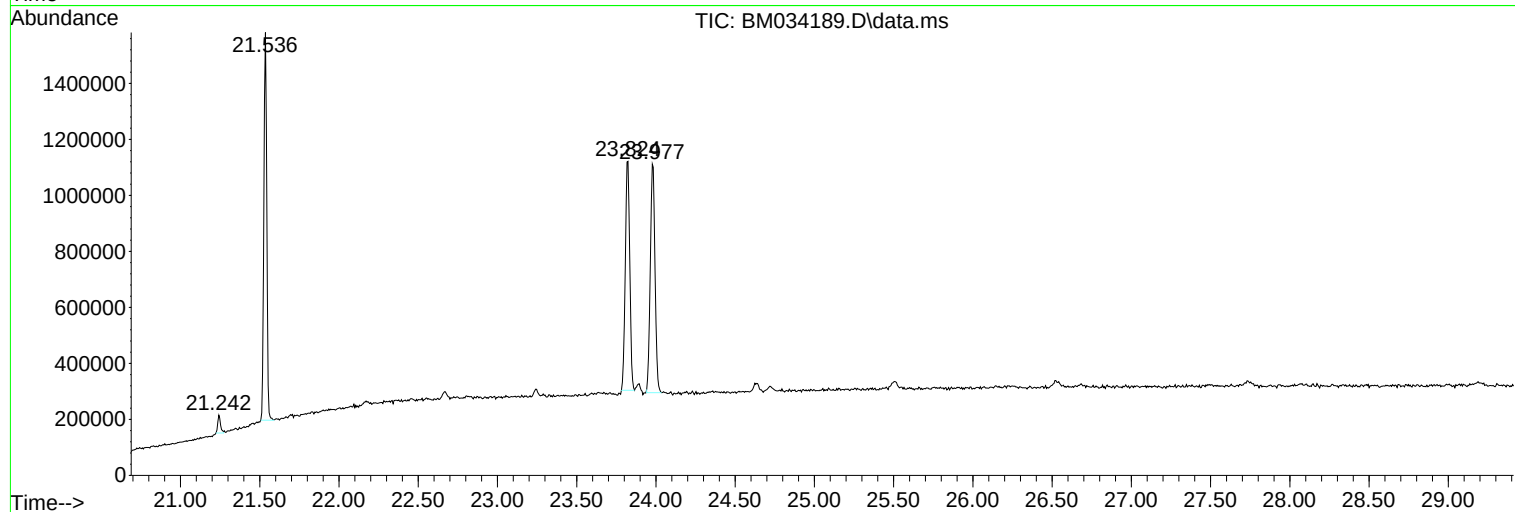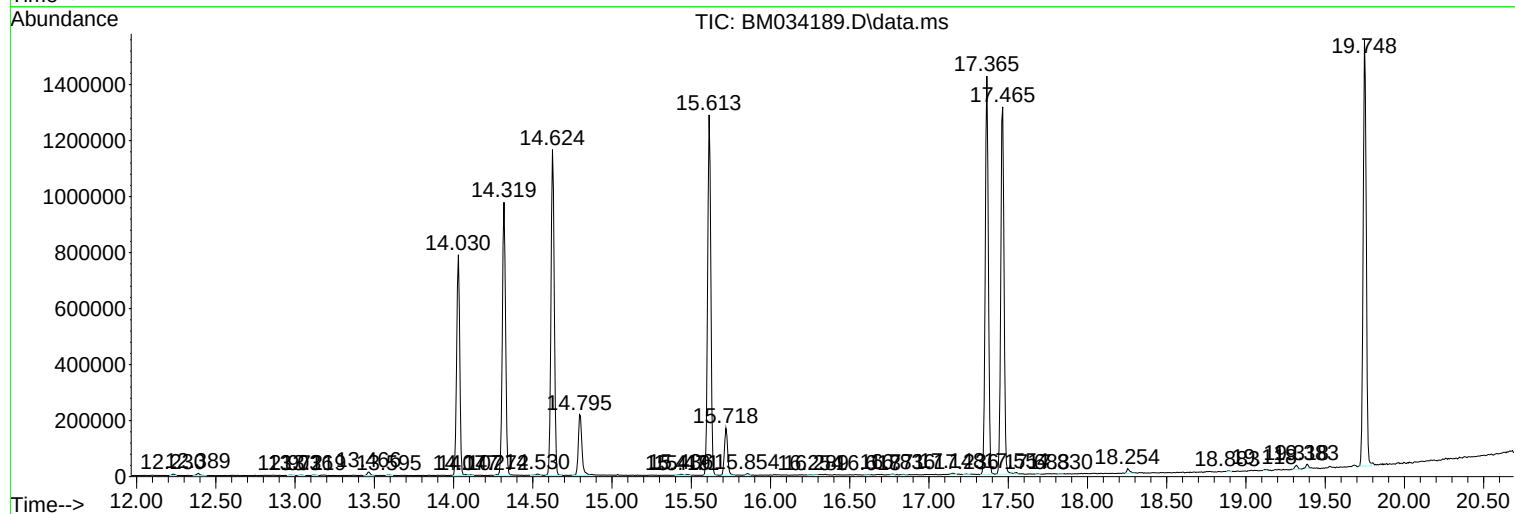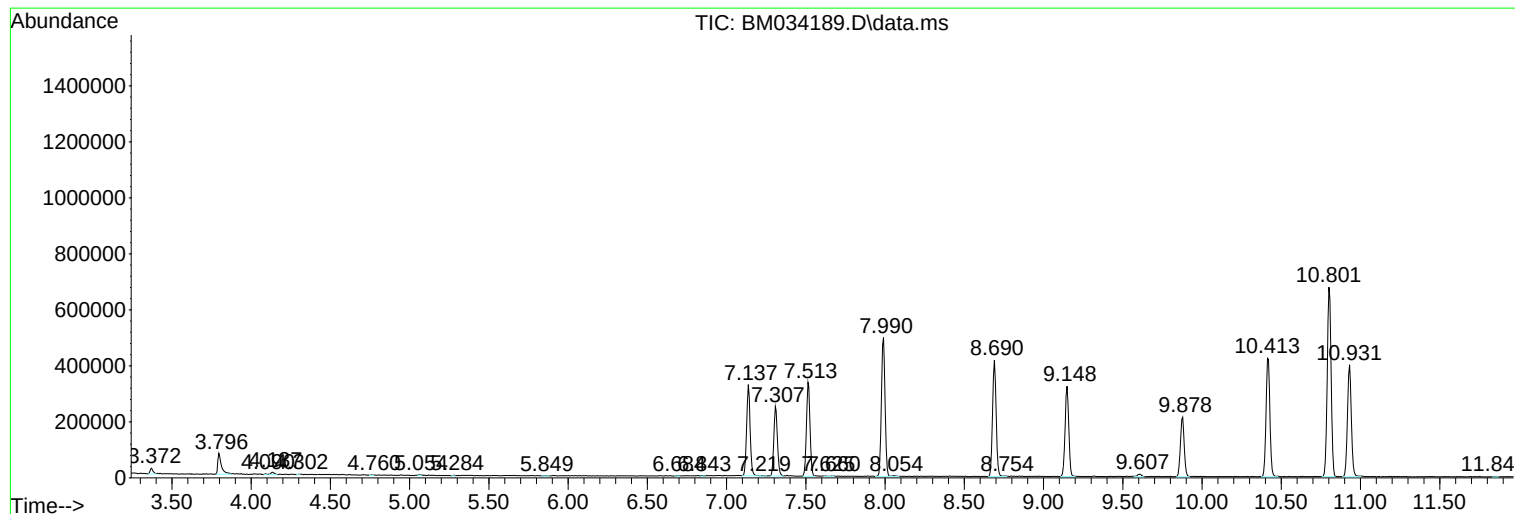

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034189.D
Acq On : 09 Mar 2022 16:57
Operator : CG/JU
Sample : N1775-06
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRV2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034189.D
Acq On : 09 Mar 2022 16:57
Operator : CG/JU
Sample : N1775-06
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRV2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------