

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034192.D
 Acq On : 09 Mar 2022 18:46
 Operator : CG/JU
 Sample : N1775-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRU8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	19	23	29	rBV	37002	48558	1.19%	0.120%
2	3.790	91	94	109	rBV	228826	351826	8.61%	0.867%
3	4.037	134	136	143	rVB7	4002	7344	0.18%	0.018%
4	4.137	149	153	158	rVB	9828	14147	0.35%	0.035%
5	5.066	308	311	314	rBV4	3694	4678	0.11%	0.012%
6	7.137	656	663	678	rVB	592109	953991	23.33%	2.351%
7	7.307	686	692	702	rVB	458071	711903	17.41%	1.755%
8	7.513	720	727	737	rBV	624641	970784	23.74%	2.393%
9	7.990	801	808	816	rVB	526018	844121	20.65%	2.081%
10	8.689	919	927	942	rBV	779827	1228006	30.03%	3.027%
11	9.148	998	1005	1016	rVB	583160	946393	23.15%	2.333%
12	9.319	1029	1034	1040	rVB6	8338	13954	0.34%	0.034%
13	9.601	1077	1082	1087	rVB3	12129	18558	0.45%	0.046%
14	9.878	1121	1129	1140	rVB	486806	803015	19.64%	1.979%
15	10.413	1213	1220	1234	rBV	802518	1340873	32.80%	3.305%
16	10.583	1242	1249	1255	rBV4	10742	21148	0.52%	0.052%
17	10.801	1278	1286	1294	rBV	734982	1220053	29.84%	3.007%
18	10.930	1300	1308	1323	rBV	768898	1289681	31.54%	3.179%
19	12.230	1526	1529	1534	rVB4	5203	5765	0.14%	0.014%
20	12.389	1550	1556	1561	rVB2	14182	22068	0.54%	0.054%
21	13.242	1697	1701	1707	rVB5	5078	6920	0.17%	0.017%
22	13.460	1733	1738	1742	rBV	13295	19530	0.48%	0.048%
23	13.530	1745	1750	1754	rVB5	5415	8962	0.22%	0.022%
24	13.601	1757	1762	1764	rBV4	4167	5718	0.14%	0.014%
25	14.030	1829	1835	1841	rBV	1616499	2135334	52.23%	5.263%
26	14.083	1841	1844	1847	rVV6	7285	8641	0.21%	0.021%
27	14.271	1870	1876	1878	rBV	21955	30370	0.74%	0.075%
28	14.319	1878	1884	1897	rVB	1781803	2553990	62.47%	6.295%
29	14.530	1915	1920	1924	rBV5	8783	11449	0.28%	0.028%
30	14.624	1930	1936	1945	rVB	1268299	1827675	44.70%	4.505%
31	14.801	1956	1966	1981	rBV	618797	925116	22.63%	2.280%
32	15.030	2001	2005	2010	rVB5	6724	8823	0.22%	0.022%
33	15.260	2039	2044	2048	rVB	8103	12100	0.30%	0.030%
34	15.430	2069	2073	2078	rBV3	18903	30327	0.74%	0.075%
35	15.477	2078	2081	2085	rVB3	8659	10787	0.26%	0.027%
36	15.613	2097	2104	2111	rBV	2356548	3250516	79.50%	8.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034192.D
 Acq On : 09 Mar 2022 18:46
 Operator : CG/JU
 Sample : N1775-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRU8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

37	15.718	2117	2122	2136	rBV	556467	750176	18.35%	1.849%
38	15.854	2141	2145	2154	rBV6	11685	20583	0.50%	0.051%
39	15.971	2161	2165	2169	rVB7	5893	8427	0.21%	0.021%
40	16.030	2169	2175	2178	rBV7	6374	10711	0.26%	0.026%
41	16.260	2210	2214	2216	rBV4	5227	7544	0.18%	0.019%
42	16.295	2216	2220	2224	rVV5	9244	12554	0.31%	0.031%
43	16.336	2224	2227	2230	rBV2	8543	10568	0.26%	0.026%
44	16.395	2235	2237	2245	rVB7	6454	11942	0.29%	0.029%
45	16.507	2251	2256	2260	rBV4	10039	15572	0.38%	0.038%
46	16.607	2270	2273	2279	rVB6	4001	5650	0.14%	0.014%
47	16.677	2279	2285	2289	rBV6	5900	10397	0.25%	0.026%
48	16.848	2309	2314	2317	rBV7	7730	11349	0.28%	0.028%
49	17.130	2357	2362	2369	rBV4	11576	26142	0.64%	0.064%
50	17.177	2369	2370	2377	rVB6	5904	7300	0.18%	0.018%
51	17.289	2385	2389	2394	rVB4	18934	24378	0.60%	0.060%
52	17.365	2395	2402	2408	rVV	1617113	2224576	54.41%	5.483%
53	17.465	2412	2419	2430	rVV	2507935	3545629	86.72%	8.740%
54	17.548	2430	2433	2437	rVB5	10471	14566	0.36%	0.036%
55	17.677	2449	2455	2457	rBV7	4716	8260	0.20%	0.020%
56	17.742	2462	2466	2468	rBV4	6276	6298	0.15%	0.016%
57	18.036	2511	2516	2521	rBV5	14048	20152	0.49%	0.050%
58	18.254	2549	2553	2560	rBV2	56045	78805	1.93%	0.194%
59	18.330	2562	2566	2572	rVB	10945	17676	0.43%	0.044%
60	18.448	2584	2586	2589	rBV4	3216	4494	0.11%	0.011%
61	18.812	2646	2648	2651	rBV4	4178	4899	0.12%	0.012%
62	18.865	2654	2657	2664	rVV8	7404	14184	0.35%	0.035%
63	19.318	2729	2734	2738	rBV3	34132	49777	1.22%	0.123%
64	19.353	2738	2740	2742	rVV3	9045	8170	0.20%	0.020%
65	19.383	2742	2745	2749	rVV	29130	36442	0.89%	0.090%
66	19.530	2767	2770	2775	rVB6	15347	15987	0.39%	0.039%
67	19.748	2801	2807	2815	rBV	2957498	4088597	100.00%	10.078%
68	21.242	3057	3061	3066	rBV	235115	281376	6.88%	0.694%
69	21.536	3106	3111	3118	rBV	1789224	2235300	54.67%	5.510%
70	23.824	3493	3500	3507	rBV	1655888	3233555	79.09%	7.970%
71	23.977	3519	3526	3538	rBV2	1025854	2084983	51.00%	5.139%



Sum of corrected areas: 40570143

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034192.D
Acq On : 09 Mar 2022 18:46
Operator : CG/JU
Sample : N1775-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRU8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

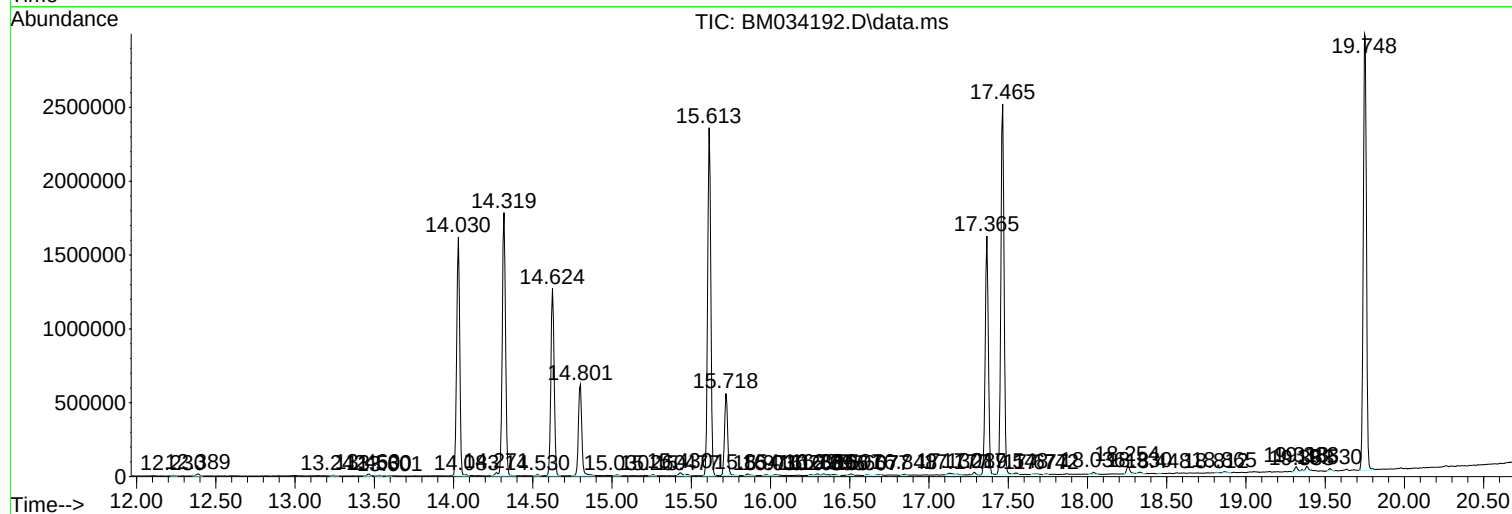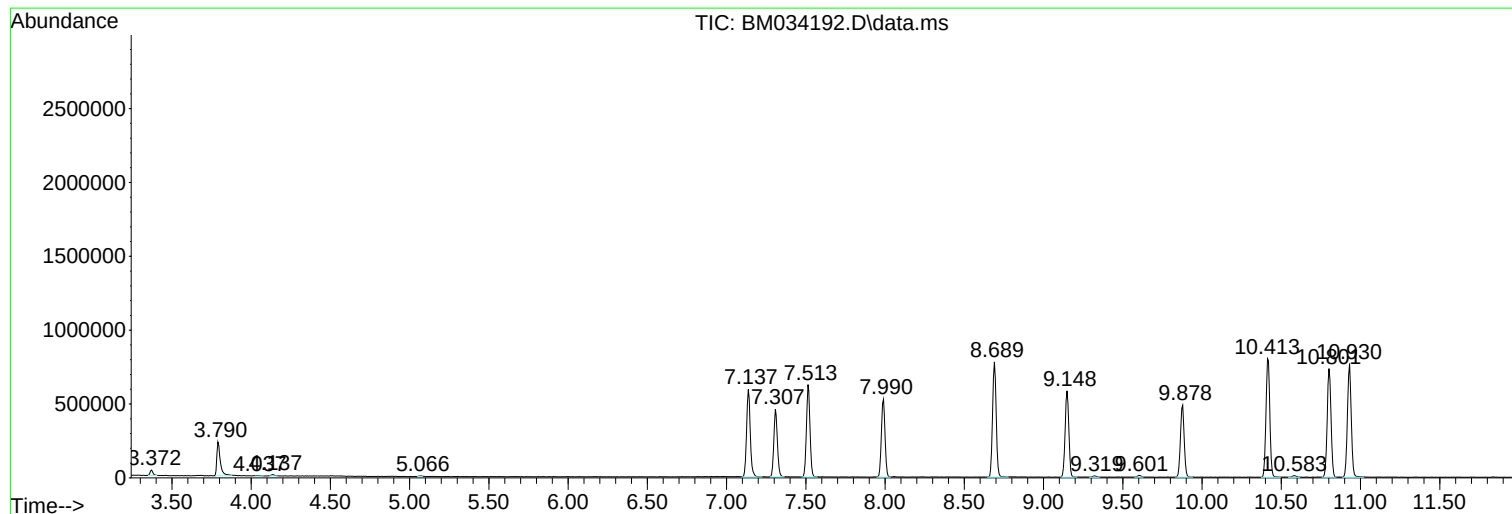

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034192.D
Acq On : 09 Mar 2022 18:46
Operator : CG/JU
Sample : N1775-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRU8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.242	2.52 ng/ul	281376	Chrysene-d12	21.536

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Nonadecene			266	C19H38	018435-45-5	99
2	1-Nonadecene			266	C19H38	018435-45-5	99
3	n-Nonadecanol-1			284	C19H40O	001454-84-8	95
4	n-Tetracosanol-1			354	C24H50O	000506-51-4	95
5	1-Heptacosanol			396	C27H56O	002004-39-9	95

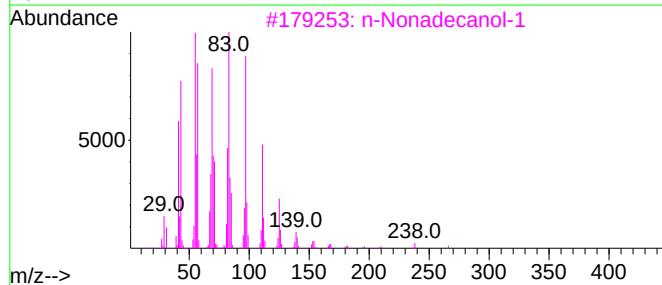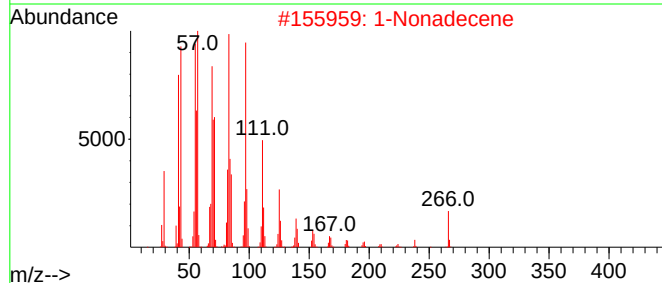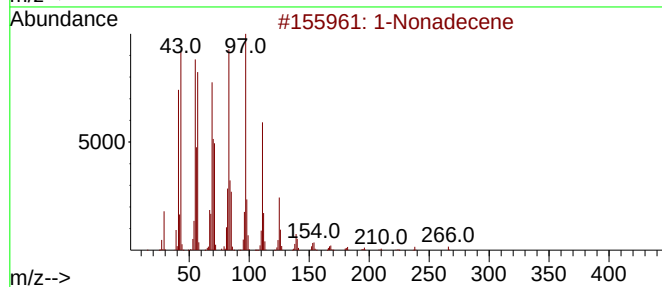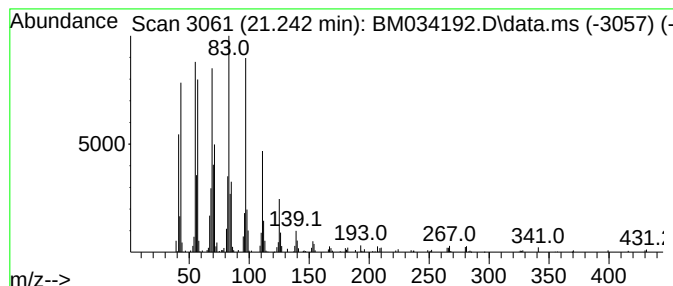

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034192.D
Acq On : 09 Mar 2022 18:46
Operator : CG/JU
Sample : N1775-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRU8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.242	2.5	ng/u1	281376	5	21.536	2235300	20.0