

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034193.D
 Acq On : 09 Mar 2022 19:22
 Operator : CG/JU
 Sample : N1775-21
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034193.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	19	23	27	rBV	25317	32493	1.00%	0.095%
2	3.790	91	94	105	rBV	179186	269814	8.34%	0.786%
3	4.131	150	152	158	rVB2	7810	10550	0.33%	0.031%
4	5.060	307	310	316	rVB6	3283	6092	0.19%	0.018%
5	5.654	406	411	413	rBV4	2497	3417	0.11%	0.010%
6	7.137	656	663	677	rVB	511629	797528	24.66%	2.323%
7	7.307	686	692	701	rBV	395440	616967	19.08%	1.797%
8	7.384	701	705	710	rVB2	5287	8323	0.26%	0.024%
9	7.513	720	727	736	rBV	528816	823347	25.46%	2.398%
10	7.990	801	808	816	rBV	516824	807415	24.96%	2.352%
11	8.054	816	819	824	rVB5	4178	6516	0.20%	0.019%
12	8.689	921	927	938	rBV	677812	1058938	32.74%	3.084%
13	9.148	997	1005	1016	rVB	522386	835291	25.83%	2.433%
14	9.325	1030	1035	1041	rVB5	3625	6038	0.19%	0.018%
15	9.607	1077	1083	1088	rVB	18458	28242	0.87%	0.082%
16	9.878	1119	1129	1143	rVB	398866	665684	20.58%	1.939%
17	10.413	1213	1220	1230	rBV	699656	1159804	35.86%	3.378%
18	10.589	1245	1250	1255	rBV3	6289	12548	0.39%	0.037%
19	10.801	1278	1286	1294	rVB	690703	1155571	35.73%	3.366%
20	10.931	1300	1308	1320	rBV	660781	1115021	34.48%	3.248%
21	12.230	1523	1529	1536	rVB6	7184	11115	0.34%	0.032%
22	12.389	1550	1556	1562	rVB	12806	21093	0.65%	0.061%
23	12.860	1632	1636	1639	rBV5	2023	3400	0.11%	0.010%
24	13.036	1663	1666	1669	rVB4	3097	4135	0.13%	0.012%
25	13.124	1678	1681	1687	rBV6	2698	4419	0.14%	0.013%
26	13.183	1687	1691	1692	rBV3	3413	3327	0.10%	0.010%
27	13.236	1697	1700	1706	rVB6	2729	5211	0.16%	0.015%
28	13.466	1733	1739	1745	rBV	19828	29322	0.91%	0.085%
29	13.524	1745	1749	1752	rBV3	4506	6440	0.20%	0.019%
30	13.595	1757	1761	1764	rBV5	3068	3978	0.12%	0.012%
31	14.030	1826	1835	1841	rBV	1340070	1785706	55.21%	5.201%
32	14.113	1847	1849	1853	rVV3	2417	3278	0.10%	0.010%
33	14.148	1853	1855	1860	rVB6	3599	5859	0.18%	0.017%
34	14.271	1872	1876	1877	rVV4	6922	8800	0.27%	0.026%
35	14.319	1877	1884	1895	rVB	1574896	2268907	70.15%	6.608%
36	14.530	1916	1920	1925	rBV3	10226	13325	0.41%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034193.D
 Acq On : 09 Mar 2022 19:22
 Operator : CG/JU
 Sample : N1775-21
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

37	14.624	1929	1936	1945	rVV	1165195	1693804	52.37%	4.933%
38	14.795	1959	1965	1979	rBV	488450	733211	22.67%	2.136%
39	15.030	2001	2005	2011	rVV6	5427	9212	0.28%	0.027%
40	15.254	2039	2043	2048	rVB4	4166	6708	0.21%	0.020%
41	15.430	2067	2073	2077	rBV6	8850	15529	0.48%	0.045%
42	15.477	2077	2081	2085	rVB7	6894	9523	0.29%	0.028%
43	15.613	2098	2104	2111	rBV	2076972	2860414	88.44%	8.331%
44	15.718	2116	2122	2130	rBV	428969	575068	17.78%	1.675%
45	15.848	2141	2144	2149	rBV5	8662	13874	0.43%	0.040%
46	15.971	2162	2165	2170	rVB6	3063	4817	0.15%	0.014%
47	16.030	2170	2175	2180	rBV6	4088	6950	0.21%	0.020%
48	16.295	2216	2220	2224	rBV5	5155	7883	0.24%	0.023%
49	16.330	2224	2226	2230	rVV4	4963	6465	0.20%	0.019%
50	16.401	2234	2238	2241	rVV4	3933	4843	0.15%	0.014%
51	16.507	2251	2256	2261	rVB7	5103	8009	0.25%	0.023%
52	16.612	2267	2274	2277	rVB8	4059	4888	0.15%	0.014%
53	16.689	2282	2287	2289	rVV5	3141	4315	0.13%	0.013%
54	16.771	2297	2301	2303	rVB5	2920	3919	0.12%	0.011%
55	16.836	2310	2312	2315	rBV4	3954	4659	0.14%	0.014%
56	17.124	2357	2361	2363	rBV5	4424	5466	0.17%	0.016%
57	17.148	2363	2365	2368	rVB	3505	3345	0.10%	0.010%
58	17.283	2385	2388	2392	rVB6	6641	8865	0.27%	0.026%
59	17.365	2395	2402	2408	rVV	1412755	1973569	61.02%	5.748%
60	17.465	2412	2419	2429	rVV	2127850	3027805	93.62%	8.819%
61	17.548	2429	2433	2439	rVB7	13718	19830	0.61%	0.058%
62	17.736	2461	2465	2470	rBV5	3437	7365	0.23%	0.021%
63	17.871	2482	2488	2491	rBV7	3783	7684	0.24%	0.022%
64	18.042	2512	2517	2521	rVB2	20915	25977	0.80%	0.076%
65	18.254	2549	2553	2562	rBV2	37052	56046	1.73%	0.163%
66	19.206	2711	2715	2720	rVB5	31389	34478	1.07%	0.100%
67	19.318	2729	2734	2738	rBV4	25898	41924	1.30%	0.122%
68	19.383	2742	2745	2753	rVV2	28748	44696	1.38%	0.130%
69	19.524	2766	2769	2776	rBV9	16247	27930	0.86%	0.081%
70	19.748	2801	2807	2813	rBV	2418266	3234284	100.00%	9.420%
71	21.242	3058	3061	3067	rBV2	112712	132471	4.10%	0.386%
72	21.536	3106	3111	3116	rBV	1396347	1746098	53.99%	5.086%
73	23.818	3492	3499	3507	rBV	1370269	2663499	82.35%	7.758%
74	23.977	3520	3526	3537	rVB2	831245	1700110	52.57%	4.952%

Sum of corrected areas: 34333447

Instrument :

BNA_M

ClientSampleId :




DBSC4

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034193.D
Acq On : 09 Mar 2022 19:22
Operator : CG/JU
Sample : N1775-21
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

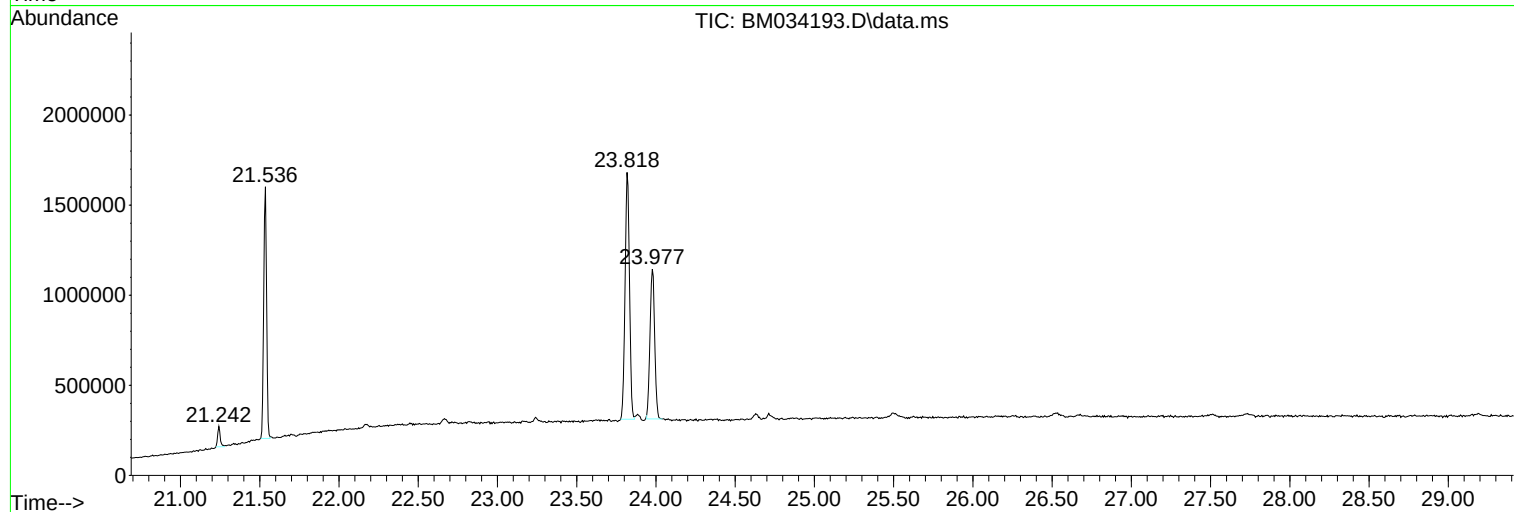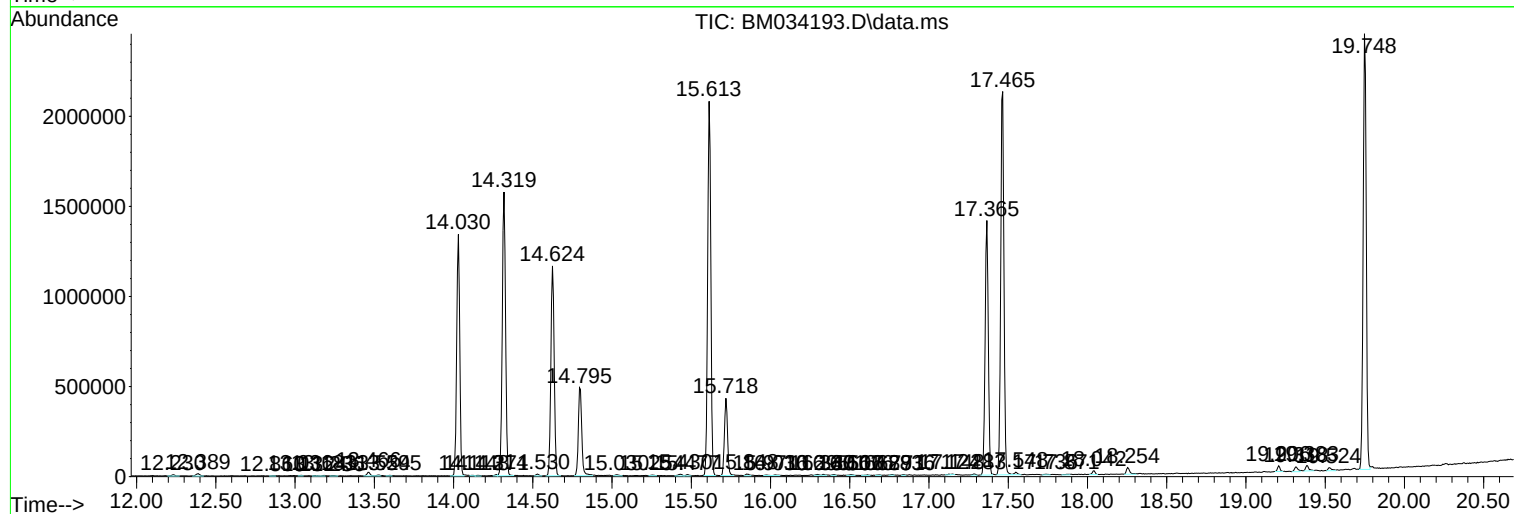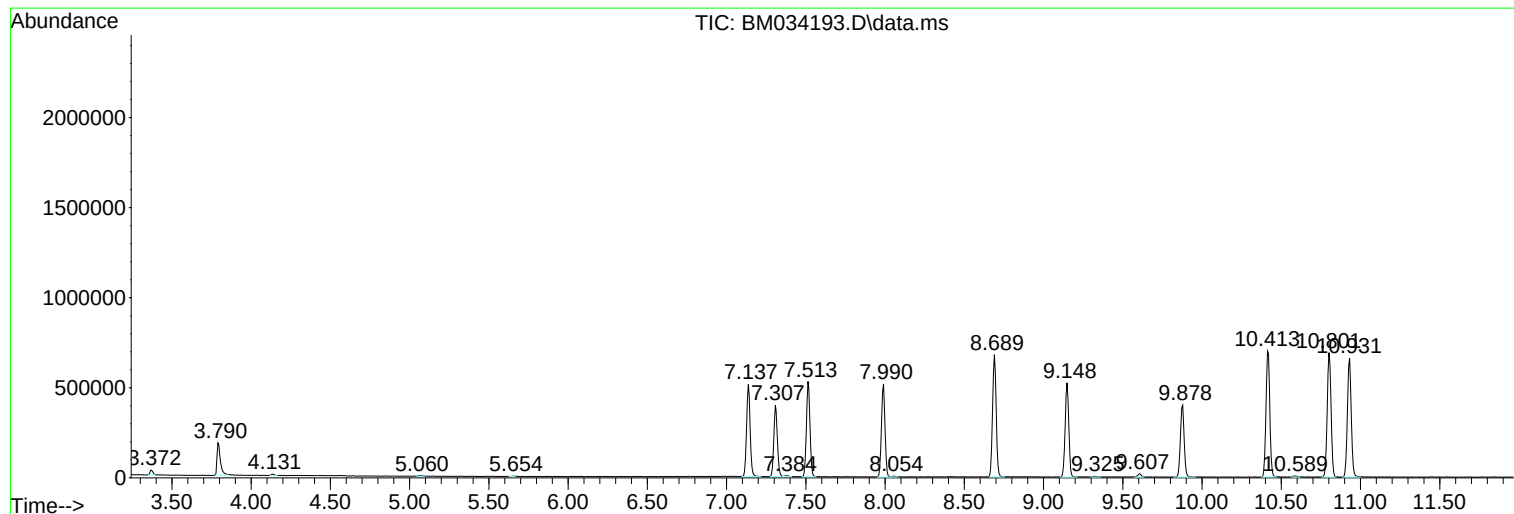

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034193.D
Acq On : 09 Mar 2022 19:22
Operator : CG/JU
Sample : N1775-21
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034193.D
Acq On : 09 Mar 2022 19:22
Operator : CG/JU
Sample : N1775-21
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------