

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034196.D
 Acq On : 09 Mar 2022 21:47
 Operator : CG/JU
 Sample : PB143147BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK147

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	18	23	29	rVB	40052	50069	1.76%	0.146%
2	3.790	90	94	108	rBV	457395	663315	23.31%	1.931%
3	4.137	149	153	158	rVB2	9105	12908	0.45%	0.038%
4	6.113	486	489	491	rBV4	2309	3019	0.11%	0.009%
5	7.137	656	663	673	rVB	579580	893528	31.39%	2.601%
6	7.307	685	692	702	rBV	450530	707596	24.86%	2.060%
7	7.513	720	727	737	rBV	614693	964637	33.89%	2.808%
8	7.989	801	808	817	rVB	538215	859132	30.19%	2.501%
9	8.689	920	927	938	rBV	746935	1176307	41.33%	3.425%
10	9.148	997	1005	1018	rVB	562803	924898	32.50%	2.693%
11	9.878	1120	1129	1141	rBV	468423	779335	27.38%	2.269%
12	10.413	1213	1220	1232	rBV	767293	1268592	44.57%	3.693%
13	10.801	1279	1286	1295	rVB	724807	1218462	42.81%	3.547%
14	10.930	1300	1308	1320	rVV	737252	1235148	43.40%	3.596%
15	11.007	1320	1321	1327	rVB5	2666	3164	0.11%	0.009%
16	12.383	1550	1555	1561	rBV2	12667	22229	0.78%	0.065%
17	13.601	1757	1762	1768	rVB6	2574	4722	0.17%	0.014%
18	14.030	1828	1835	1841	rBV	1420922	1907612	67.02%	5.554%
19	14.077	1841	1843	1850	rVB8	3403	5848	0.21%	0.017%
20	14.318	1877	1884	1893	rBV	1550436	2258229	79.34%	6.574%
21	14.624	1929	1936	1950	rVB	1194587	1698587	59.68%	4.945%
22	14.795	1959	1965	1980	rBV	518442	765976	26.91%	2.230%
23	15.436	2069	2074	2077	rBV6	2633	4095	0.14%	0.012%
24	15.612	2097	2104	2111	rBV	1978989	2752782	96.72%	8.014%
25	15.718	2116	2122	2134	rVB	507749	674203	23.69%	1.963%
26	15.854	2141	2145	2150	rVB3	8817	12674	0.45%	0.037%
27	16.595	2267	2271	2275	rBV5	1967	3267	0.11%	0.010%
28	17.148	2362	2365	2370	rVB4	4672	7608	0.27%	0.022%
29	17.365	2394	2402	2408	rBV	1247651	1778039	62.47%	5.176%
30	17.459	2411	2418	2433	rBV	1902392	2735890	96.12%	7.965%
31	18.324	2563	2565	2570	rVB6	2505	3708	0.13%	0.011%
32	18.712	2627	2631	2634	rBV5	2831	4216	0.15%	0.012%
33	19.318	2730	2734	2739	rVB3	20929	29770	1.05%	0.087%
34	19.383	2741	2745	2751	rVV2	22076	29787	1.05%	0.087%
35	19.748	2801	2807	2814	rBV	2203574	2846186	100.00%	8.286%
36	21.530	3106	3110	3116	rVB	1231061	1572885	55.26%	4.579%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034196.D
Acq On : 09 Mar 2022 21:47
Operator : CG/JU
Sample : PB143147BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK147

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Title : SVOA CALIBRATION

37	23.818	3492	3499	3506	rBV2	1395935	2736457	96.14%	7.967%
38	23.977	3519	3526	3535	rVB2	865118	1733558	60.91%	5.047%




Sum of corrected areas: 34348438

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034196.D
Acq On : 09 Mar 2022 21:47
Operator : CG/JU
Sample : PB143147BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK147

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

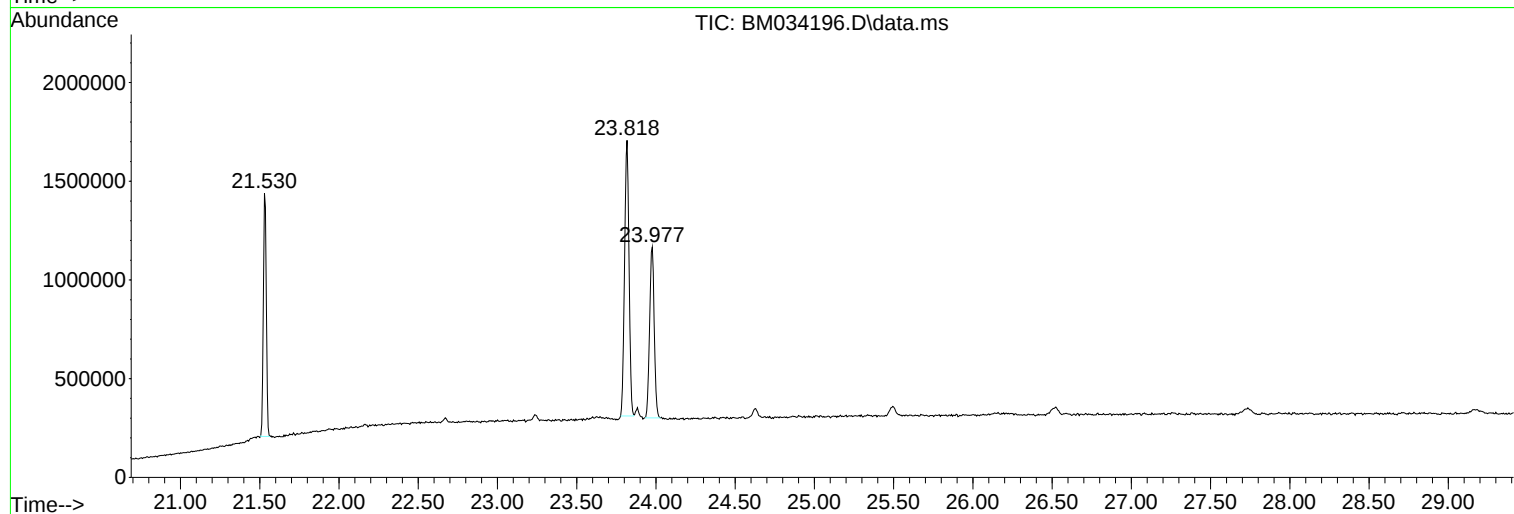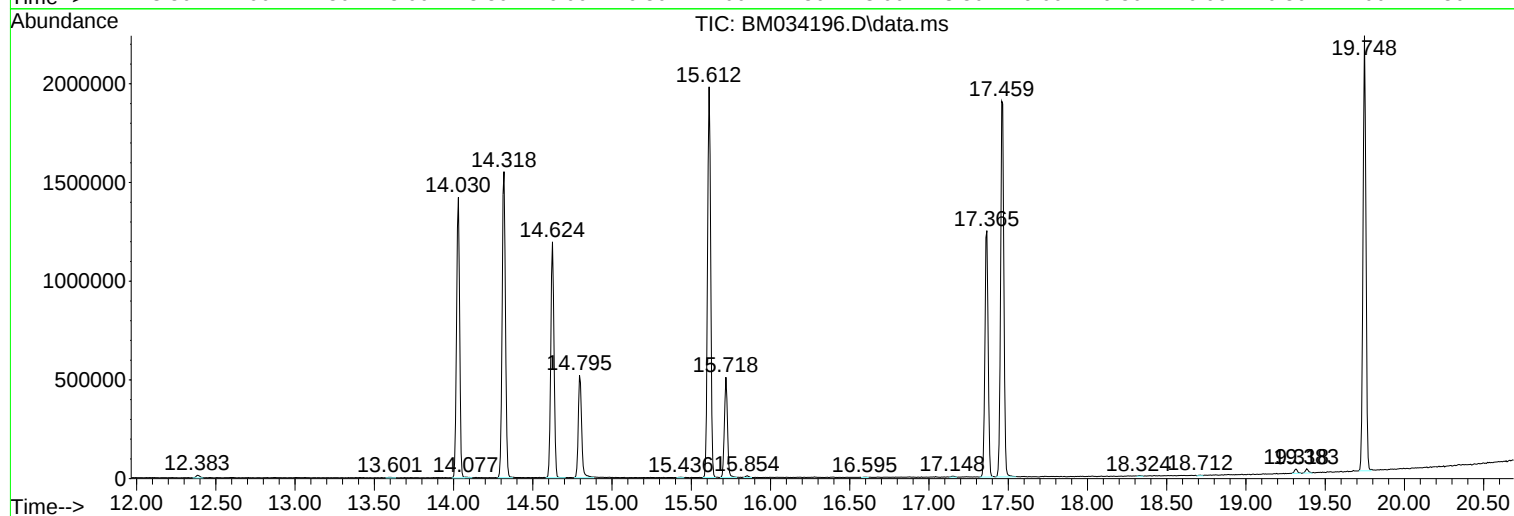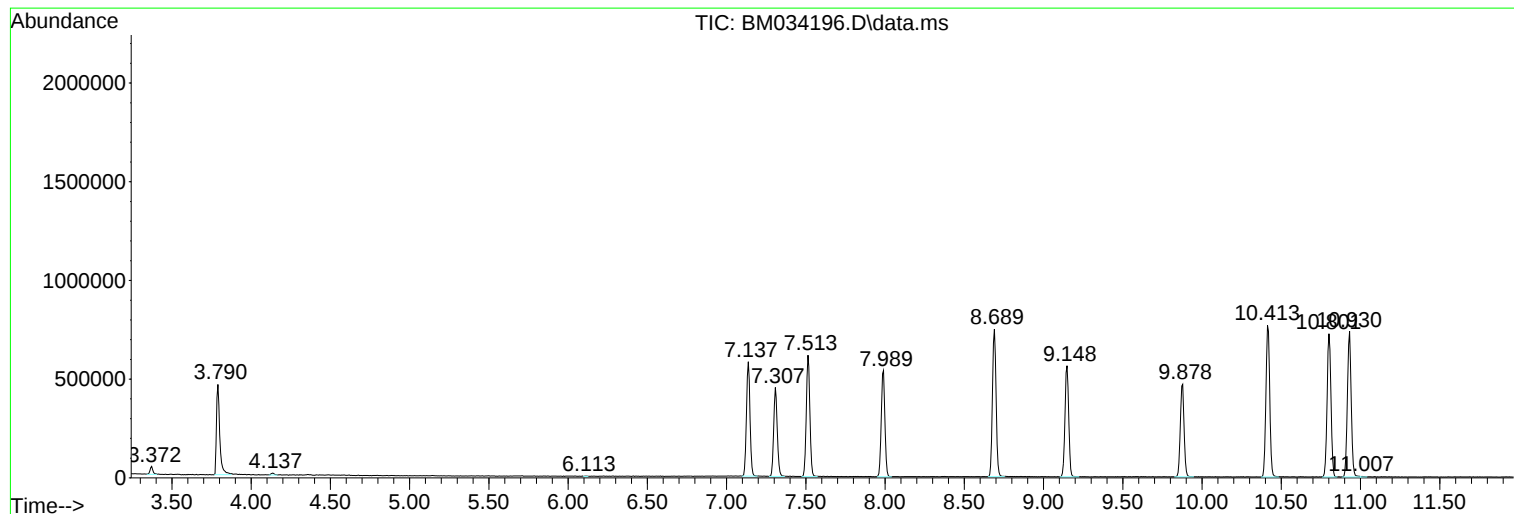

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034196.D
Acq On : 09 Mar 2022 21:47
Operator : CG/JU
Sample : PB143147BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK147

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034196.D
Acq On : 09 Mar 2022 21:47
Operator : CG/JU
Sample : PB143147BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK147

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------