

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034197.D
 Acq On : 09 Mar 2022 22:23
 Operator : CG/JU
 Sample : N1775-20
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	19	23	29	rVB	35608	48580	1.53%	0.131%
2	3.790	90	94	115	rBV	422123	622769	19.62%	1.683%
3	4.131	148	152	157	rBV	9017	13394	0.42%	0.036%
4	5.066	308	311	318	rVB6	4359	6152	0.19%	0.017%
5	5.660	408	412	417	rVB7	3256	5950	0.19%	0.016%
6	7.137	656	663	673	rVB	594439	921624	29.04%	2.491%
7	7.307	686	692	700	rBV	457467	703461	22.17%	1.902%
8	7.378	700	704	711	rVB	5474	9861	0.31%	0.027%
9	7.513	720	727	736	rVB	626527	964792	30.40%	2.608%
10	7.989	800	808	815	rBV	526528	827320	26.07%	2.236%
11	8.054	815	819	825	rVB8	3668	5660	0.18%	0.015%
12	8.689	920	927	937	rBV	782115	1227425	38.67%	3.318%
13	9.148	997	1005	1013	rBV	586554	947453	29.85%	2.561%
14	9.601	1077	1082	1087	rBV2	13146	20486	0.65%	0.055%
15	9.872	1122	1128	1142	rVB	488176	802280	25.28%	2.169%
16	10.413	1210	1220	1231	rBV	807631	1337087	42.13%	3.614%
17	10.583	1244	1249	1259	rBV4	6951	12455	0.39%	0.034%
18	10.801	1279	1286	1294	rVB	704543	1174313	37.00%	3.174%
19	10.930	1300	1308	1317	rBV	753648	1273607	40.13%	3.443%
20	12.230	1524	1529	1534	rBV4	5302	8240	0.26%	0.022%
21	12.383	1550	1555	1561	rBV	13904	21815	0.69%	0.059%
22	13.177	1687	1690	1694	rBV5	3493	5075	0.16%	0.014%
23	13.242	1696	1701	1705	rVB4	2474	4048	0.13%	0.011%
24	13.460	1733	1738	1744	rBV	14645	21359	0.67%	0.058%
25	13.601	1758	1762	1766	rBV5	3203	5114	0.16%	0.014%
26	14.030	1828	1835	1842	rBV	1528131	2073576	65.34%	5.605%
27	14.077	1842	1843	1848	rVV5	5753	6944	0.22%	0.019%
28	14.154	1852	1856	1861	rVB7	3425	5310	0.17%	0.014%
29	14.271	1871	1876	1877	rBV4	6272	7351	0.23%	0.020%
30	14.318	1877	1884	1892	rVB	1684522	2437966	76.82%	6.590%
31	14.530	1915	1920	1923	rVB4	8276	10135	0.32%	0.027%
32	14.624	1929	1936	1943	rBV	1138991	1655322	52.16%	4.475%
33	14.795	1954	1965	1985	rBV	548837	825051	26.00%	2.230%
34	14.983	1993	1997	2000	rVB4	2919	4338	0.14%	0.012%
35	15.030	2000	2005	2009	rBV7	4969	8681	0.27%	0.023%
36	15.148	2022	2025	2031	rVB6	2302	4788	0.15%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034197.D
 Acq On : 09 Mar 2022 22:23
 Operator : CG/JU
 Sample : N1775-20
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

37	15.254	2039	2043	2048	rVB3	4565	6407	0.20%	0.017%
38	15.430	2068	2073	2077	rBV5	7504	12342	0.39%	0.033%
39	15.477	2077	2081	2085	rVB5	6685	7338	0.23%	0.020%
40	15.612	2094	2104	2112	rBV	2201620	3036651	95.68%	8.209%
41	15.718	2116	2122	2130	rBV	550777	725699	22.87%	1.962%
42	15.848	2139	2144	2149	rBV3	9498	13625	0.43%	0.037%
43	16.295	2215	2220	2224	rVV7	5086	9568	0.30%	0.026%
44	16.336	2224	2227	2230	rVV5	4767	6079	0.19%	0.016%
45	16.395	2234	2237	2242	rVB6	4084	7126	0.22%	0.019%
46	16.512	2252	2257	2260	rVB6	3823	5333	0.17%	0.014%
47	16.677	2280	2285	2288	rBV5	3049	5243	0.17%	0.014%
48	16.765	2297	2300	2303	rBV5	3286	4293	0.14%	0.012%
49	17.036	2343	2346	2349	rBV5	3264	3722	0.12%	0.010%
50	17.124	2358	2361	2363	rBV4	4373	5849	0.18%	0.016%
51	17.148	2363	2365	2370	rVB	4142	5348	0.17%	0.014%
52	17.283	2384	2388	2392	rVB7	4971	6778	0.21%	0.018%
53	17.365	2395	2402	2408	rVV	1299755	1824120	57.48%	4.931%
54	17.459	2411	2418	2430	rBV	2130978	3066514	96.62%	8.289%
55	17.548	2430	2433	2438	rVB6	10365	15431	0.49%	0.042%
56	17.918	2493	2496	2498	rBV4	2708	3276	0.10%	0.009%
57	18.036	2513	2516	2522	rVB5	9077	10827	0.34%	0.029%
58	18.253	2549	2553	2562	rBV	104841	140591	4.43%	0.380%
59	19.312	2729	2733	2737	rBV3	26356	35553	1.12%	0.096%
60	19.383	2741	2745	2753	rVB2	33158	55754	1.76%	0.151%
61	19.530	2766	2770	2773	rBV4	23371	32158	1.01%	0.087%
62	19.748	2801	2807	2813	rBV	2435925	3173717	100.00%	8.579%
63	21.242	3057	3061	3069	rBV2	240653	326896	10.30%	0.884%
64	21.530	3105	3110	3117	rBV	1269838	1666781	52.52%	4.506%
65	23.818	3492	3499	3507	rBV2	1528864	2985908	94.08%	8.071%
66	23.977	3519	3526	3536	rVB2	874830	1764817	55.61%	4.771%




Sum of corrected areas: 36993526

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034197.D
Acq On : 09 Mar 2022 22:23
Operator : CG/JU
Sample : N1775-20
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

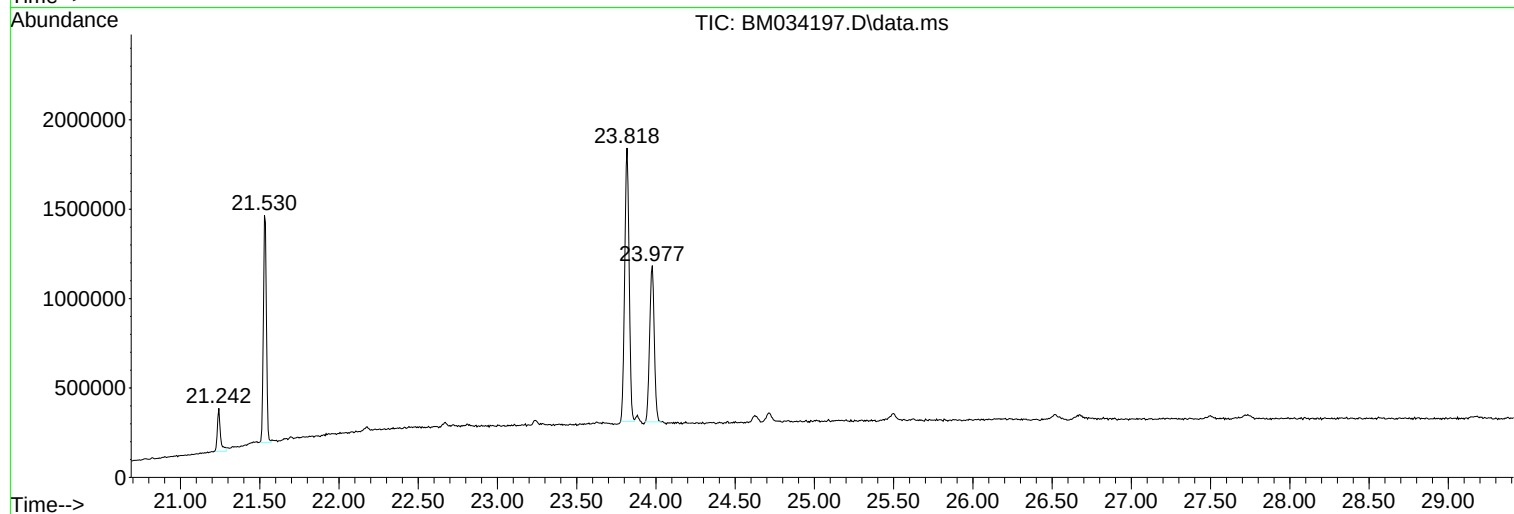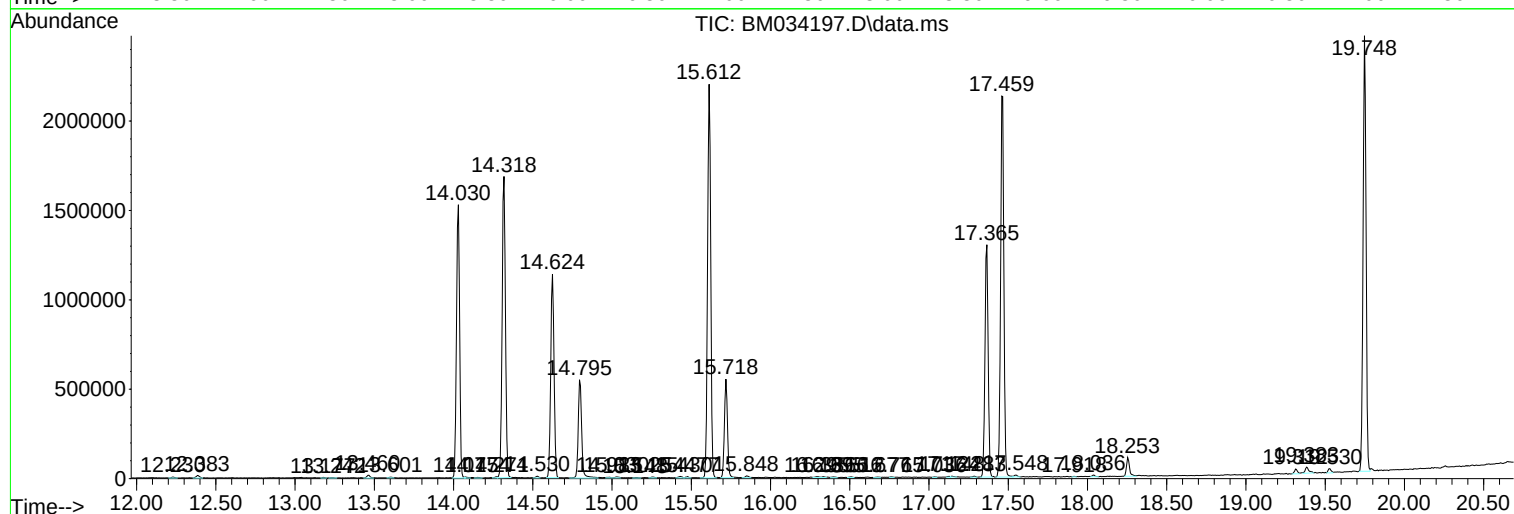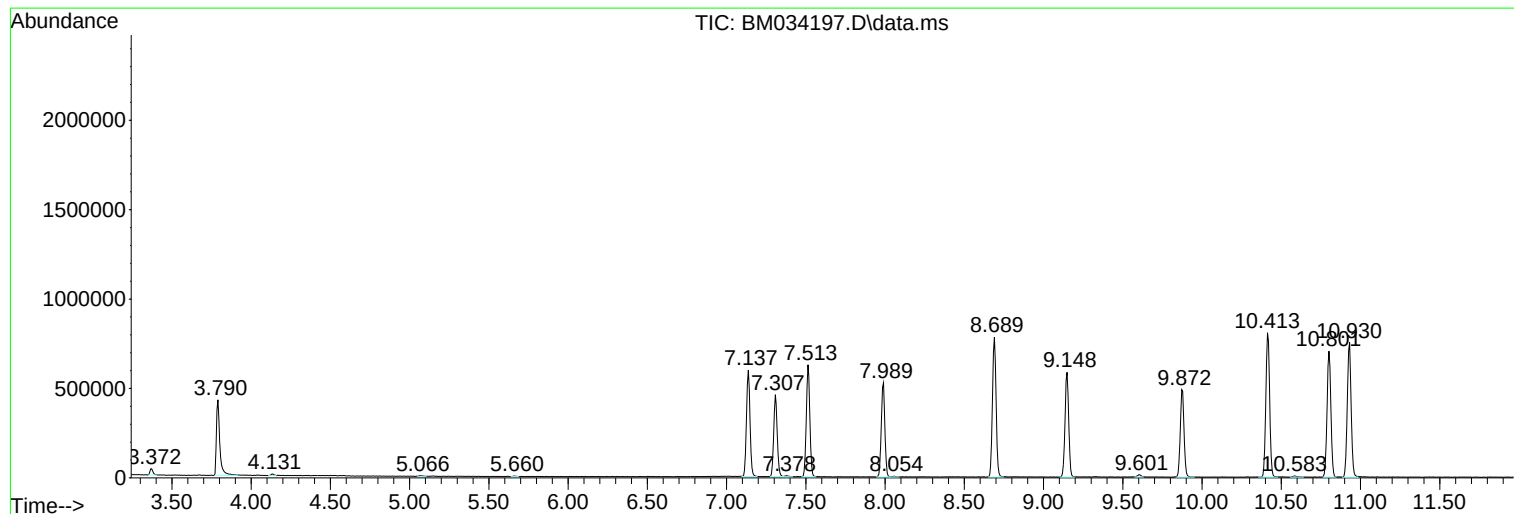

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034197.D
Acq On : 09 Mar 2022 22:23
Operator : CG/JU
Sample : N1775-20
Misc :
ALS Vial : 57 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
DBSC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.241	3.92 ng/ul	326896	Chrysene-d12		21.530	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Hexacosene		364	C26H52	018835-33-1	95
2	Behenic alcohol		326	C22H46O	000661-19-8	95
3	1-Tetracosene		336	C24H48	010192-32-2	95
4	n-Tetracosanol-1		354	C24H50O	000506-51-4	94
5	n-Nonadecanol-1		284	C19H40O	001454-84-8	94

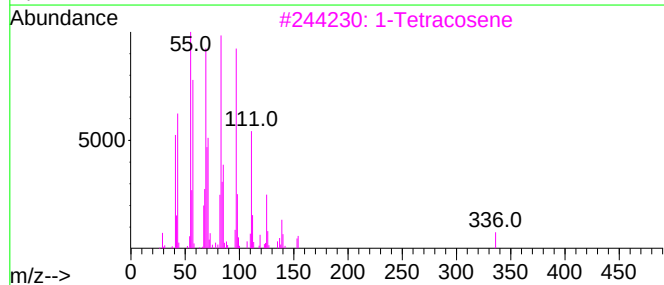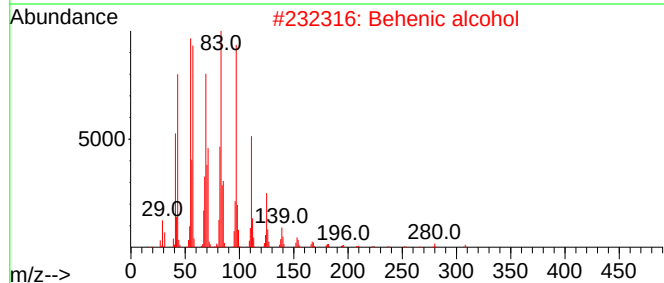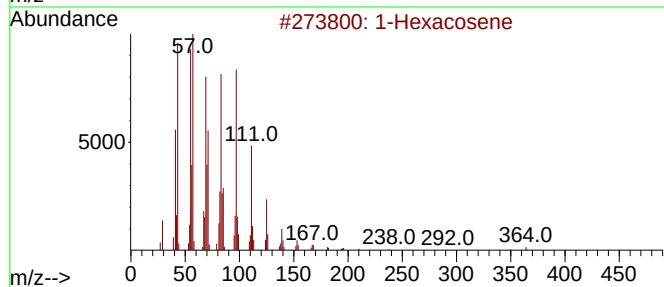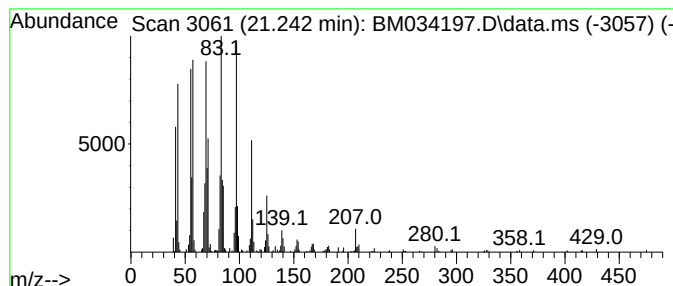

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034197.D
Acq On : 09 Mar 2022 22:23
Operator : CG/JU
Sample : N1775-20
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.241	3.9	ng/u1	326896	5	21.530	1666780	20.0