

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034198.D
 Acq On : 09 Mar 2022 23:00
 Operator : CG/JU
 Sample : N1775-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRV0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	19	23	28	rVB	17606	23695	1.00%	0.092%
2	3.725	81	83	85	rBV3	2218	2664	0.11%	0.010%
3	3.796	92	95	106	rBV	68005	110121	4.66%	0.427%
4	4.137	149	153	159	rVB	8227	13357	0.57%	0.052%
5	5.207	331	335	338	rBV6	1598	2544	0.11%	0.010%
6	5.449	372	376	378	rBV6	2064	2897	0.12%	0.011%
7	7.137	657	663	676	rVB	391671	624431	26.44%	2.424%
8	7.307	686	692	702	rBV	362589	562641	23.83%	2.184%
9	7.513	720	727	736	rBV	419716	649821	27.52%	2.522%
10	7.984	800	807	815	rBV	502585	813232	34.44%	3.157%
11	8.048	815	818	823	rVB3	2213	3147	0.13%	0.012%
12	8.689	920	927	936	rBV	510453	813495	34.45%	3.158%
13	9.148	998	1005	1012	rBV	432184	717219	30.37%	2.784%
14	9.601	1076	1082	1088	rVB4	9447	13972	0.59%	0.054%
15	9.872	1121	1128	1138	rBV	116761	195972	8.30%	0.761%
16	10.413	1212	1220	1231	rBV	504680	818436	34.66%	3.177%
17	10.801	1278	1286	1297	rVB	693096	1154925	48.91%	4.483%
18	10.931	1299	1308	1316	rBV	218339	383667	16.25%	1.489%
19	11.595	1417	1421	1424	rBV4	1465	2378	0.10%	0.009%
20	12.230	1526	1529	1532	rBV4	2979	3666	0.16%	0.014%
21	12.389	1548	1556	1562	rBV2	10406	19572	0.83%	0.076%
22	13.042	1662	1667	1673	rVB7	1485	2446	0.10%	0.009%
23	13.466	1733	1739	1744	rBV3	8737	12747	0.54%	0.049%
24	14.024	1828	1834	1840	rBV	363231	492031	20.84%	1.910%
25	14.071	1840	1842	1847	rVB6	2517	3408	0.14%	0.013%
26	14.271	1870	1876	1877	rBV5	9390	11484	0.49%	0.045%
27	14.319	1877	1884	1895	rVB	1297260	1870948	79.23%	7.262%
28	14.524	1915	1919	1926	rBV4	6670	11077	0.47%	0.043%
29	14.624	1929	1936	1946	rVV	1110056	1635452	69.26%	6.348%
30	14.795	1960	1965	1974	rBV	108858	178487	7.56%	0.693%
31	14.971	1991	1995	1996	rBV3	1868	2430	0.10%	0.009%
32	15.266	2041	2045	2047	rVB4	1879	2772	0.12%	0.011%
33	15.430	2068	2073	2076	rBV5	3357	5929	0.25%	0.023%
34	15.477	2078	2081	2083	rVV2	5120	4296	0.18%	0.017%
35	15.613	2096	2104	2112	rBV	1647764	2327074	98.55%	9.033%
36	15.718	2116	2122	2130	rBV	68608	94686	4.01%	0.368%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034198.D
 Acq On : 09 Mar 2022 23:00
 Operator : CG/JU
 Sample : N1775-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBRV0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

37	15.783	2130	2133	2137	rVB5	1785	2623	0.11%	0.010%
38	15.854	2137	2145	2148	rBV5	6978	10965	0.46%	0.043%
39	16.024	2172	2174	2178	rVB4	3683	4118	0.17%	0.016%
40	16.101	2184	2187	2190	rBV5	1703	2887	0.12%	0.011%
41	16.248	2207	2212	2215	rVB5	2799	3270	0.14%	0.013%
42	16.295	2215	2220	2223	rBV7	3022	4925	0.21%	0.019%
43	16.336	2223	2227	2229	rVV4	4391	5245	0.22%	0.020%
44	16.401	2236	2238	2243	rVB6	2704	3161	0.13%	0.012%
45	16.512	2252	2257	2261	rBV5	5052	8052	0.34%	0.031%
46	16.618	2270	2275	2277	rBV5	1949	3535	0.15%	0.014%
47	16.677	2280	2285	2287	rBV5	2928	4608	0.20%	0.018%
48	16.836	2309	2312	2314	rBV4	3051	3769	0.16%	0.015%
49	17.130	2352	2362	2369	rBV6	7672	23730	1.00%	0.092%
50	17.177	2369	2370	2375	rVB5	5694	4956	0.21%	0.019%
51	17.283	2385	2388	2392	rVB6	5642	7285	0.31%	0.028%
52	17.365	2395	2402	2408	rVV	1221546	1766035	74.79%	6.855%
53	17.460	2412	2418	2429	rVV	1668156	2312750	97.94%	8.977%
54	17.665	2448	2453	2454	rBV4	2578	3197	0.14%	0.012%
55	17.748	2462	2467	2471	rBV8	2675	5825	0.25%	0.023%
56	18.036	2512	2516	2523	rVB8	5780	7584	0.32%	0.029%
57	18.142	2530	2534	2535	rBV4	2787	3239	0.14%	0.013%
58	18.254	2550	2553	2559	rBV7	7733	12971	0.55%	0.050%
59	18.324	2563	2565	2567	rBV3	2376	2904	0.12%	0.011%
60	18.571	2603	2607	2608	rBV4	3373	3514	0.15%	0.014%
61	19.312	2729	2733	2737	rBV2	20129	28865	1.22%	0.112%
62	19.348	2737	2739	2742	rBV4	5967	6387	0.27%	0.025%
63	19.383	2742	2745	2748	rBV	15016	20134	0.85%	0.078%
64	19.748	2801	2807	2813	rBV	1816646	2361281	100.00%	9.166%
65	21.242	3057	3061	3066	rBV3	86804	116025	4.91%	0.450%
66	21.530	3106	3110	3116	rBV	1192342	1537858	65.13%	5.969%
67	23.818	3492	3499	3507	rBV2	1135295	2217574	93.91%	8.608%
68	23.977	3519	3526	3536	rVB2	834135	1675860	70.97%	6.505%


Sum of corrected areas: 25762251

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034198.D
Acq On : 09 Mar 2022 23:00
Operator : CG/JU
Sample : N1775-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRV0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

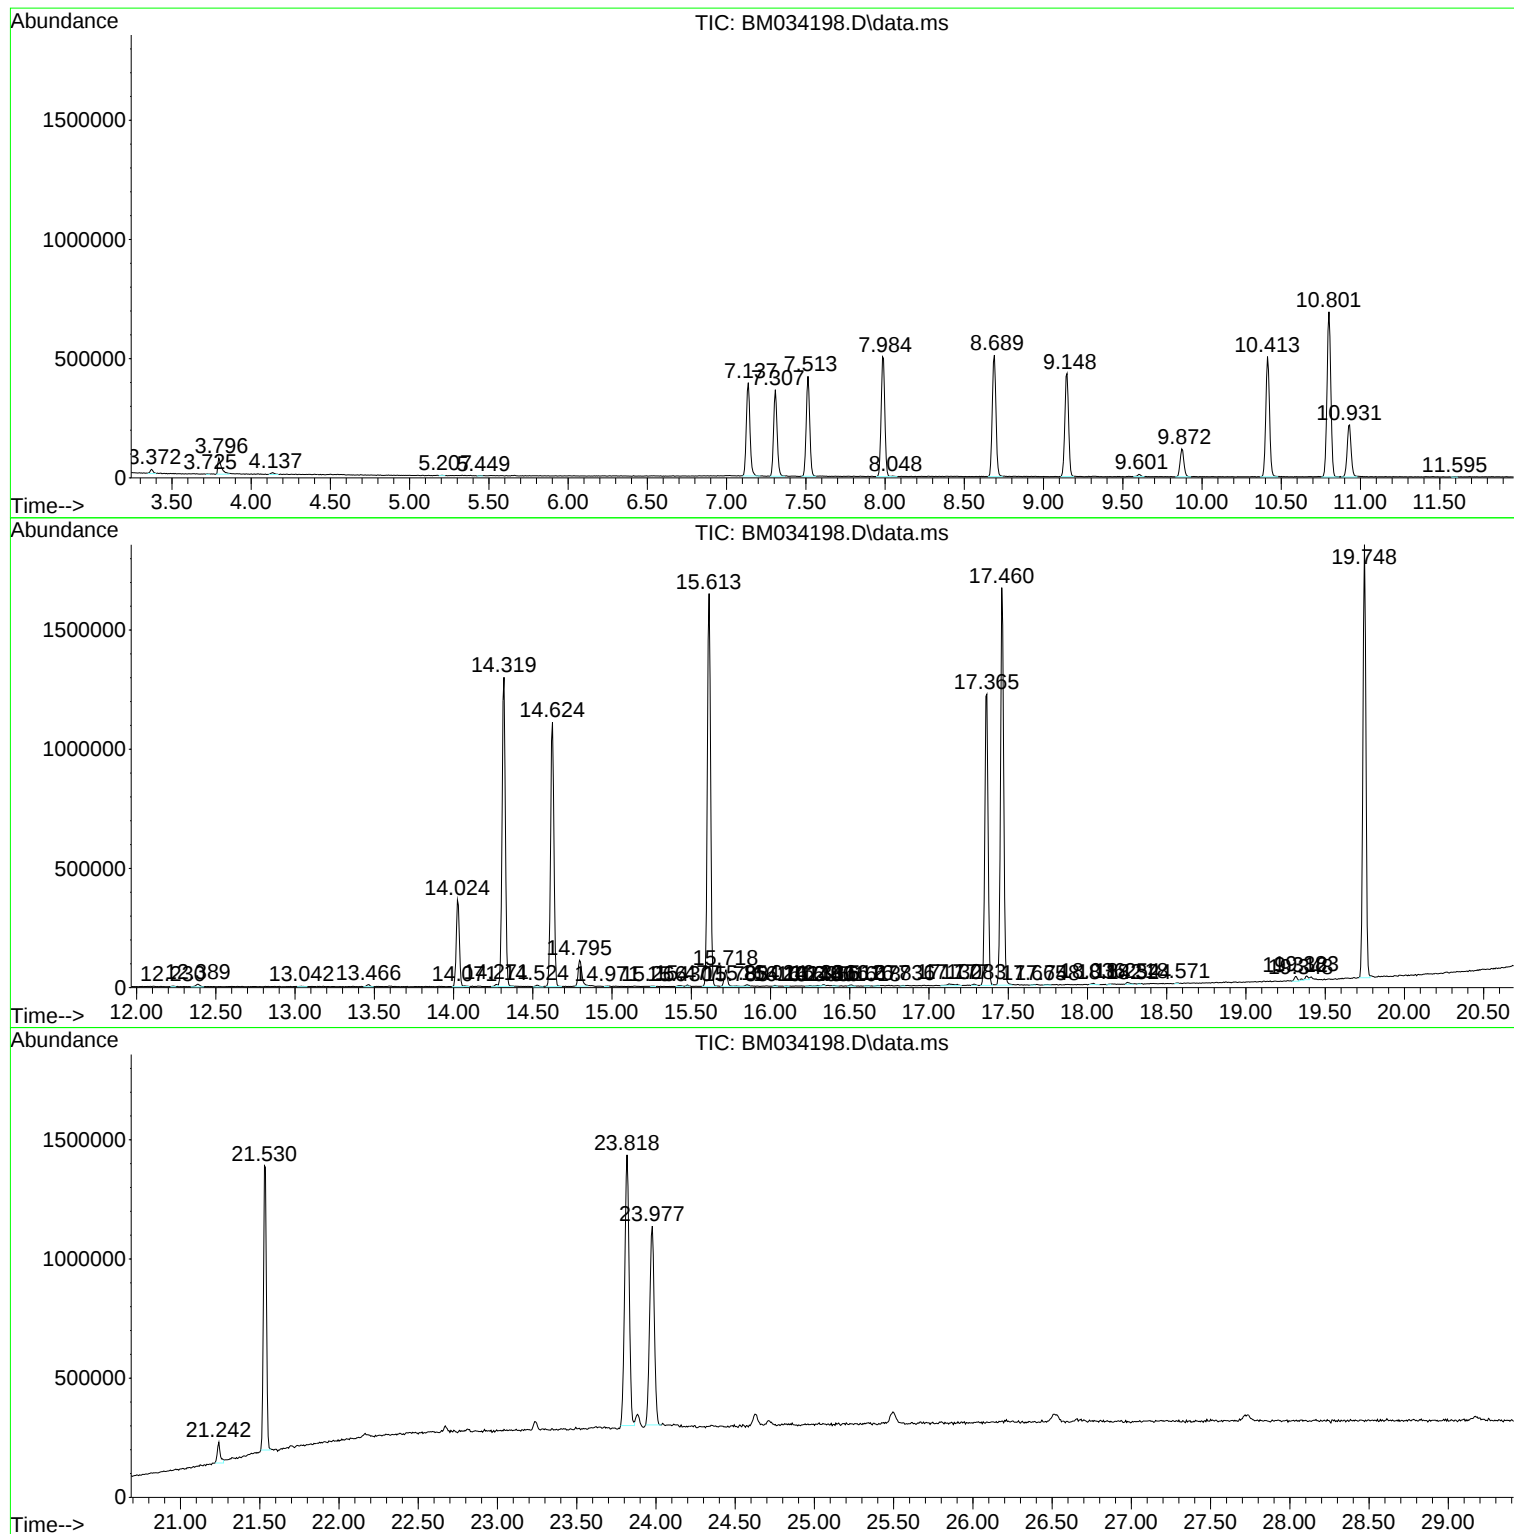

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034198.D
Acq On : 09 Mar 2022 23:00
Operator : CG/JU
Sample : N1775-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRV0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034198.D
Acq On : 09 Mar 2022 23:00
Operator : CG/JU
Sample : N1775-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBRV0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc