

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034201.D
 Acq On : 10 Mar 2022 00:48
 Operator : CG/JU
 Sample : N1775-17
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.372	19	23	31	rVB	13988	20964	1.19%	0.097%
2	3.796	91	95	109	rBV	90194	146494	8.33%	0.679%
3	4.043	133	137	140	rVB3	4791	6718	0.38%	0.031%
4	4.131	148	152	158	rVB2	7783	11479	0.65%	0.053%
5	4.219	164	167	172	rBV5	2547	4651	0.26%	0.022%
6	4.372	192	193	196	rBV2	2628	2451	0.14%	0.011%
7	4.696	246	248	252	rBV4	2495	2809	0.16%	0.013%
8	5.066	306	311	317	rBV	12947	18573	1.06%	0.086%
9	5.831	439	441	444	rBV2	2790	3045	0.17%	0.014%
10	6.407	538	539	543	rVB3	2432	2578	0.15%	0.012%
11	6.472	547	550	554	rVB5	1222	2002	0.11%	0.009%
12	6.707	588	590	594	rVB4	1808	2077	0.12%	0.010%
13	6.996	632	639	640	rBV6	4112	7034	0.40%	0.033%
14	7.137	656	663	673	rVB	246439	399633	22.73%	1.851%
15	7.307	686	692	700	rBV	196539	307764	17.50%	1.426%
16	7.513	720	727	736	rVB	265772	408065	23.21%	1.890%
17	7.619	742	745	749	rVB6	2959	3612	0.21%	0.017%
18	7.713	758	761	764	rBV5	1623	2681	0.15%	0.012%
19	7.984	801	807	815	rBV	522217	832802	47.36%	3.858%
20	8.048	817	818	824	rVV6	3018	3709	0.21%	0.017%
21	8.137	828	833	836	rBV4	1344	2445	0.14%	0.011%
22	8.301	858	861	864	rVB5	1698	2232	0.13%	0.010%
23	8.690	920	927	934	rBV	319815	512647	29.15%	2.375%
24	8.807	941	947	956	rVB	15038	26026	1.48%	0.121%
25	9.142	998	1004	1014	rBV	238090	397626	22.61%	1.842%
26	9.319	1033	1034	1038	rVB3	3329	2531	0.14%	0.012%
27	9.601	1076	1082	1087	rVB2	14588	21775	1.24%	0.101%
28	9.872	1118	1128	1136	rBV	193780	324709	18.47%	1.504%
29	10.231	1186	1189	1195	rVB4	2101	3339	0.19%	0.015%
30	10.413	1213	1220	1229	rBV	335534	546961	31.10%	2.534%
31	10.584	1247	1249	1253	rBV4	2110	3421	0.19%	0.016%
32	10.801	1279	1286	1295	rVB	716367	1179273	67.06%	5.463%
33	10.925	1300	1307	1318	rBV	280307	490591	27.90%	2.273%
34	11.331	1370	1376	1379	rBV6	1938	3448	0.20%	0.016%
35	11.607	1417	1423	1428	rBV6	1509	3630	0.21%	0.017%
36	11.672	1432	1434	1437	rVB4	1755	1926	0.11%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034201.D
 Acq On : 10 Mar 2022 00:48
 Operator : CG/JU
 Sample : N1775-17
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

37	11.707	1437	1440	1443	rBV3	1826	2217	0.13%	0.010%
38	12.230	1524	1529	1532	rVB5	3736	5307	0.30%	0.025%
39	12.383	1551	1555	1561	rVB3	6107	9418	0.54%	0.044%
40	12.566	1582	1586	1589	rBV4	1811	3251	0.18%	0.015%

41	12.995	1655	1659	1663	rBV6	2042	3556	0.20%	0.016%
42	13.183	1687	1691	1694	rBV5	1636	2408	0.14%	0.011%
43	13.242	1697	1701	1705	rVV5	3526	5097	0.29%	0.024%
44	13.460	1733	1738	1742	rBV	9563	12353	0.70%	0.057%
45	13.589	1755	1760	1763	rBV5	2193	2724	0.15%	0.013%

46	14.024	1828	1834	1841	rBV	671549	921515	52.40%	4.269%
47	14.113	1847	1849	1852	rBV4	2230	2819	0.16%	0.013%
48	14.272	1872	1876	1877	rVV2	5123	6184	0.35%	0.029%
49	14.313	1877	1883	1891	rVB	686963	1007225	57.28%	4.666%
50	14.530	1916	1920	1923	rVB3	6324	7120	0.40%	0.033%

51	14.624	1929	1936	1943	rVV	1127105	1639597	93.24%	7.596%
52	14.795	1959	1965	1976	rBV	207829	320045	18.20%	1.483%
53	15.030	1999	2005	2009	rVV4	16030	22718	1.29%	0.105%
54	15.060	2009	2010	2015	rVB5	2586	2768	0.16%	0.013%
55	15.224	2032	2038	2039	rBV5	1939	2475	0.14%	0.011%

56	15.254	2039	2043	2047	rVV7	3293	4595	0.26%	0.021%
57	15.430	2069	2073	2078	rVV2	9385	14356	0.82%	0.067%
58	15.477	2078	2081	2084	rVB4	4508	5242	0.30%	0.024%
59	15.613	2097	2104	2116	rBV	939398	1328864	75.57%	6.156%
60	15.719	2116	2122	2130	rVV	216886	300333	17.08%	1.391%

61	15.848	2140	2144	2149	rBV7	3706	6421	0.37%	0.030%
62	15.971	2161	2165	2169	rBV5	3464	4398	0.25%	0.020%
63	16.024	2171	2174	2175	rBV3	2079	2165	0.12%	0.010%
64	16.254	2209	2213	2217	rVB6	2015	2905	0.17%	0.013%
65	16.301	2217	2221	2223	rBV4	4099	4919	0.28%	0.023%

66	16.401	2235	2238	2240	rBV4	2121	2008	0.11%	0.009%
67	16.448	2244	2246	2249	rBV3	1694	2156	0.12%	0.010%
68	16.507	2252	2256	2257	rBV4	3440	3634	0.21%	0.017%
69	16.683	2284	2286	2291	rVB4	2356	3050	0.17%	0.014%
70	16.818	2306	2309	2310	rBV2	2393	2493	0.14%	0.012%

71	16.836	2310	2312	2316	rVV4	3636	5100	0.29%	0.024%
72	16.877	2316	2319	2321	rVB3	2213	2513	0.14%	0.012%
73	17.124	2356	2361	2362	rBV5	4280	5139	0.29%	0.024%
74	17.154	2362	2366	2370	rVV3	5315	9756	0.55%	0.045%
75	17.289	2386	2389	2393	rVB4	5400	6093	0.35%	0.028%

76	17.360	2395	2401	2408	rBV	1234969	1758503	100.00%	8.147%
----	--------	------	------	------	-----	---------	---------	---------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
 Data File : BM034201.D
 Acq On : 10 Mar 2022 00:48
 Operator : CG/JU
 Sample : N1775-17
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSC0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
 Title : SVOA CALIBRATION

77	17.460	2411	2418	2429	rVV	1017549	1432864	81.48%	6.638%
78	17.548	2429	2433	2439	rVB6	11732	18383	1.05%	0.085%
79	17.648	2449	2450	2451	rBV	3667	2155	0.12%	0.010%
80	17.765	2467	2470	2477	rVB8	2627	4917	0.28%	0.023%
81	17.871	2483	2488	2489	rBV5	3141	3902	0.22%	0.018%
82	17.960	2501	2503	2504	rBV2	2421	2223	0.13%	0.010%
83	17.983	2504	2507	2512	rVV7	4007	5627	0.32%	0.026%
84	18.036	2512	2516	2521	rVV7	7327	10167	0.58%	0.047%
85	18.136	2529	2533	2535	rBV4	3166	3455	0.20%	0.016%
86	18.165	2536	2538	2541	rVB4	2620	2372	0.13%	0.011%
87	18.254	2548	2553	2561	rBV	44661	66342	3.77%	0.307%
88	18.330	2564	2566	2570	rVB3	5875	5669	0.32%	0.026%
89	18.559	2602	2605	2606	rBV3	2659	2667	0.15%	0.012%
90	18.948	2669	2671	2672	rBV2	3173	2556	0.15%	0.012%
91	19.265	2723	2725	2727	rBV3	4010	2861	0.16%	0.013%
92	19.312	2730	2733	2737	rVV4	12203	17501	1.00%	0.081%
93	19.383	2742	2745	2747	rBV2	14082	17211	0.98%	0.080%
94	19.530	2768	2770	2774	rVB4	12076	8640	0.49%	0.040%
95	19.748	2801	2807	2811	rBV	1191920	1604411	91.24%	7.433%
96	19.783	2811	2813	2820	rVB	163493	189081	10.75%	0.876%
97	21.236	3057	3060	3065	rBV2	78132	110679	6.29%	0.513%
98	21.530	3105	3110	3120	rBV	1278616	1666907	94.79%	7.722%
99	23.812	3492	3498	3507	rBV	759802	1488790	84.66%	6.897%
100	23.971	3519	3525	3534	rVB2	853710	1751151	99.58%	8.113%




Sum of corrected areas: 21585692

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034201.D
Acq On : 10 Mar 2022 00:48
Operator : CG/JU
Sample : N1775-17
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

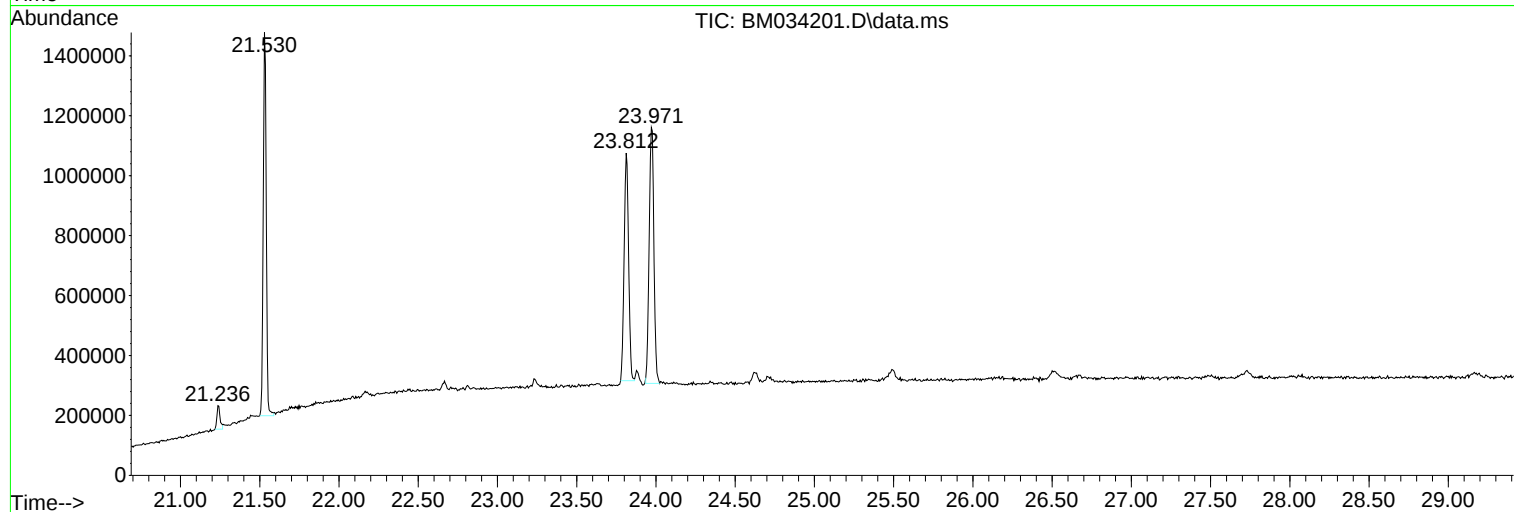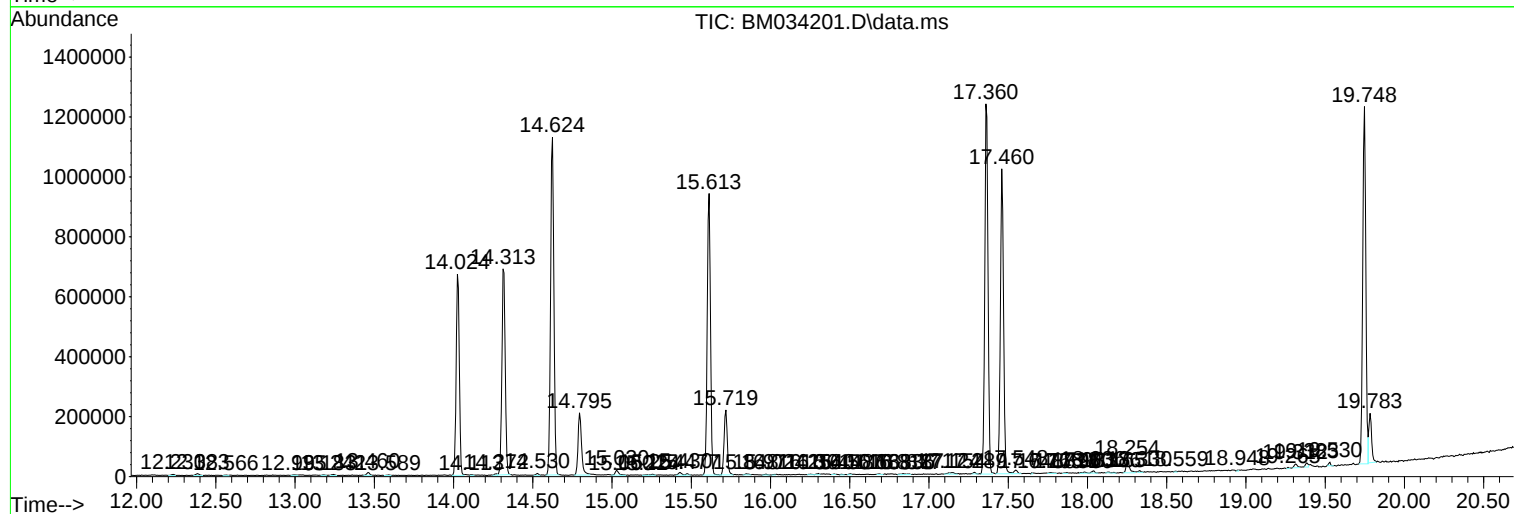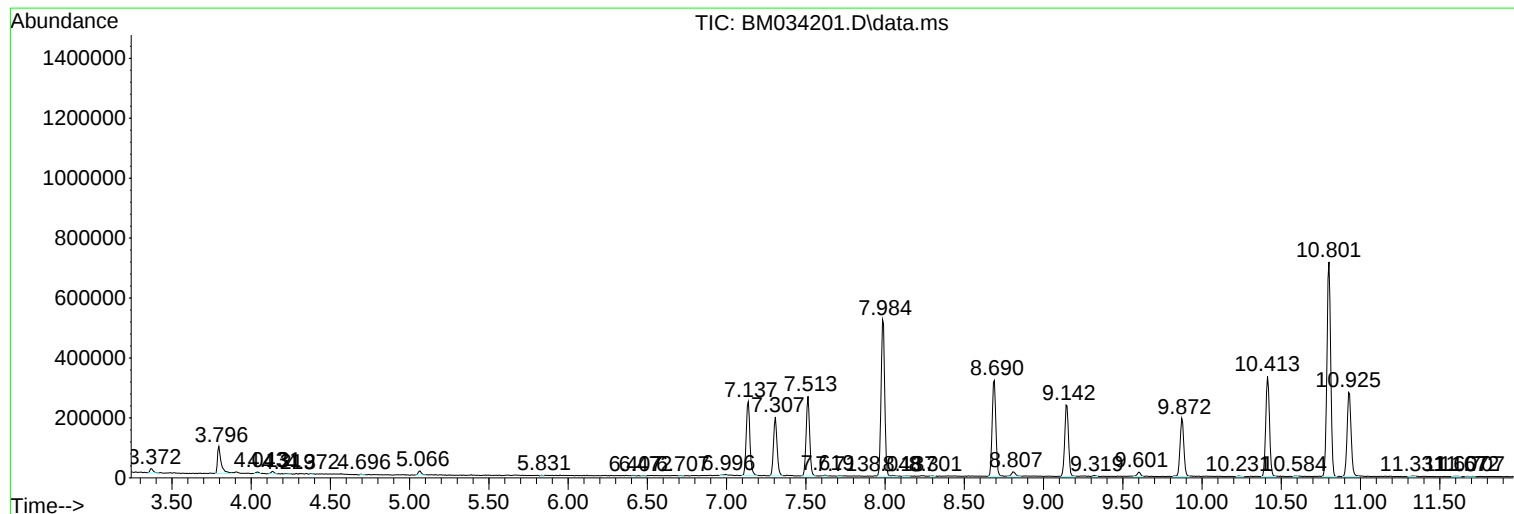

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034201.D
Acq On : 10 Mar 2022 00:48
Operator : CG/JU
Sample : N1775-17
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030822\
Data File : BM034201.D
Acq On : 10 Mar 2022 00:48
Operator : CG/JU
Sample : N1775-17
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------