


Hexachlorocyclopentadiene

Response Ratio

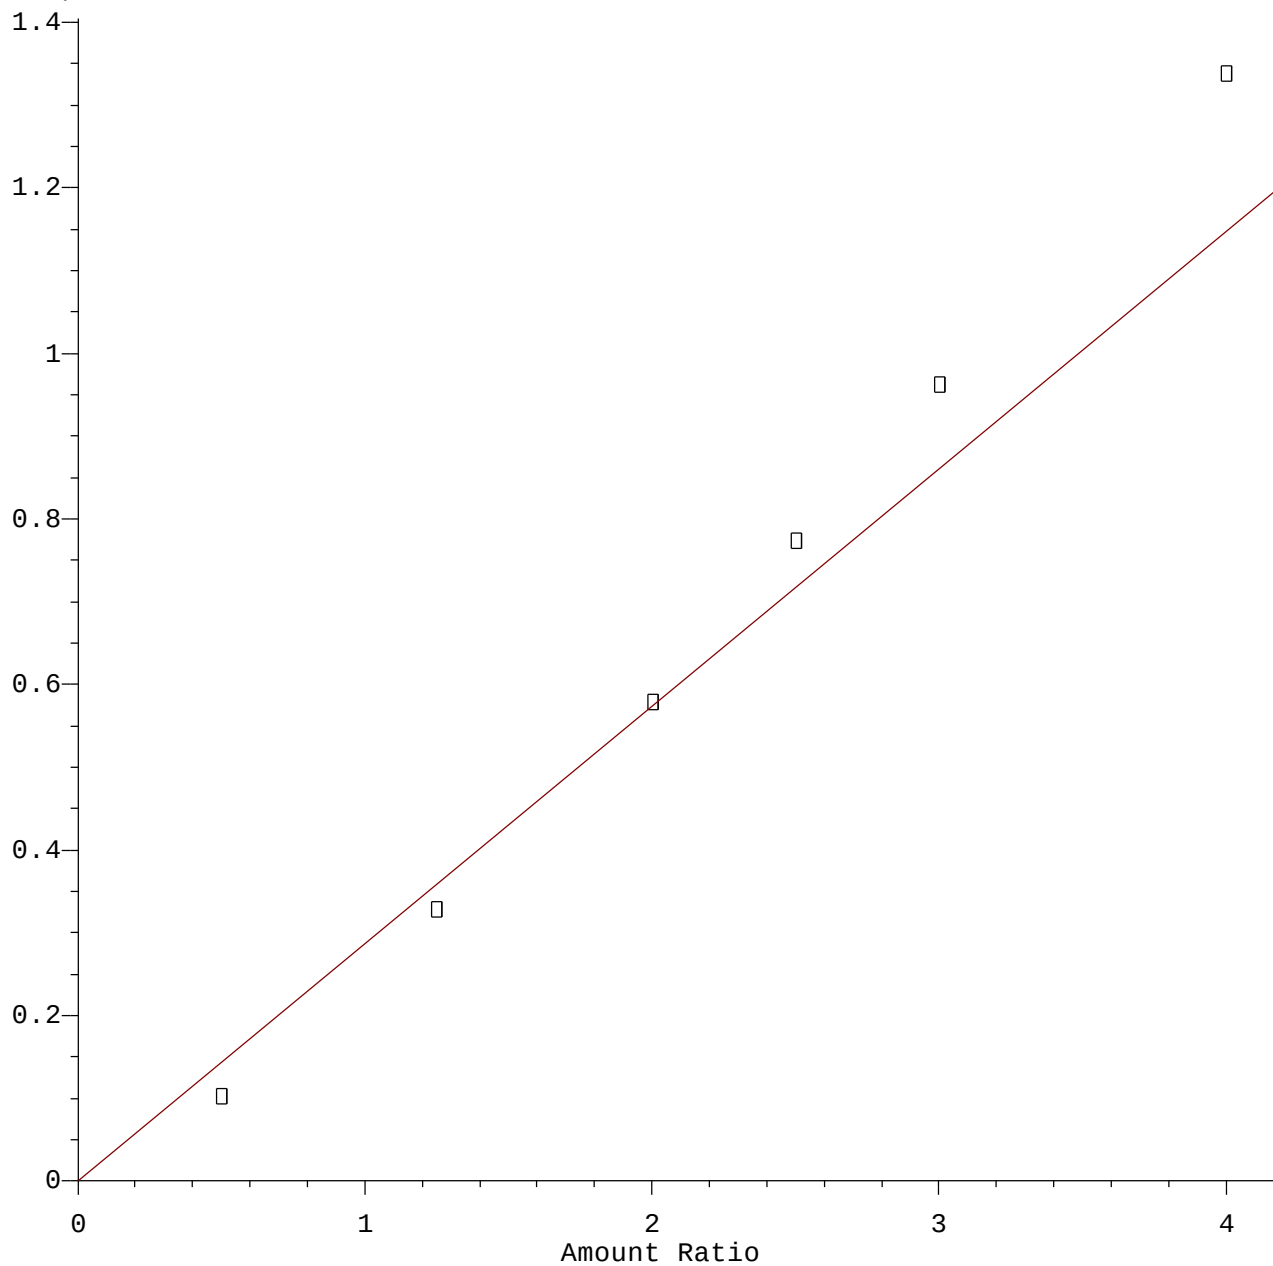


Resp Ratio = 2.87e-001 * Amt
RF Rel Std Dev = 16.8% Curve Fit: Avg RF

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Calibration Table Last Updated: Mon Mar 11 17:30:46 2019

2,4-Dinitrophenol

Response Ratio

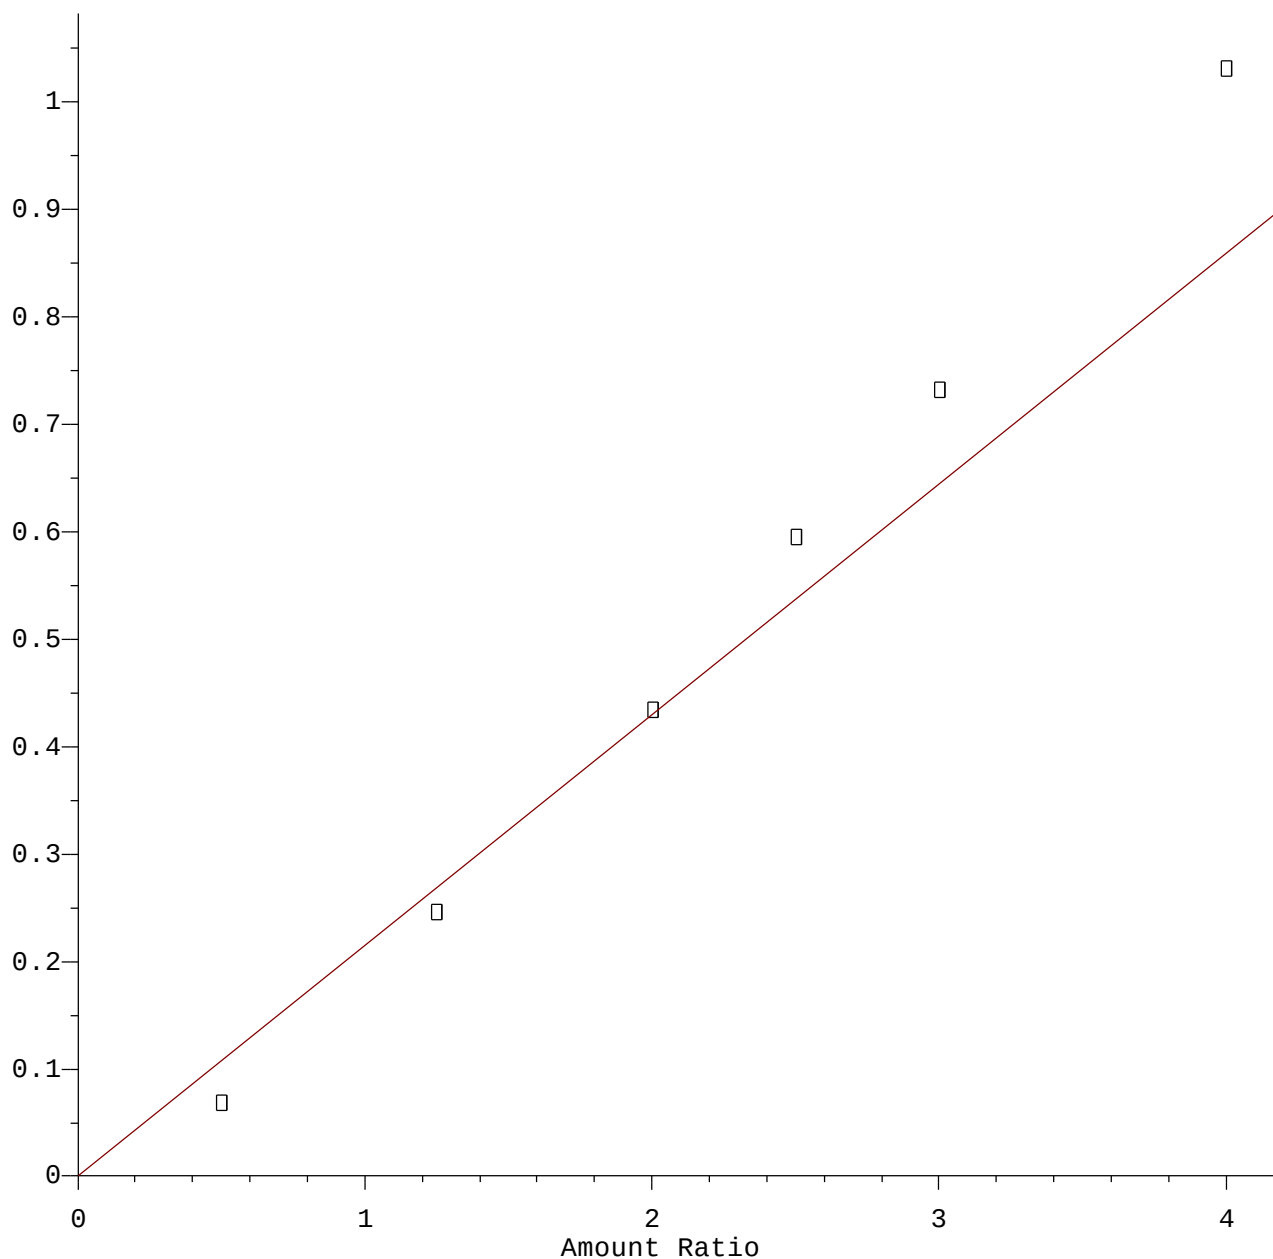

Resp Ratio = 2.15e-001 * Amt
RF Rel Std Dev = 20.6% Curve Fit: Avg RF

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Calibration Table Last Updated: Mon Mar 11 17:30:46 2019