
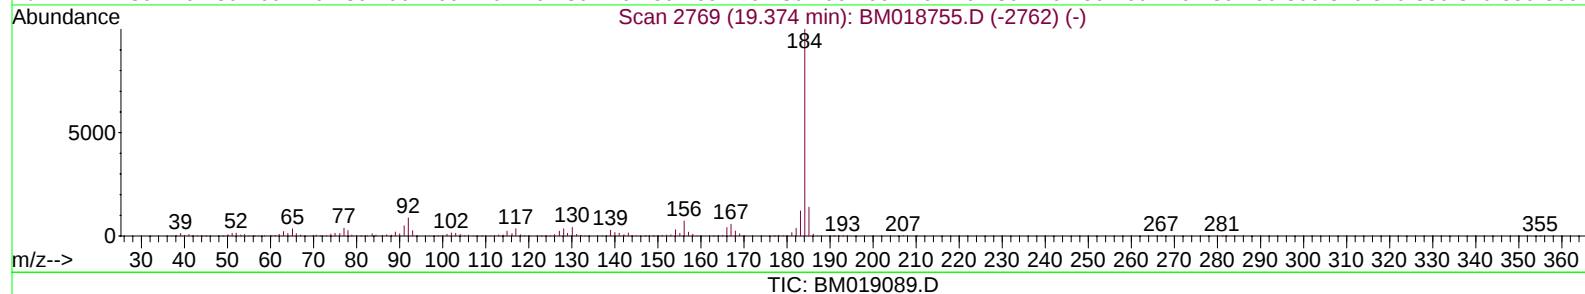
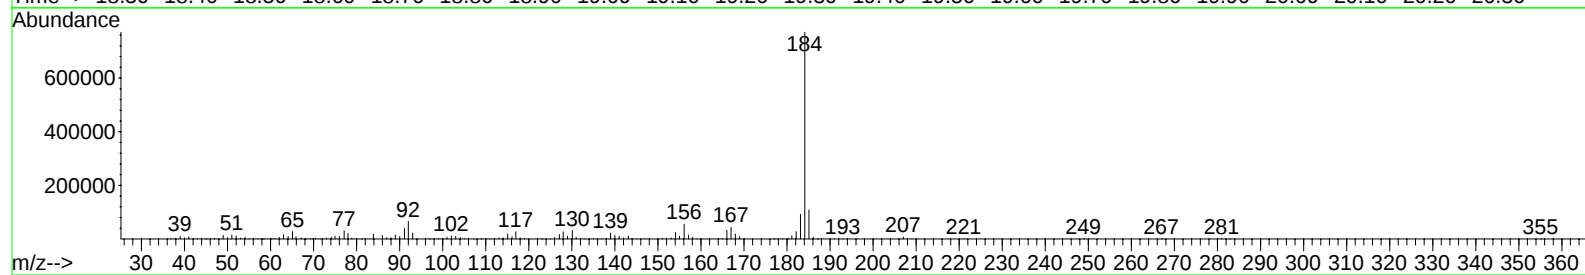


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031119\
 Data File : BM019089.D
 Acq On : 11 Mar 2019 12:16
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 13:27:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 05 03:36:13 2019
 Response via : Initial Calibration

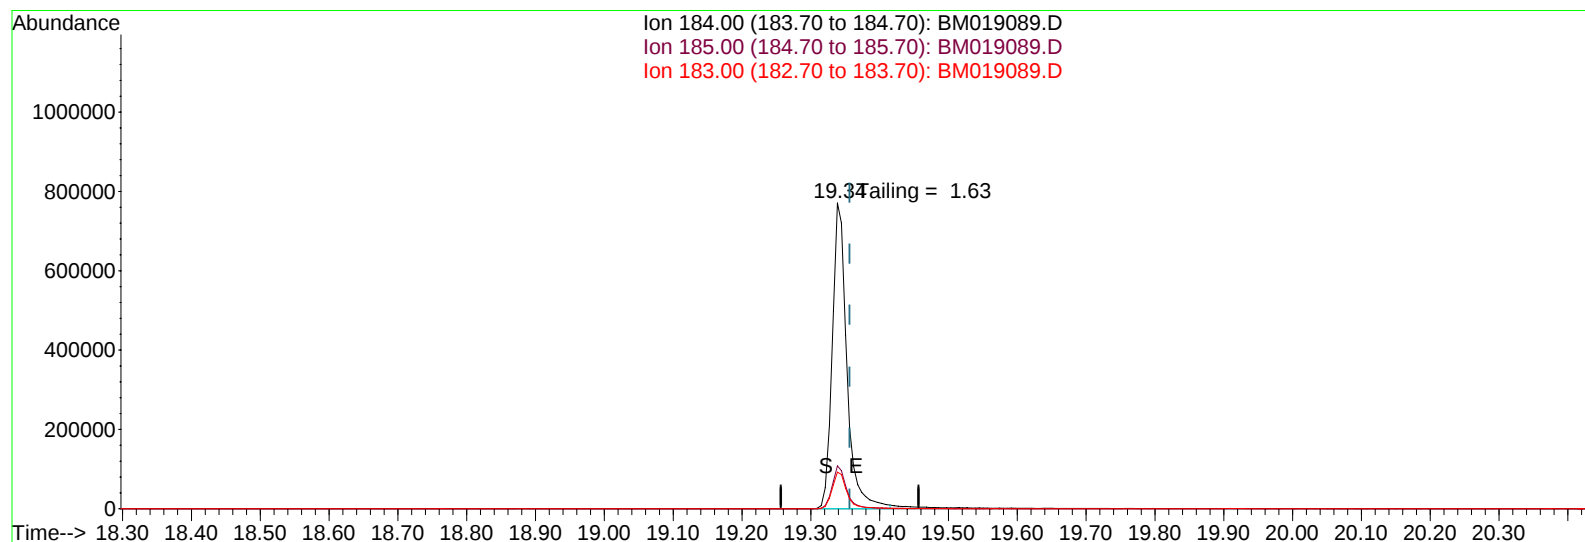

(77) Benzidine


19.339min (-0.018) 32256.39ng

response 1145627

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	14.01
183.00	12.10	11.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031119\
Data File : BM019089.D
Acq On : 11 Mar 2019 12:16
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 13:27:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 05 03:36:13 2019
Response via : Initial Calibration

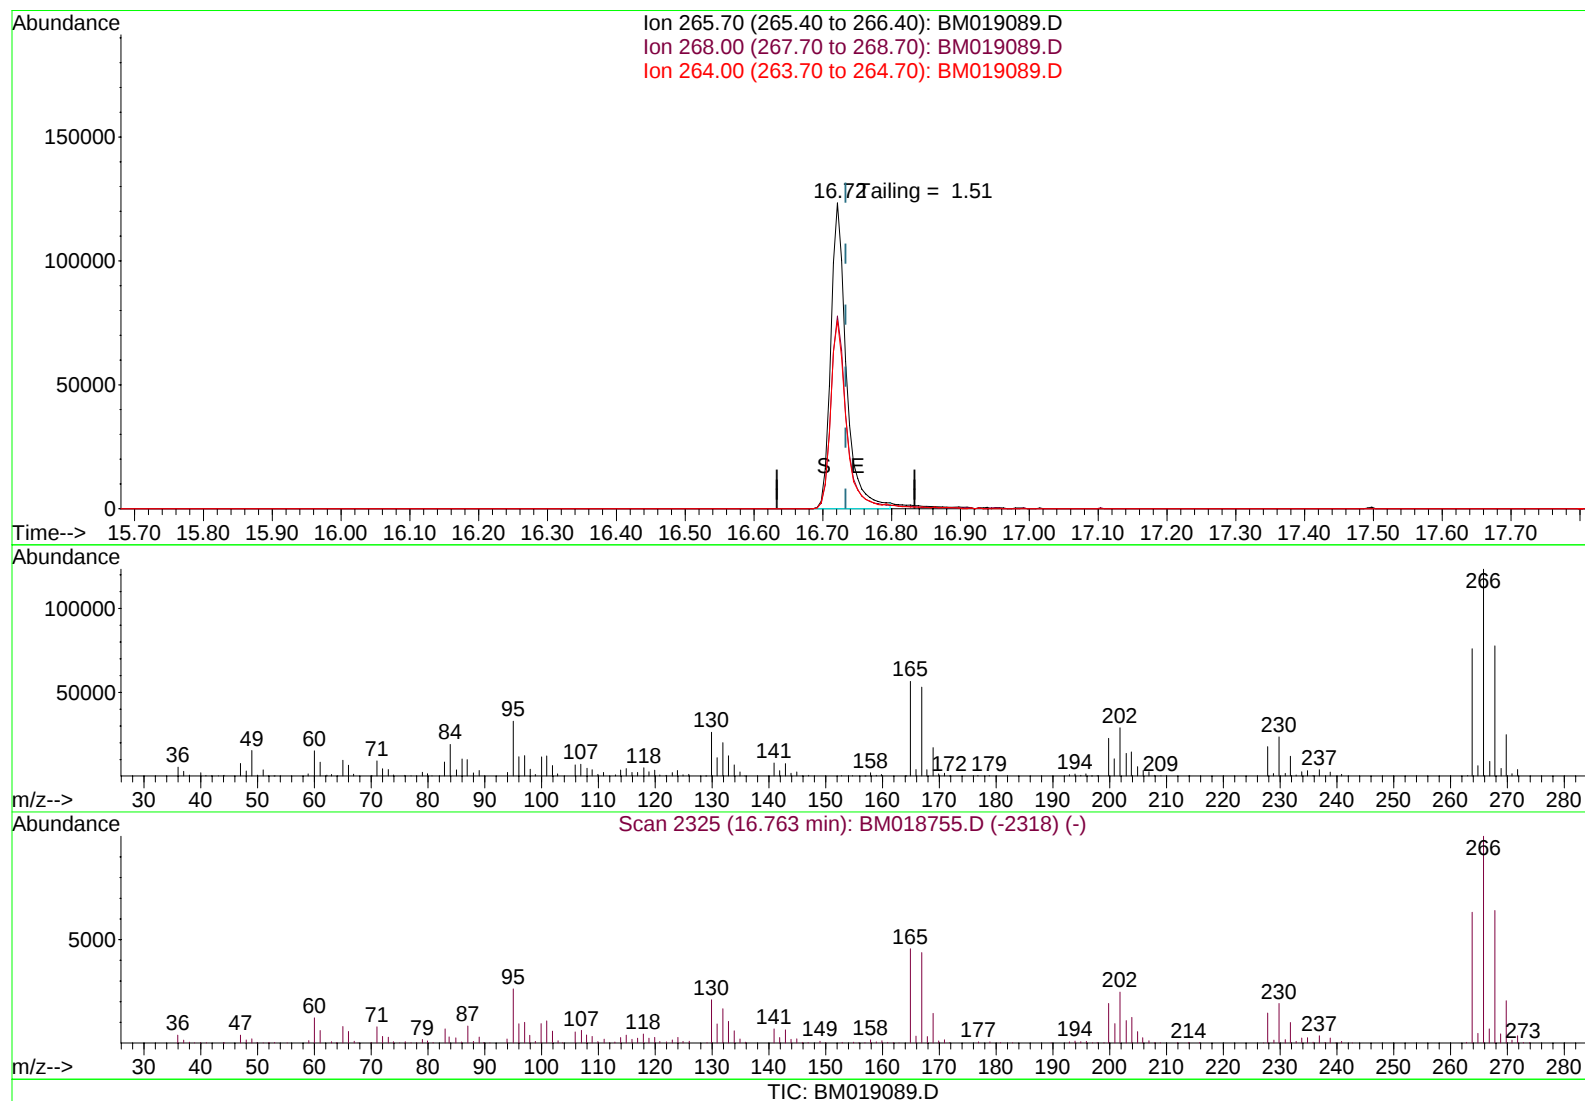

(70) Pentachlorophenol (C)

16.721min (-0.012) 0.00ng

response 194615

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	63.01
264.00	63.20	61.60
0.00	0.00	0.00