


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031119\
 Data File : BM019089.D
 Acq On : 11 Mar 2019 12:16
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 11 17:30:46 2019

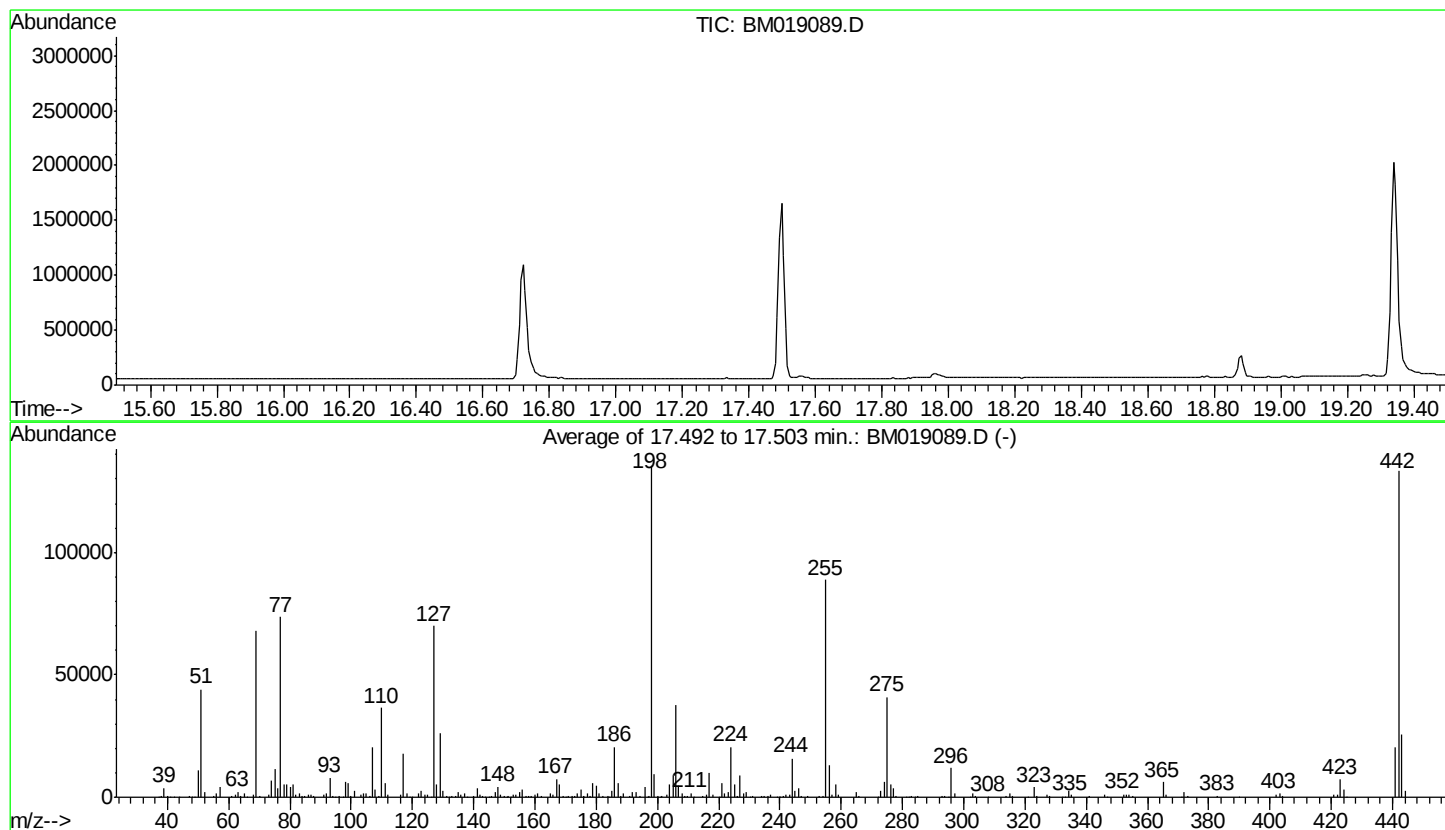

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	43922	PASS
68	69	0.00	2	1.9	1261	PASS
69	198	0.00	100	50.3	68098	PASS
70	69	0.00	2	0.7	497	PASS
127	198	10	80	51.7	69960	PASS
197	198	0.00	2	0.5	701	PASS
198	198	100	100	100.0	135445	PASS
199	198	5	9	6.8	9196	PASS
275	198	10	60	30.3	41061	PASS
365	198	1	100	4.6	6275	PASS
441	198	0.01	100	14.9	20175	PASS
442	198	50	100	98.4	133253	PASS
443	442	15	24	19.1	25437	PASS