

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031519\
 Data File : BM019210.D
 Acq On : 16 Mar 2019 05:38
 Operator : JU/SJ
 Sample : K1905-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 RT-3483

Quant Time: Mar 16 06:30:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 11 17:30:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	199389	20.00	ng	-0.01
21) Naphthalene-d8	10.43	136	823299	20.00	ng	-0.02
39) Acenaphthene-d10	14.30	164	540200	20.00	ng	-0.02
64) Phenanthrene-d10	17.06	188	1209499	20.00	ng	-0.01
76) Chrysene-d12	21.26	240	970604	20.00	ng	-0.02
87) Perylene-d12	23.49	264	867420	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	1681877	136.61	ng	0.00
7) Phenol-d6	6.83	99	2089721	116.04	ng	-0.01
23) Nitrobenzene-d5	8.82	82	1802079	103.47	ng	-0.01
42) 2,4,6-Tribromophenol	15.81	330	1281798	160.71	ng	-0.01
45) 2-Fluorobiphenyl	12.92	172	3939956	94.87	ng	-0.02
79) Terphenyl-d14	19.70	244	6759105	138.25	ng	-0.01


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031519\
Data File : BM019210.D
Acq On : 16 Mar 2019 05:38
Operator : JU/SJ
Sample : K1905-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RT-3483

Quant Time: Mar 16 06:30:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 11 17:30:46 2019
Response via : Initial Calibration

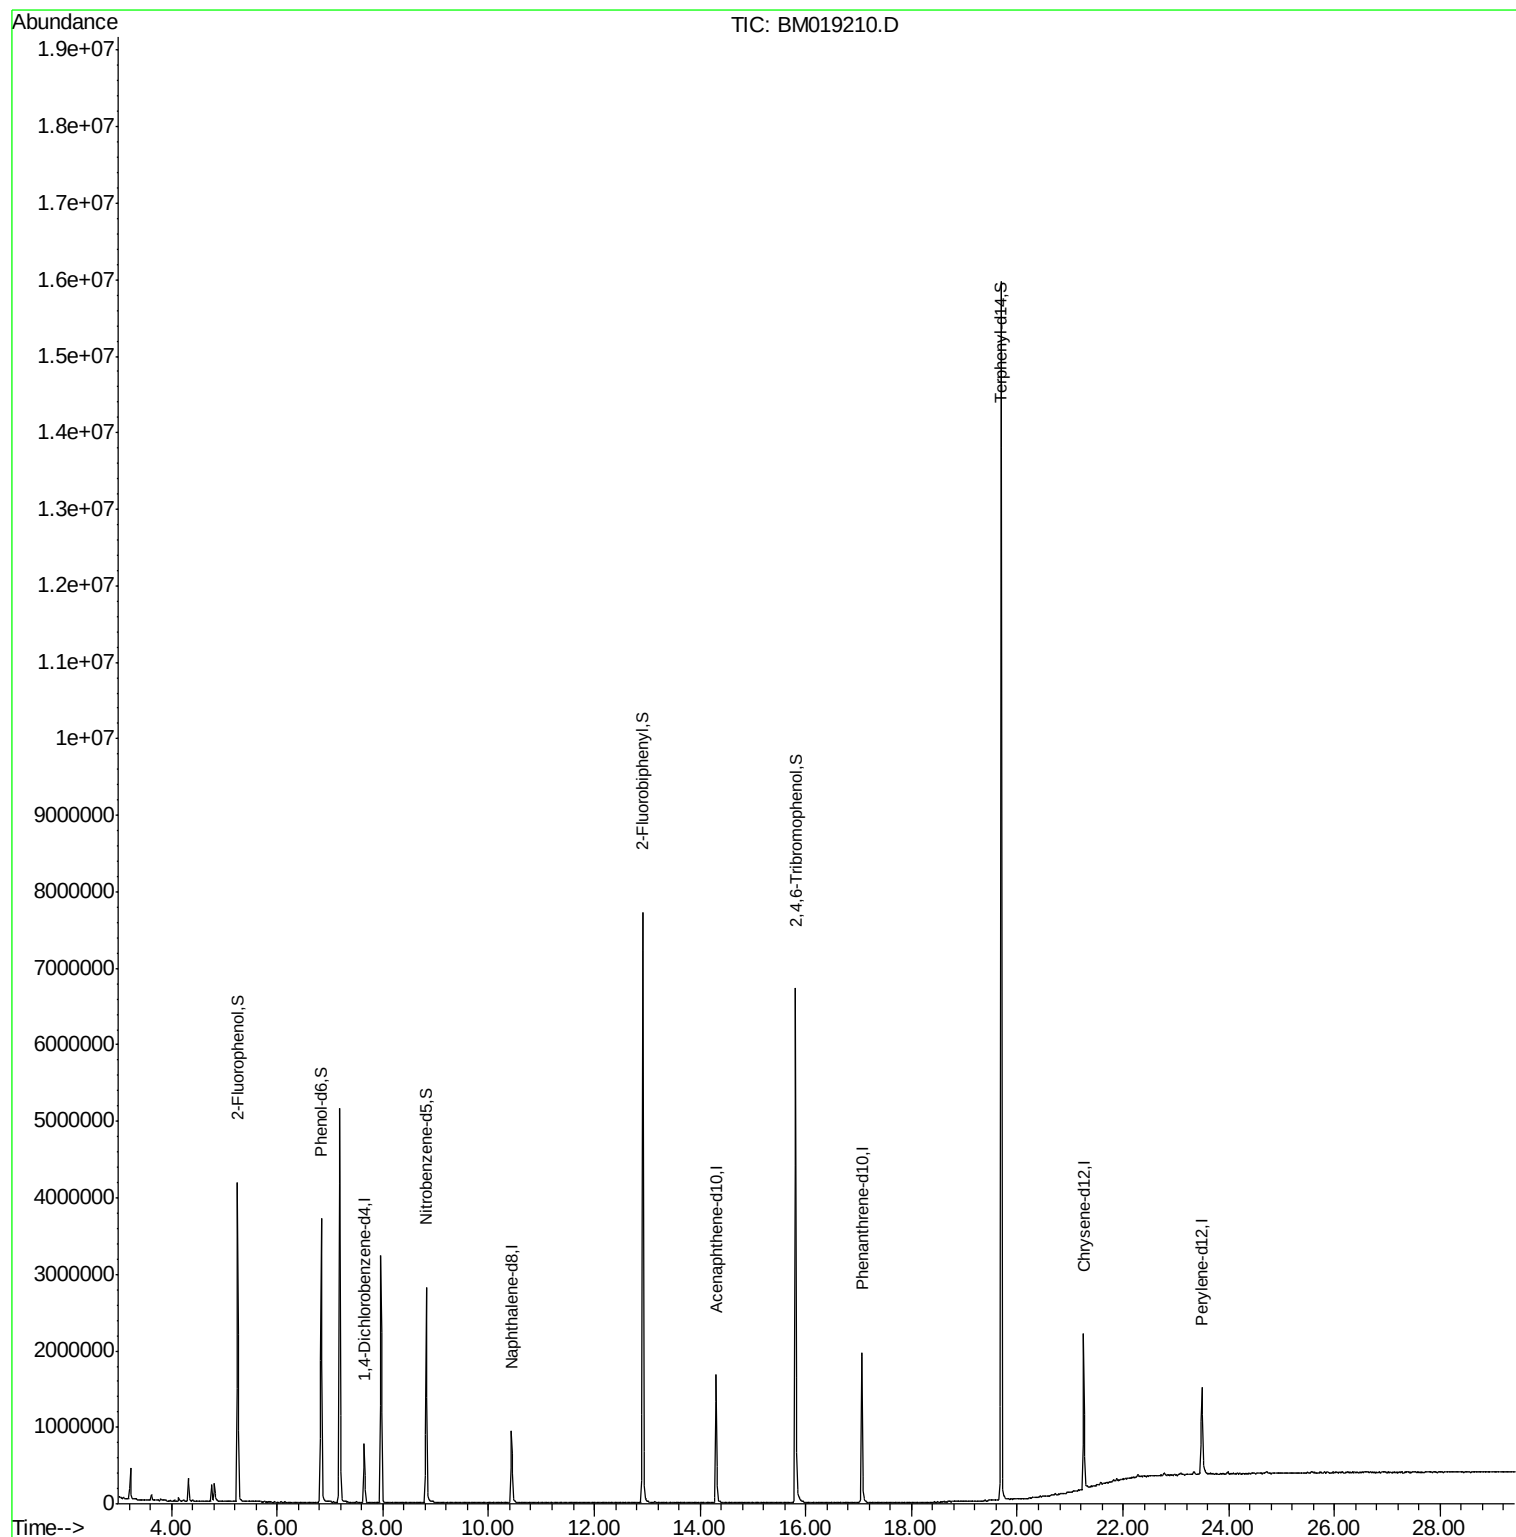




#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.65 min Scan# 793
 Delta R.T. -0.01 min
 Lab File: BM019210.D
 Acq: 16 Mar 2019 05:38

Instrument :
 BNA_M
 ClientSampleId :
 RT-3483

Tgt Ion	Resp	Lower	Upper
152	100		
150	155.9	125.3	187.9
115	61.0	49.4	74.0



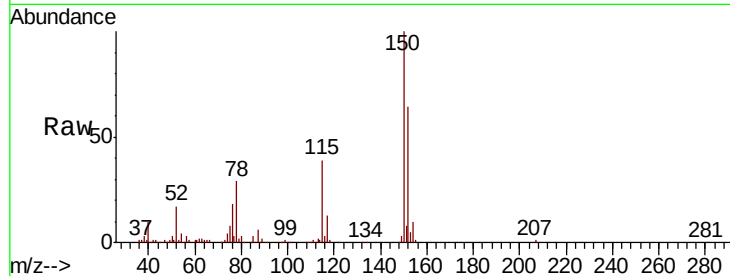


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

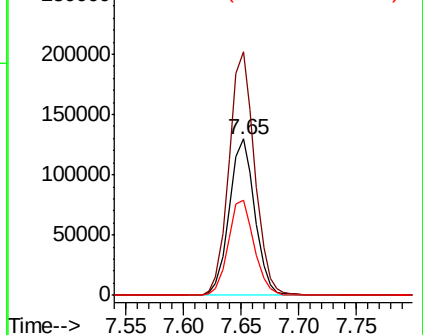

#5

2-Fluorophenol
 Concen: 136.605 ng
 RT: 5.25 min Scan# 385
 Delta R.T. -0.01 min
 Lab File: BM019210.D
 Acq: 16 Mar 2019 05:38

Tgt Ion	Resp	Lower	Upper
112	100		
64	63.2	51.4	77.0
63	32.3	26.6	40.0


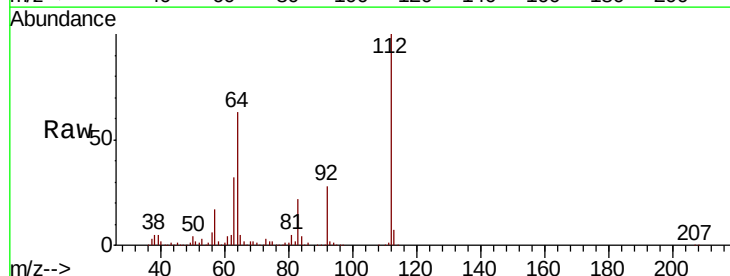



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

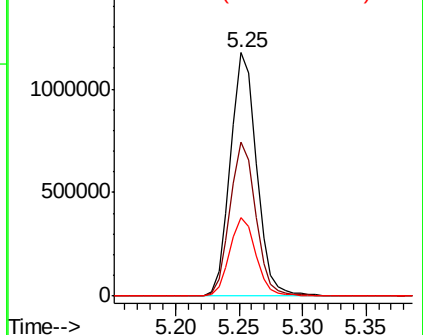



#7

Phenol-d6

Concen: 116.039 ng

RT: 6.83 min Scan# 654

Delta R.T. -0.01 min

Lab File: BM019210.D

Acq: 16 Mar 2019 05:38

Instrument :

BNA_M

ClientSampleId :

RT-3483


Tgt Ion: 99 Resp: 2089721

Ion Ratio Lower Upper

99 100

42 14.0 10.9 16.3

71 37.9 30.3 45.5






Abundance

Ion 99.00 (98.70 to 99.70): BM019210.D (-639) (-)

Ion 42.00 (41.70 to 42.70): BM019210.D (-639) (-)

Ion 71.00 (70.70 to 71.70): BM019210.D (-639) (-)

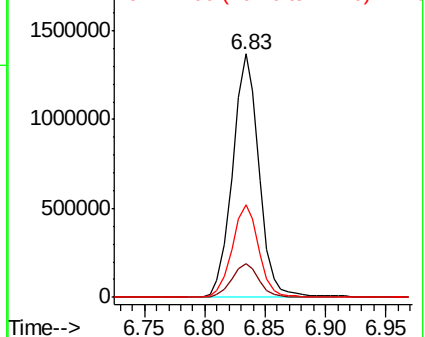

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.43 min Scan# 1266

Delta R.T. -0.02 min

Lab File: BM019210.D

Acq: 16 Mar 2019 05:38

Tgt Ion: 136 Resp: 823299


Ion Ratio Lower Upper

136 100

137 11.0 8.6 13.0

54 6.5 5.2 7.8

68 7.6 5.8 8.8





Abundance


Ion 136.00 (135.70 to 136.70): BM019210.D (-1252) (-)

Ion 137.00 (136.70 to 137.70): BM019210.D (-1252) (-)

Ion 54.00 (53.70 to 54.70): BM019210.D (-1252) (-)

Ion 68.00 (67.70 to 68.70): BM019210.D (-1252) (-)

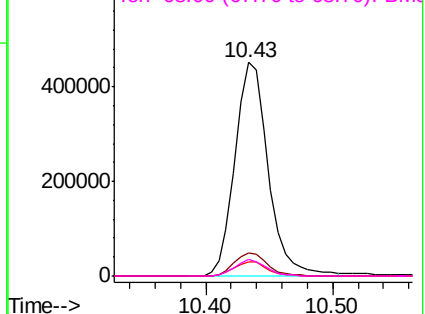







#23
Nitrobenzene-d5
Concen: 103.467 ng
RT: 8.82 min Scan# 992
Delta R.T. -0.01 min
Lab File: BM019210.D
Acq: 16 Mar 2019 05:38

Instrument :
BNA_M
ClientSampleID :
RT-3483

Tgt Ion: 82 Resp: 1802079
Ion Ratio Lower Upper
82 100
128 37.8 29.4 44.2
54 37.0 29.9 44.9

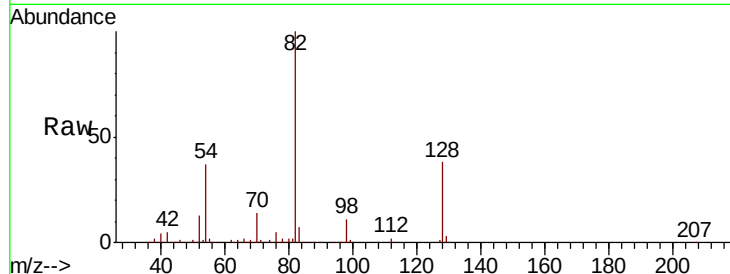


Abundance Ion 82.00 (81.70 to 82.70): BM019210.D (-977) (-)
Ion 128.00 (127.70 to 128.70): BM019210.D (-977) (-)
Ion 54.00 (53.70 to 54.70): BM019210.D (-977) (-)

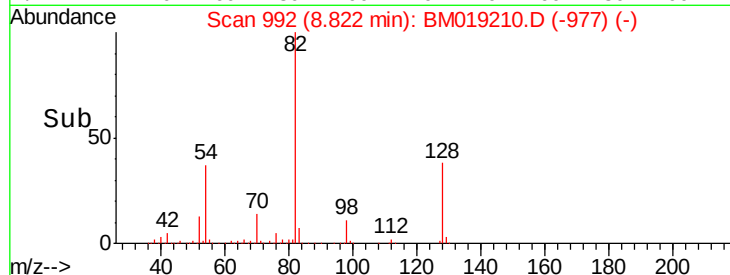
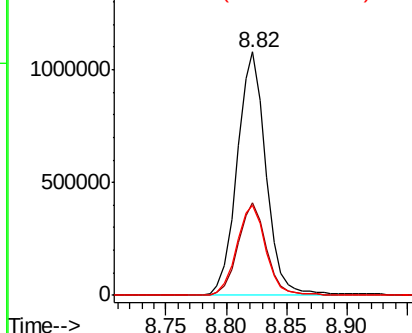



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.30 min Scan# 1924
Delta R.T. -0.02 min
Lab File: BM019210.D
Acq: 16 Mar 2019 05:38

Tgt Ion: 164 Resp: 540200
Ion Ratio Lower Upper
164 100
162 102.8 83.5 125.3
160 46.1 36.3 54.5

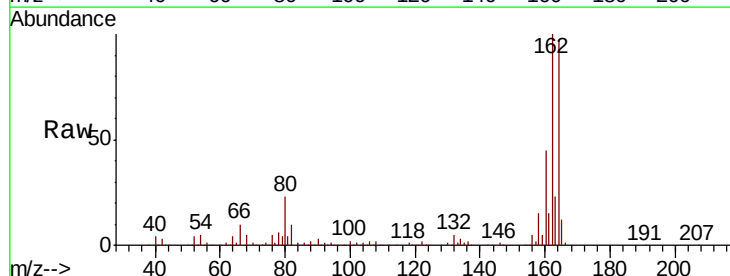

Abundance Ion 164.00 (163.70 to 164.70): BM019210.D (-1910) (-)
Ion 162.00 (161.70 to 162.70): BM019210.D (-1910) (-)
Ion 160.00 (159.70 to 160.70): BM019210.D (-1910) (-)

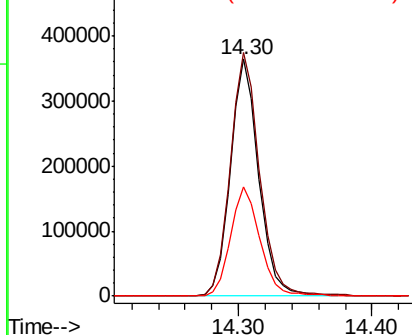



#42

2,4,6-Tribromophenol

Concen: 160.710 ng

RT: 15.81 min Scan# 2180

Delta R.T. -0.01 min

Lab File: BM019210.D

Acq: 16 Mar 2019 05:38

Instrument :

BNA_M

ClientSampleId :

RT-3483


Tgt Ion:330 Resp: 1281798

Ion Ratio Lower Upper

330 100

332 96.6 76.8 115.2




141 32.9 27.0 40.4

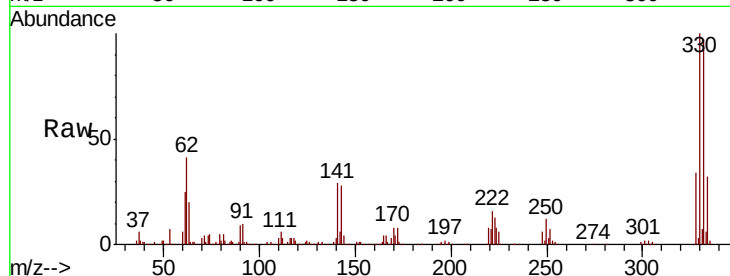

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

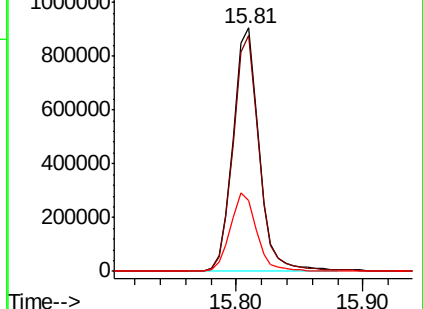

#45

2-Fluorobiphenyl

Concen: 94.871 ng

RT: 12.92 min Scan# 1688

Delta R.T. -0.02 min

Lab File: BM019210.D

Acq: 16 Mar 2019 05:38


Tgt Ion:172 Resp: 3939956

Ion Ratio Lower Upper

172 100

171 36.2 28.6 42.8



170 23.6 18.6 28.0




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



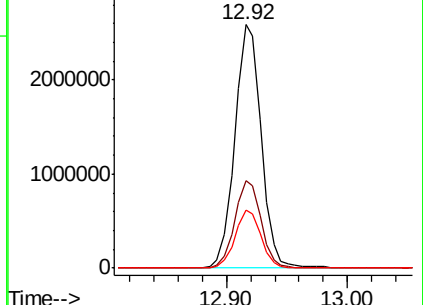





#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.06 min Scan# 2393
Delta R.T. -0.01 min
Lab File: BM019210.D
Acq: 16 Mar 2019 05:38




Instrument :
BNA_M
ClientSampled :
RT-3483


Tgt Ion:188 Resp: 1209499
Ion Ratio Lower Upper
188 100
94 9.7 8.1 12.1
80 12.0 9.7 14.5

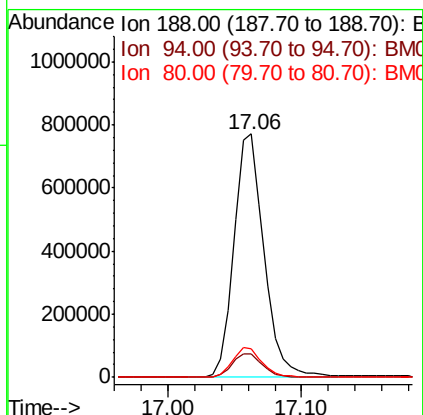

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.26 min Scan# 3106
Delta R.T. -0.02 min
Lab File: BM019210.D
Acq: 16 Mar 2019 05:38

Tgt Ion:240 Resp: 970604
Ion Ratio Lower Upper
240 100
120 11.2 8.9 13.3
236 25.4 21.0 31.4

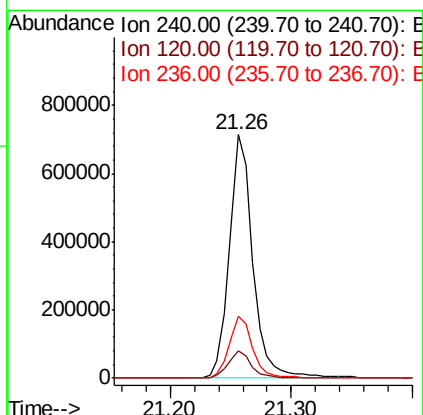

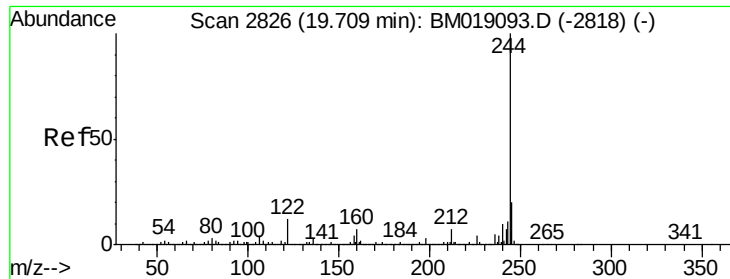

#79

Terphenyl-d14

Concen: 138.247 ng

RT: 19.70 min Scan# 2841

Delta R.T. -0.01 min

Lab File: BM019210.D

Acq: 16 Mar 2019 05:38

Instrument :

BNA_M

ClientSampleId :

RT-3483


Tgt Ion:244 Resp: 6759105

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.2




122 12.0 9.4 14.2

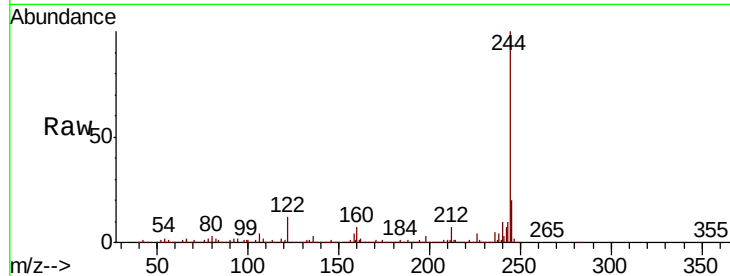

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

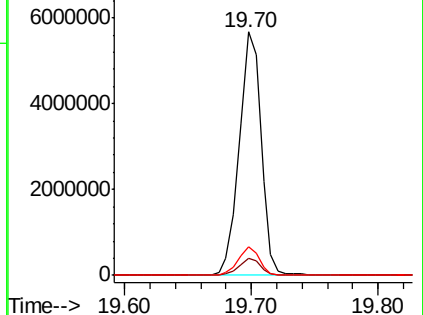

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.49 min Scan# 3486

Delta R.T. -0.02 min

Lab File: BM019210.D

Acq: 16 Mar 2019 05:38


Tgt Ion:264 Resp: 867420

Ion Ratio Lower Upper

264 100

260 23.3 18.6 28.0

265 21.9 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

