

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031519\
 Data File : BM019190.D
 Acq On : 15 Mar 2019 17:26
 Operator : JU/SJ
 Sample : K1905-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 RBR-200050

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.257	379	386	404	rBV	4683490	6996066	46.76%	7.960%
2	6.840	647	655	675	rBV	5155069	8606178	57.52%	9.792%
3	7.193	707	715	730	rBV	5228114	8224721	54.97%	9.358%
4	7.651	787	793	801	rBV	853299	1325806	8.86%	1.508%
5	7.969	838	847	859	rBV	3404132	5368770	35.88%	6.108%
6	8.822	984	992	1009	rBV	2830487	4818972	32.21%	5.483%
7	10.439	1259	1267	1280	rBV	1163036	2035782	13.61%	2.316%
8	12.922	1682	1689	1713	rBV	7592989	11084381	74.08%	12.612%
9	13.774	1828	1834	1847	rBV	316307	517065	3.46%	0.588%
10	14.310	1912	1925	1939	rBV2	1860136	2945800	19.69%	3.352%
11	15.810	2173	2180	2198	rBV	6756638	9720645	64.97%	11.060%
12	17.062	2386	2393	2410	rBV2	2382597	3461257	23.13%	3.938%
13	17.951	2539	2544	2550	rBV	194017	297811	1.99%	0.339%
14	19.703	2836	2842	2857	rBV	12120522	14962638	100.00%	17.024%
15	20.962	3052	3056	3068	rBV	786662	1086119	7.26%	1.236%
16	21.262	3102	3107	3116	rBV	2565955	3347303	22.37%	3.808%
17	22.286	3279	3281	3288	rVB2	148445	166921	1.12%	0.190%
18	22.786	3364	3366	3372	rVB	159908	201344	1.35%	0.229%
19	23.503	3481	3488	3496	rVB	1414839	2723467	18.20%	3.099%


Sum of corrected areas: 87891046

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031519\
Data File : BM019190.D
Acq On : 15 Mar 2019 17:26
Operator : JU/SJ
Sample : K1905-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RBR-200050

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

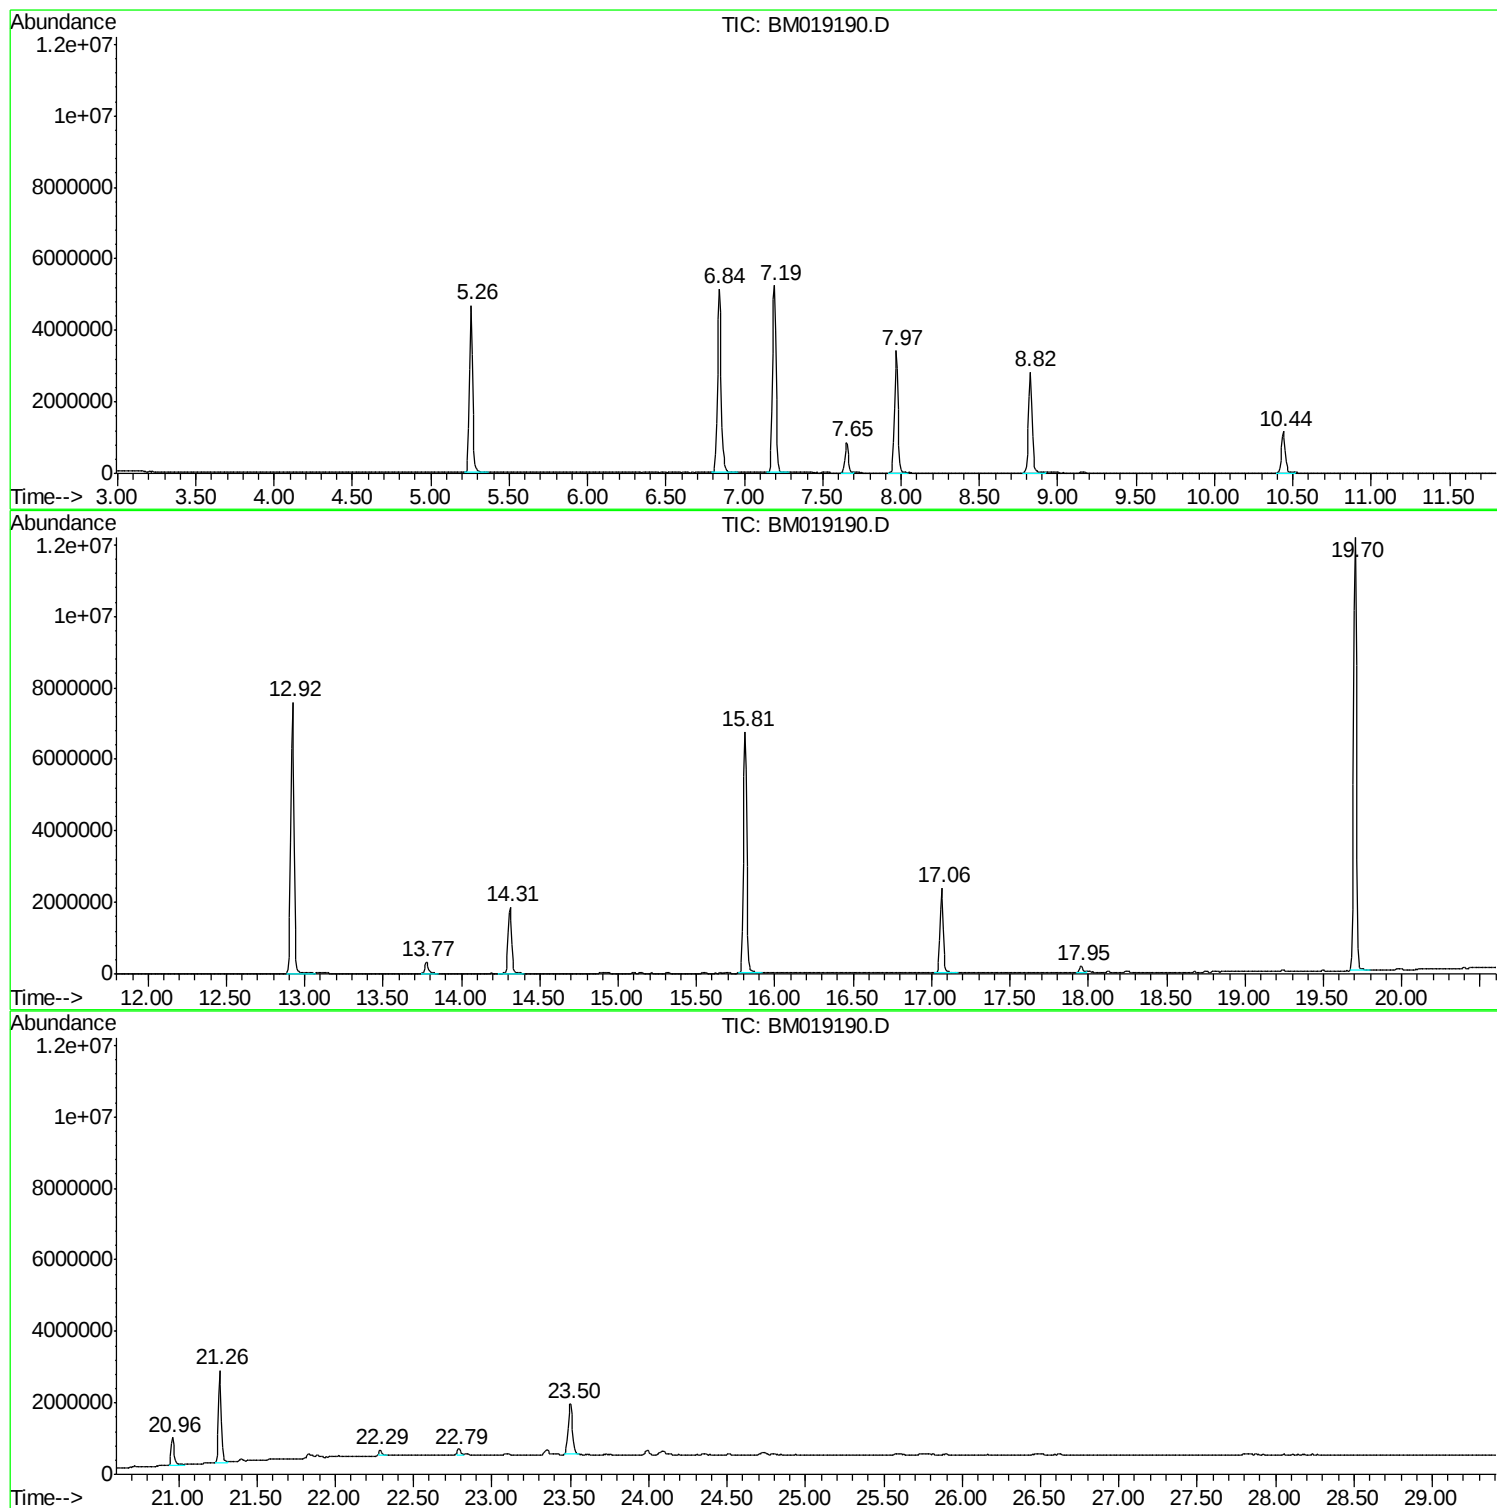

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031519\
Data File : BM019190.D
Acq On : 15 Mar 2019 17:26
Operator : JU/SJ
Sample : K1905-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
RBR-200050










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.19 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.19	124.07 ng	8224720	1,4-Dichlorobenzene-d4	7.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Tranvlcvpromine-propionyl	189	C12H15NO	1000123-86-3	12
2		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9

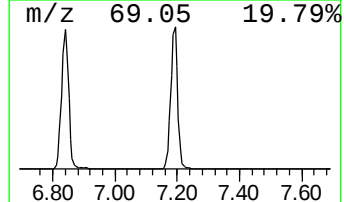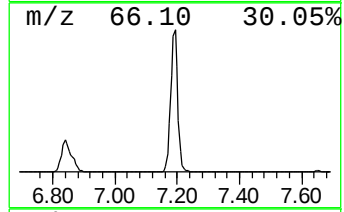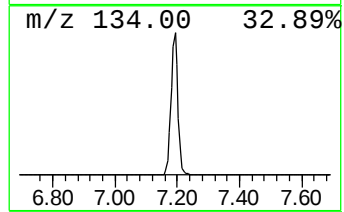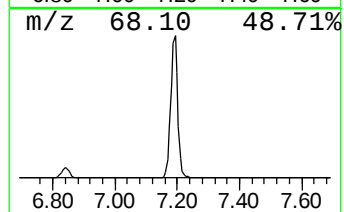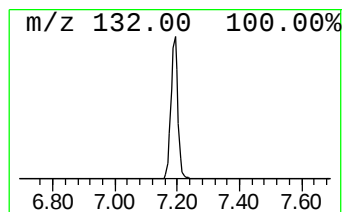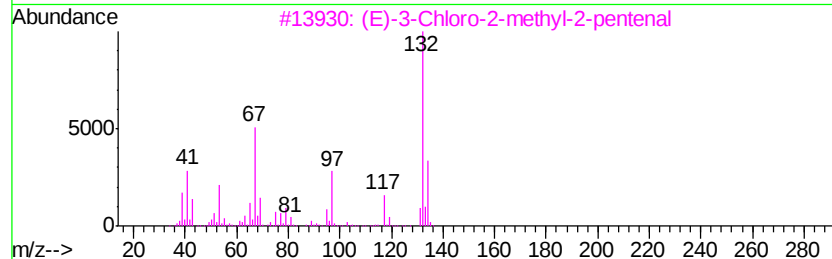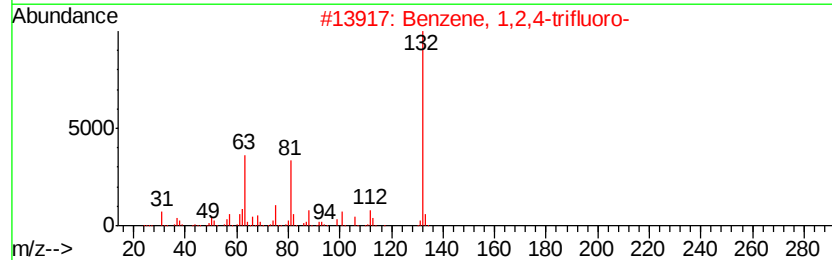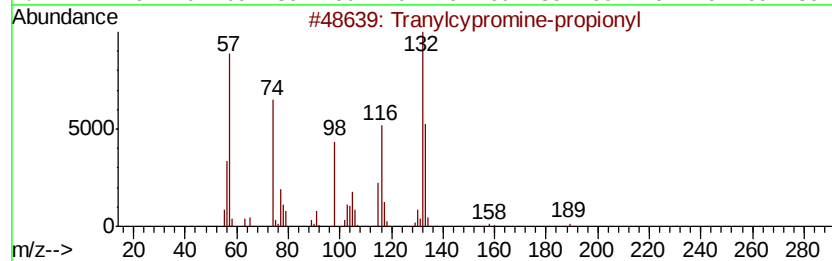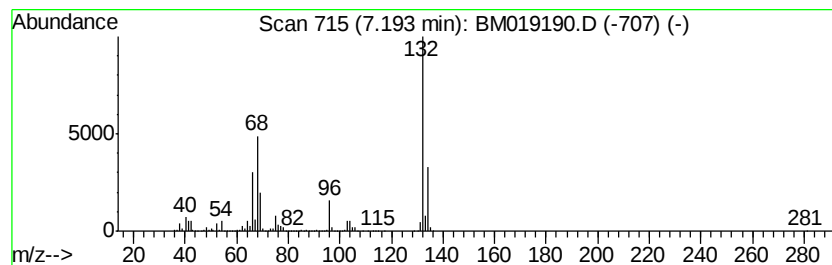

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031519\
Data File : BM019190.D
Acq On : 15 Mar 2019 17:26
Operator : JU/SJ
Sample : K1905-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RBR-200050










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Trichloroacetic acid, hexad... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.96	6.49 ng	1086120	Chrysene-d12	21.26

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	91
2		9-Eicosene, (E)-	280	C20H40	074685-29-3	91
3		Bromoacetic acid, octadecyl ester	390	C20H39BrO2	018992-03-5	91
4		Heptafluorobutanoic acid, heptad...	452	C21H35F7O2	1000282-97-3	91
5		Cyclotetradecane	196	C14H28	000295-17-0	90

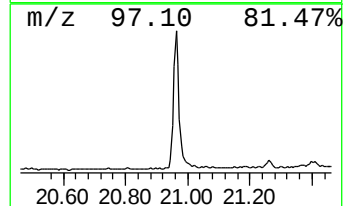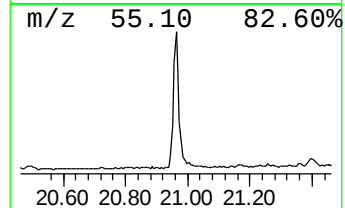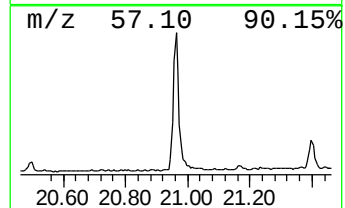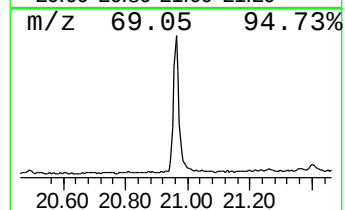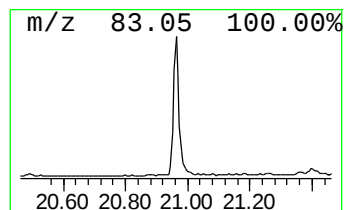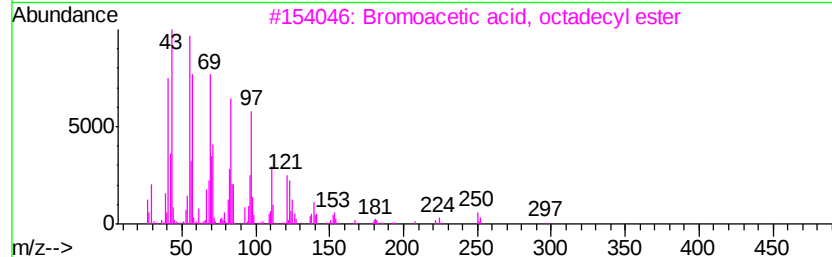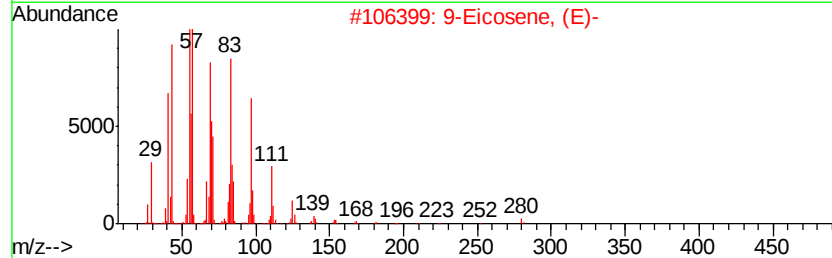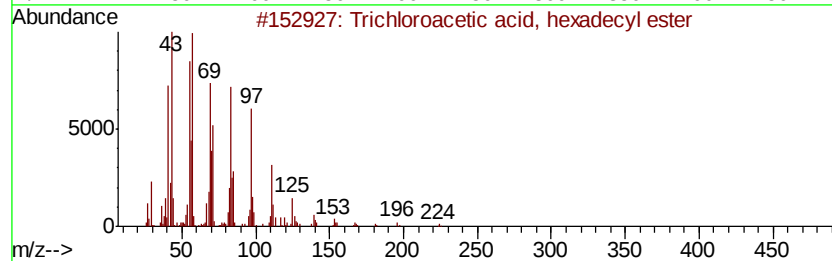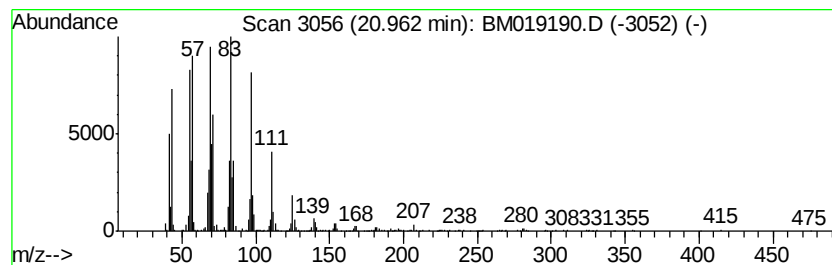

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031519\
Data File : BM019190.D
Acq On : 15 Mar 2019 17:26
Operator : JU/SJ
Sample : K1905-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RBR-200050

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.19	7.19	124.1	ng	8224720	1	7.65	1325810	20.0
Trichloroacetic a...	20.96	6.5	ng	1086120	5	21.26	3347300	20.0