


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031519\
 Data File : BM019180.D
 Acq On : 15 Mar 2019 10:44
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 11 17:30:46 2019

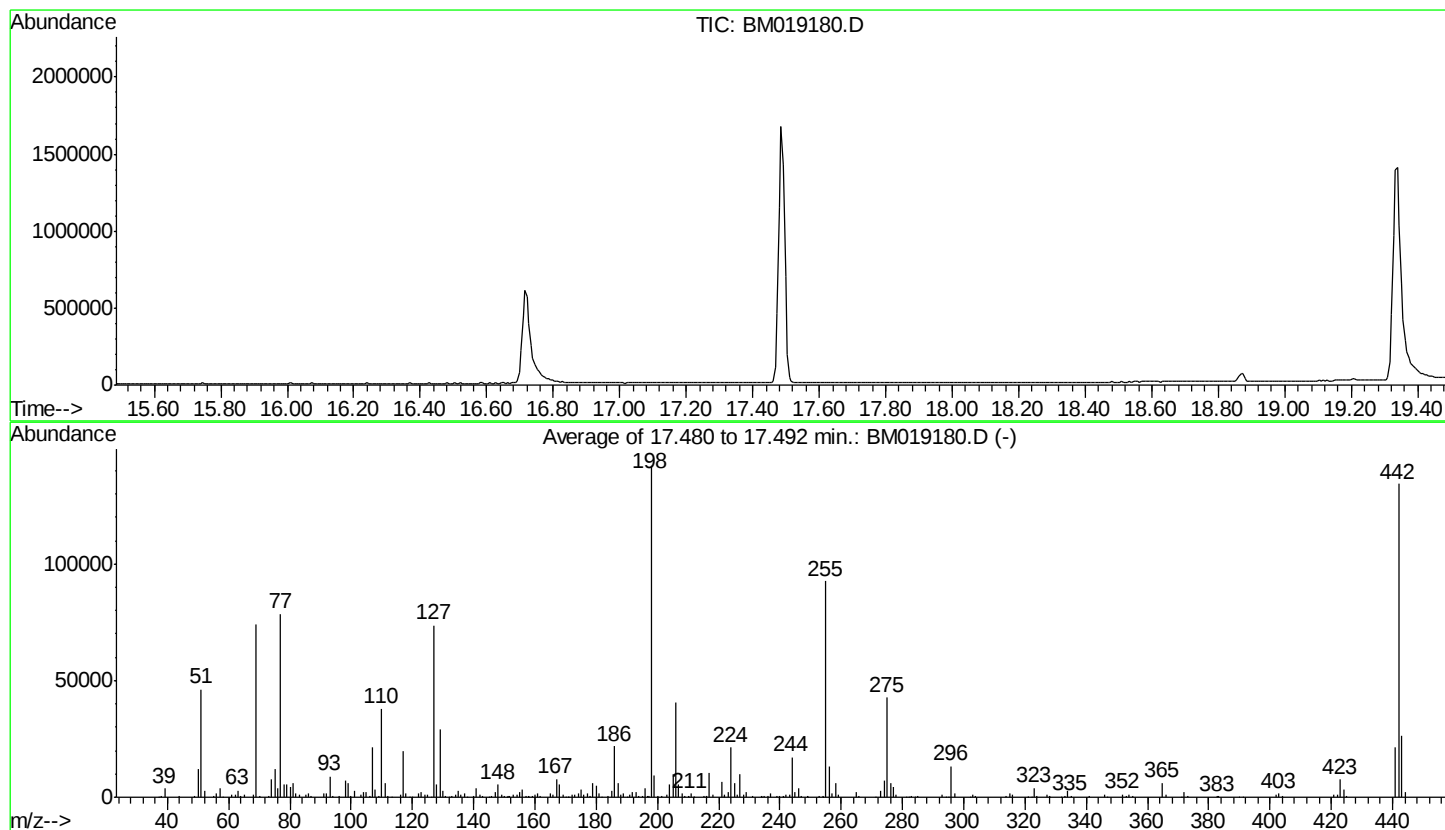

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	46357	PASS
68	69	0.00	2	1.8	1314	PASS
69	198	0.00	100	52.1	74077	PASS
70	69	0.00	2	0.6	449	PASS
127	198	10	80	51.8	73592	PASS
197	198	0.00	2	0.4	571	PASS
198	198	100	100	100.0	142170	PASS
199	198	5	9	6.7	9460	PASS
275	198	10	60	30.0	42608	PASS
365	198	1	100	4.4	6239	PASS
441	198	0.01	100	15.0	21322	PASS
442	198	50	100	94.5	134405	PASS
443	442	15	24	19.5	26193	PASS