


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031519\
 Data File : BM019198.D
 Acq On : 15 Mar 2019 22:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 11 17:30:46 2019

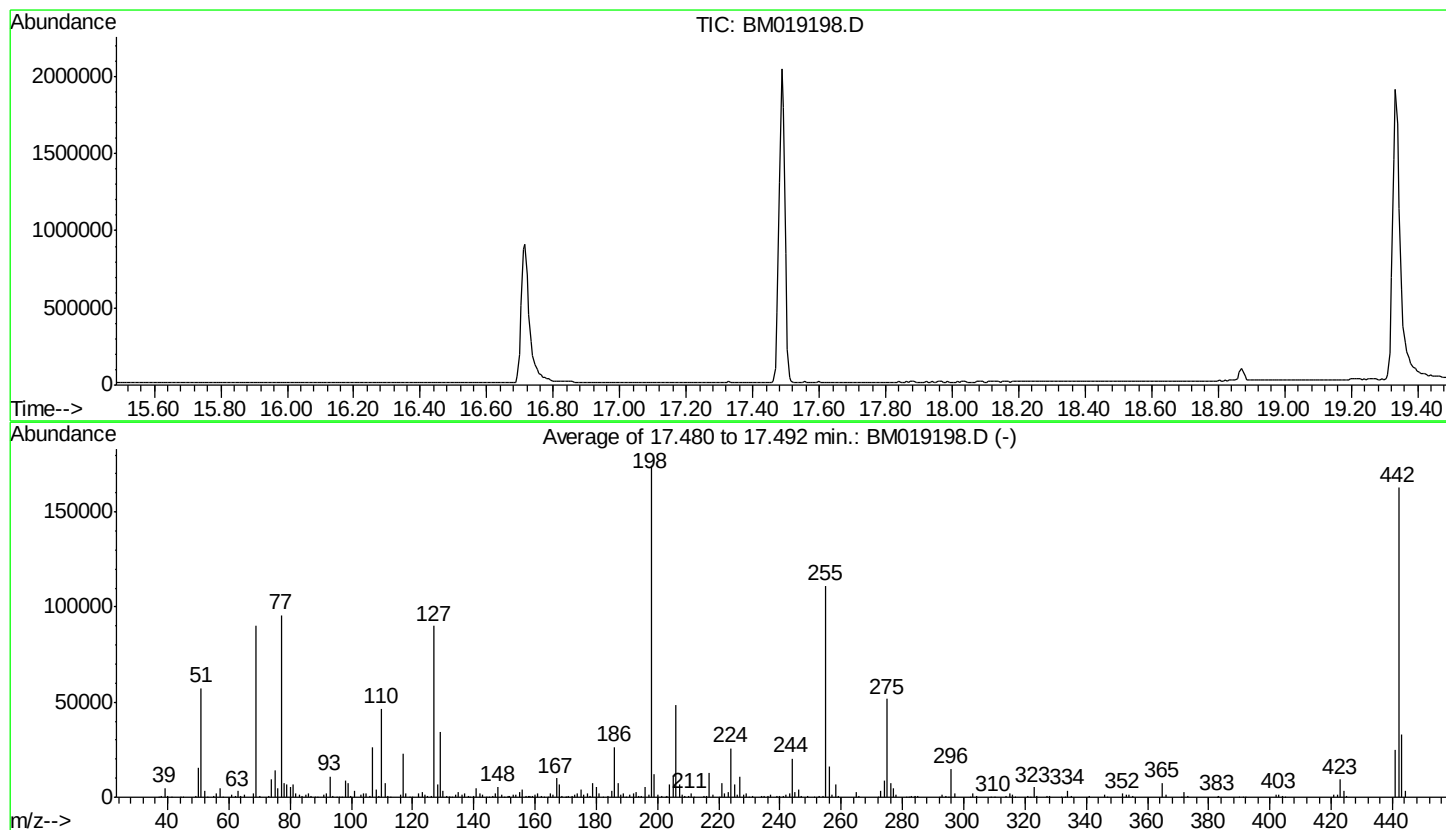

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	57200	PASS
68	69	0.00	2	2.0	1768	PASS
69	198	0.00	100	51.7	90189	PASS
70	69	0.00	2	0.6	499	PASS
127	198	10	80	51.6	89957	PASS
197	198	0.00	2	0.7	1135	PASS
198	198	100	100	100.0	174293	PASS
199	198	5	9	7.1	12365	PASS
275	198	10	60	29.6	51538	PASS
365	198	1	100	4.3	7477	PASS
441	198	0.01	100	14.2	24742	PASS
442	198	50	100	93.2	162512	PASS
443	442	15	24	20.1	32701	PASS