
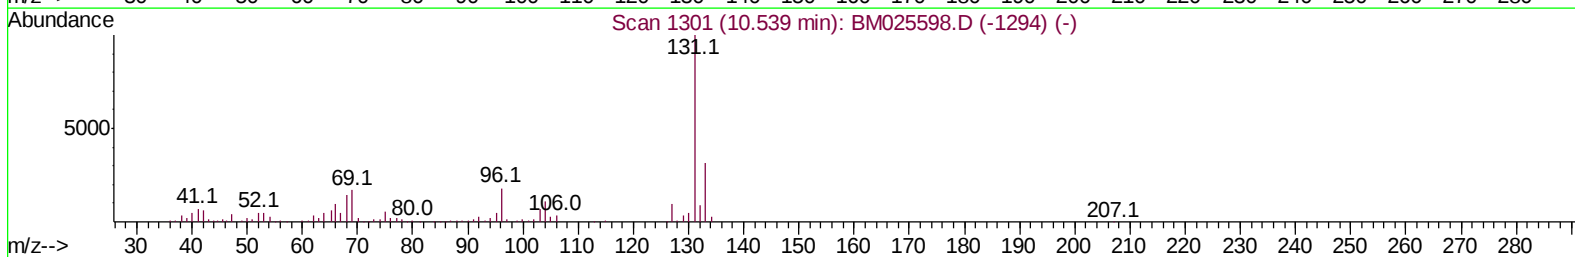
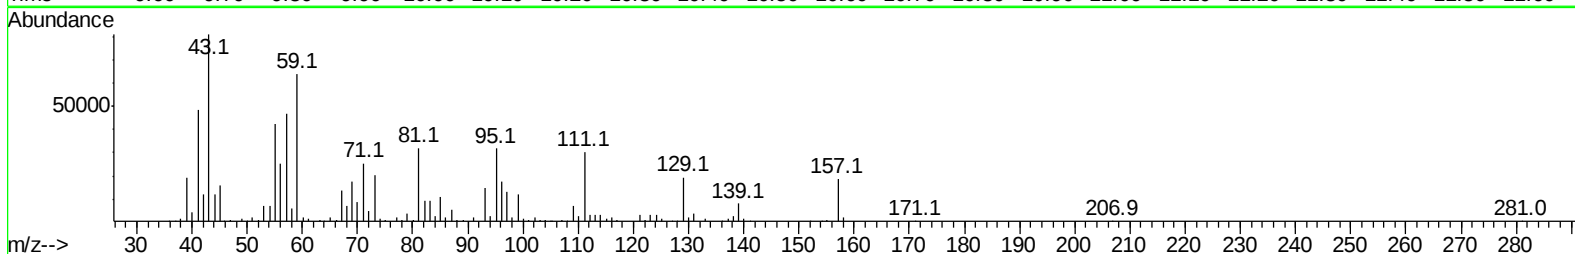


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031620\
Data File : BM025599.D
Acq On : 17 Mar 2020 03:41
Operator : CG/JU
Sample : L1840-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Mar 17 07:35:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 17 07:33:38 2020
Response via : Initial Calibration

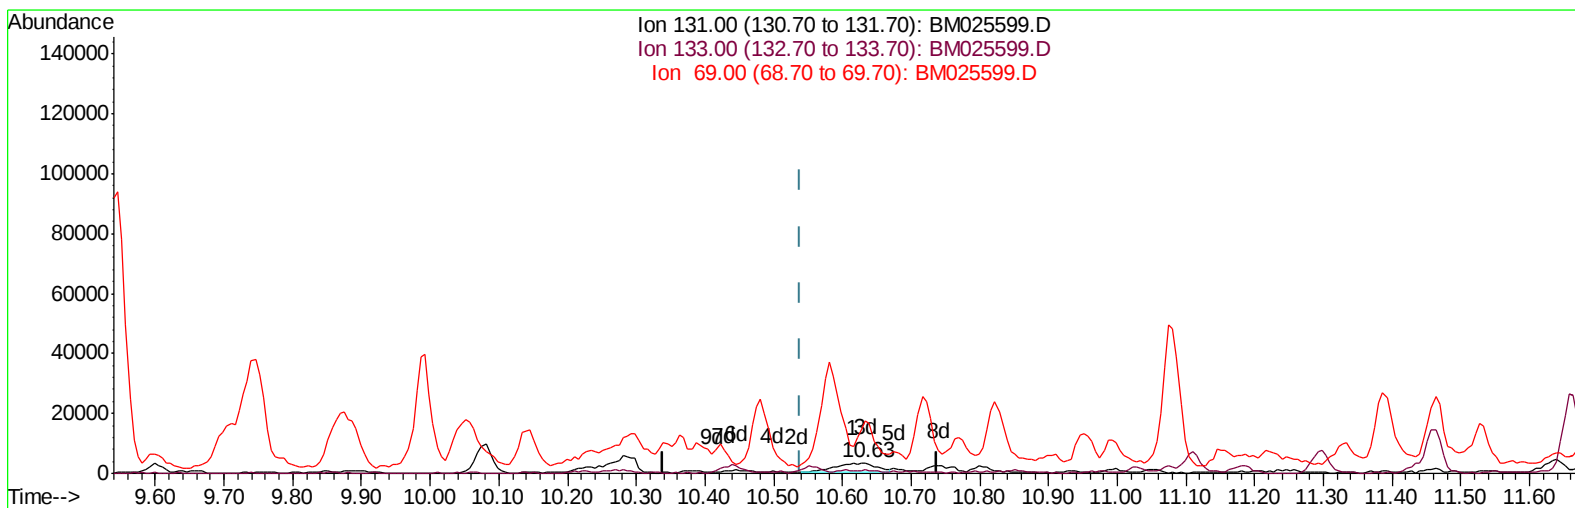

TIC: BM025599.D

(29) 4-Chloroaniline-d4 (S)

10.634min (+0.094) 1.11ng/ul m

response 13954

Ion	Exp%	Act%
131.00	100	100
133.00	32.10	32.91
69.00	17.20	488.83#
0.00	0.00	0.00