

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031620\
 Data File : BM025582.D
 Acq On : 16 Mar 2020 16:21
 Operator : CG/JU
 Sample : L1906-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0AG4

Quant Time: Mar 16 16:52:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 16 04:27:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	222732	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	965395	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	610334	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1290712	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	1243840	20.00	ng/ul	0.00
86) Perylene-d12	23.38	264	1438124	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	26271	4.95	ng/uL	0.00
5) Phenol-d5	6.82	99	521727	29.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	322847	32.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	448636	31.45	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	442225	30.62	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	228048	31.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	253915	33.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	462432	29.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	642099	35.45	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1457102	31.41	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1777600	31.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	230579	26.11	ng/ul	0.00
58) Fluorene-d10	15.27	176	1271404	31.23	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	178609	22.68	ng/ul	0.00
71) Anthracene-d10	17.11	188	1913527	31.74	ng/ul	0.00
79) Pyrene-d10	19.41	212	2037204	34.10	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.24	264	2400936	32.61	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.73	163	261594	5.418	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031620\
Data File : BM025582.D
Acq On : 16 Mar 2020 16:21
Operator : CG/JU
Sample : L1906-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B0AG4

Quant Time: Mar 16 16:52:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 16 04:27:51 2020
Response via : Initial Calibration

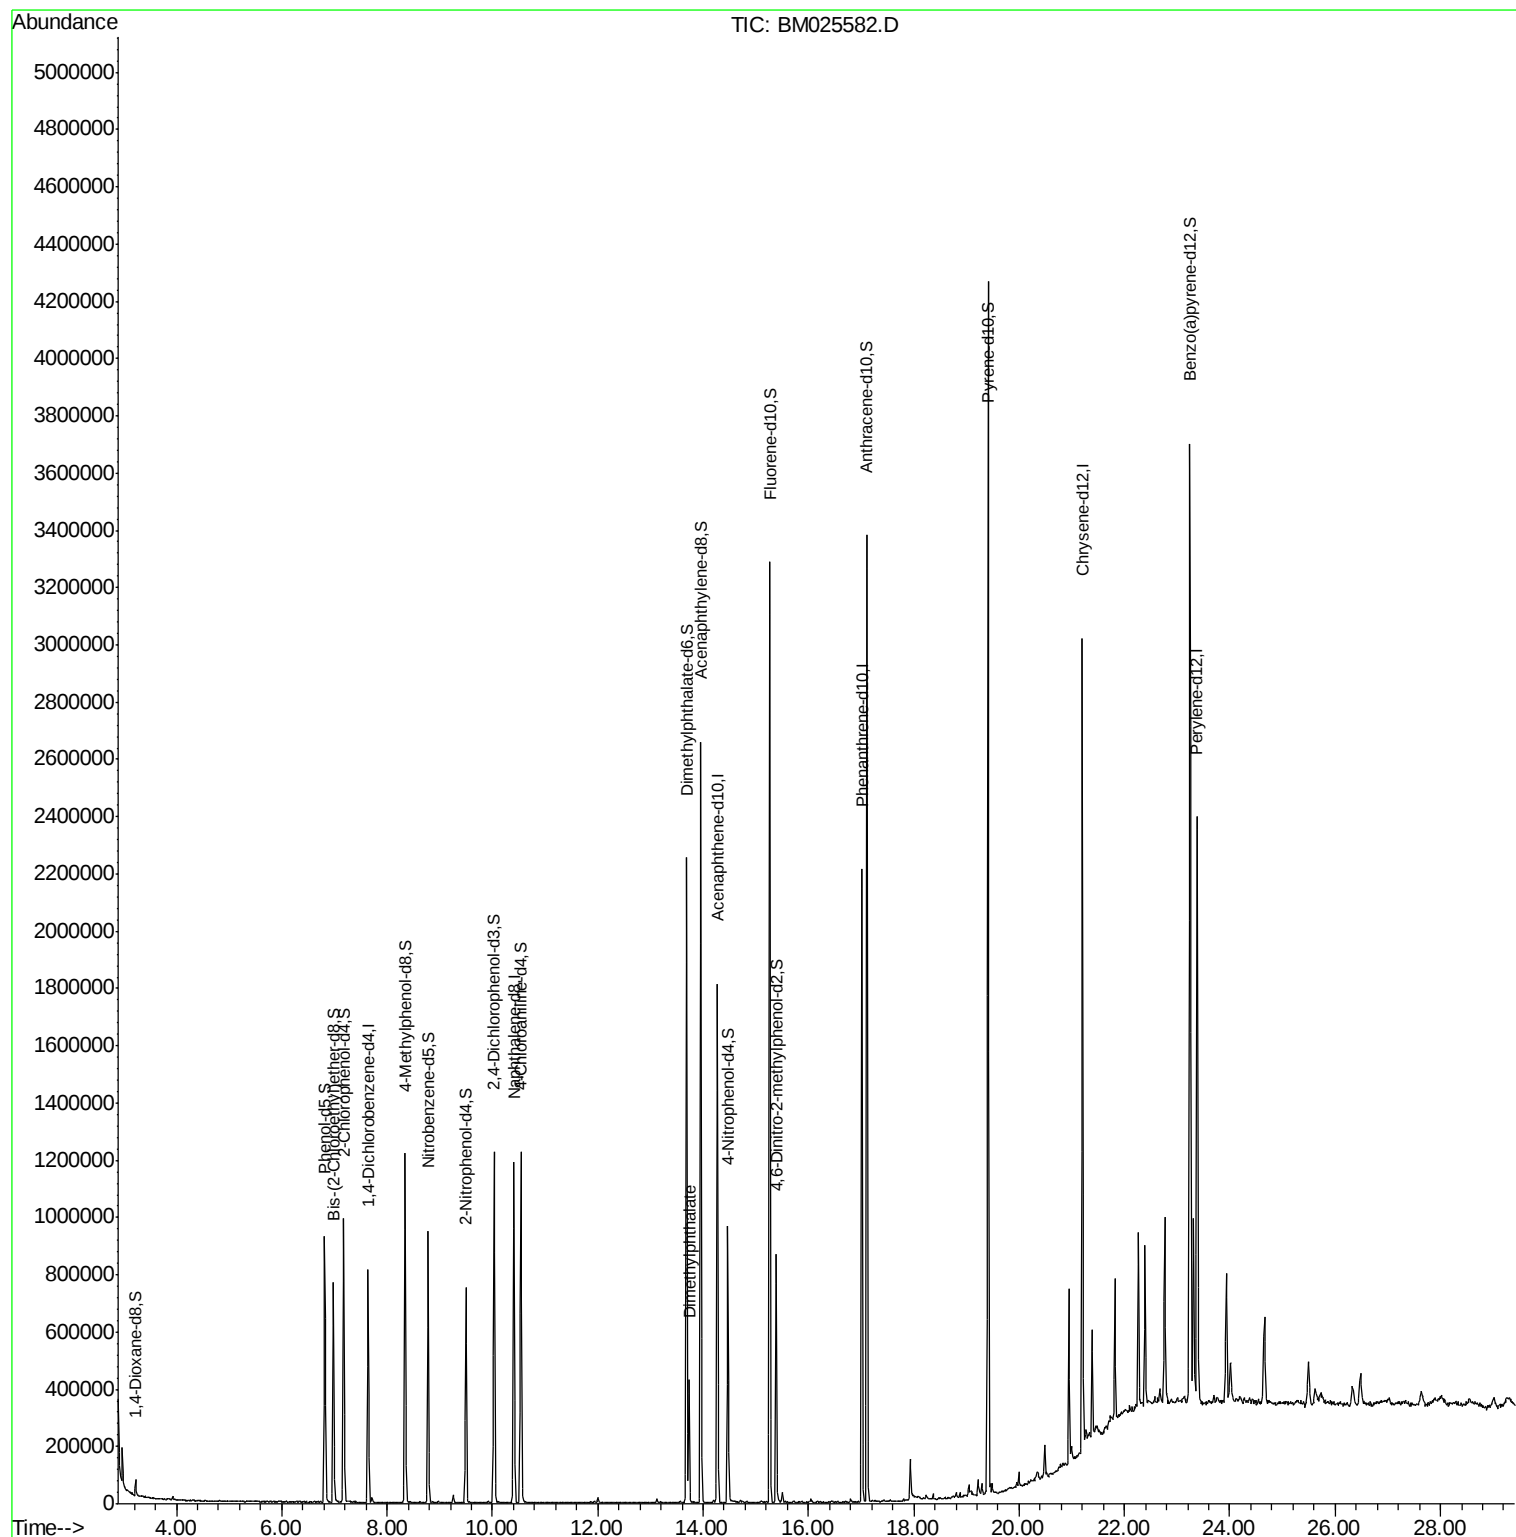

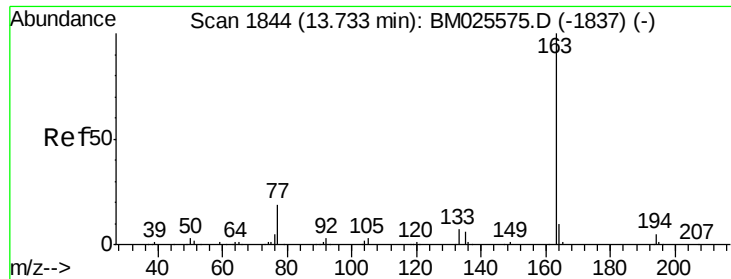

#45

Dimethylphthalate

Concen: 5.418 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. 0.00 min

Lab File: BM025582.D

Acq: 16 Mar 2020 16:21

Instrument :

BNA_M

ClientSampleId :

B0AG4


Tot Ion:163 Resp: 261594

Ion Ratio Lower Upper

163 100

194 4.5 3.5 5.3

164 9.7 8.2 12.4

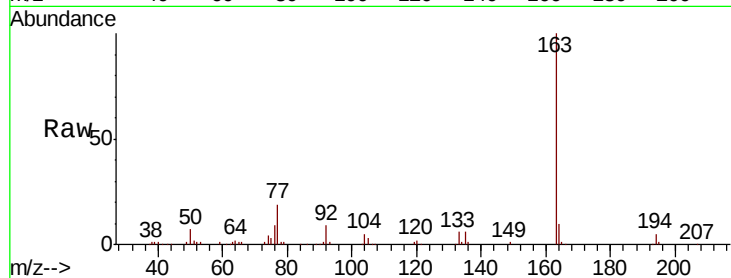

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

