
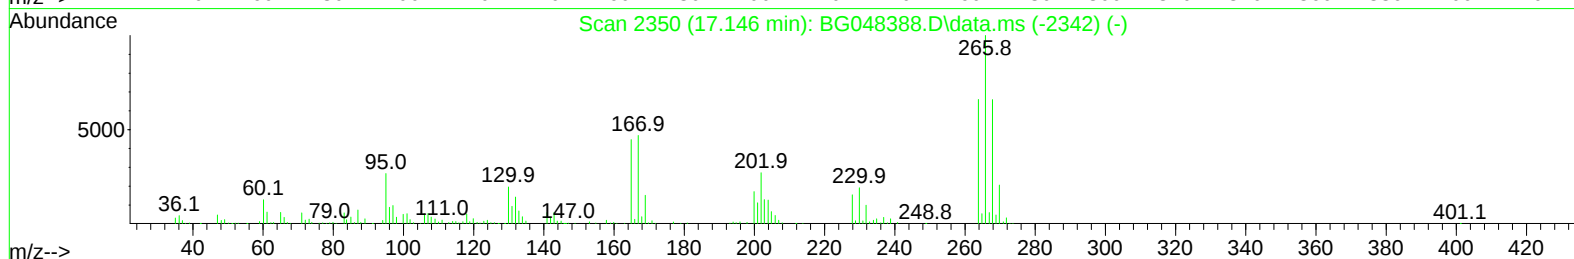
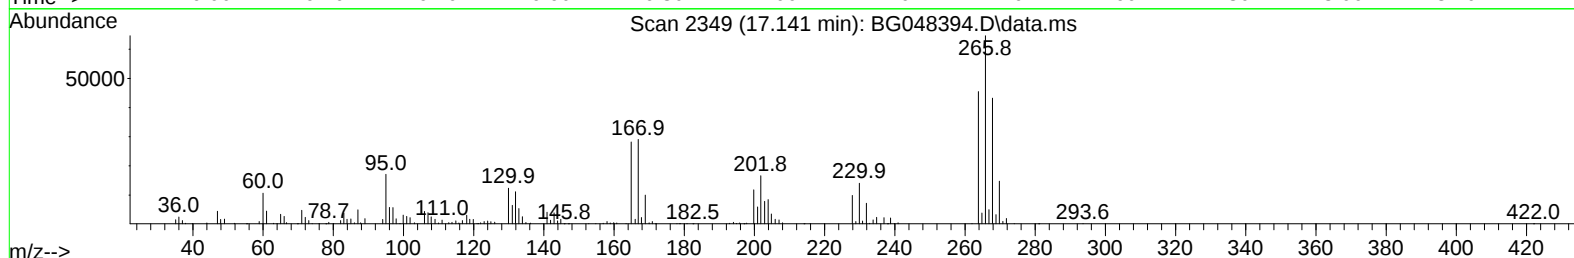


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG031721\  
Data File : BG048394.D  
Acq On : 17 Mar 2021 12:08  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 13:09:28 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG031621.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Mar 16 16:05:10 2021  
Response via : Initial Calibration

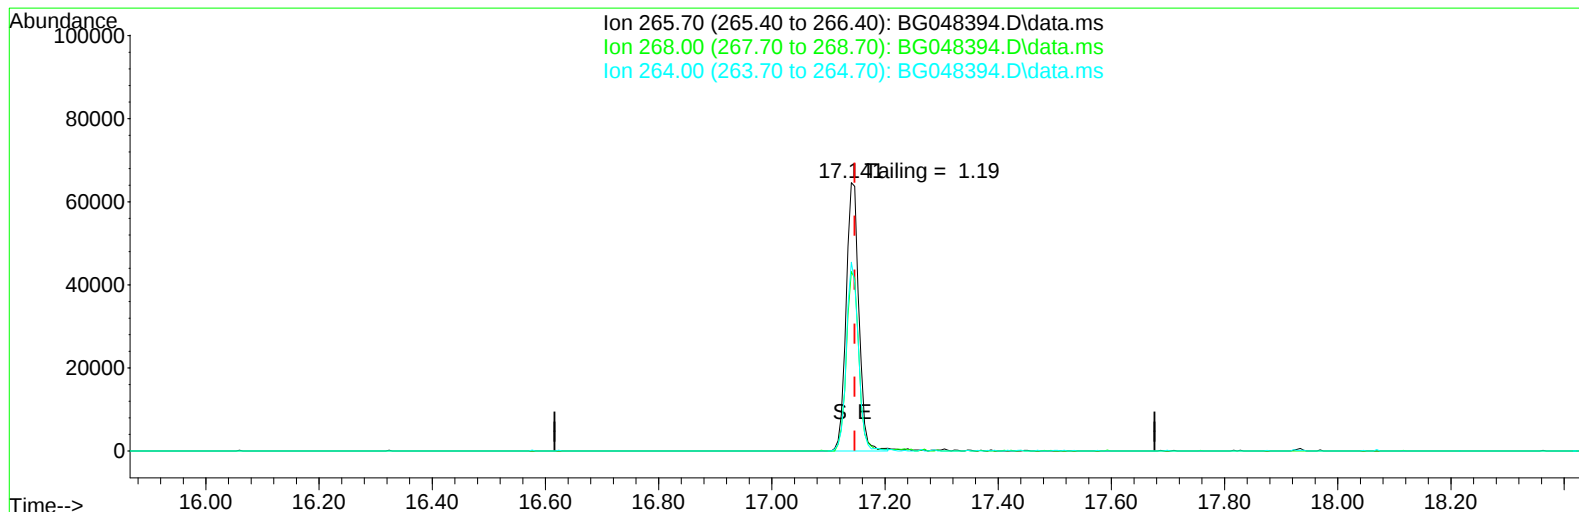

TIC: BG048394.D\data.ms

**(70) Pentachlorophenol (C)**

17.141min (-0.005) 225311.60 ng

response 100691

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 66.87  |
| 264.00 | 61.60  | 70.36  |
| 0.00   | 0.00   | 0.00   |