
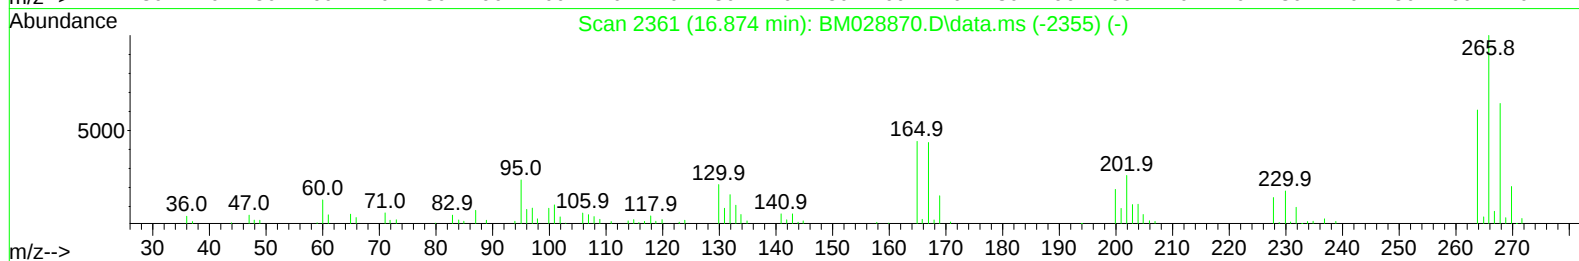
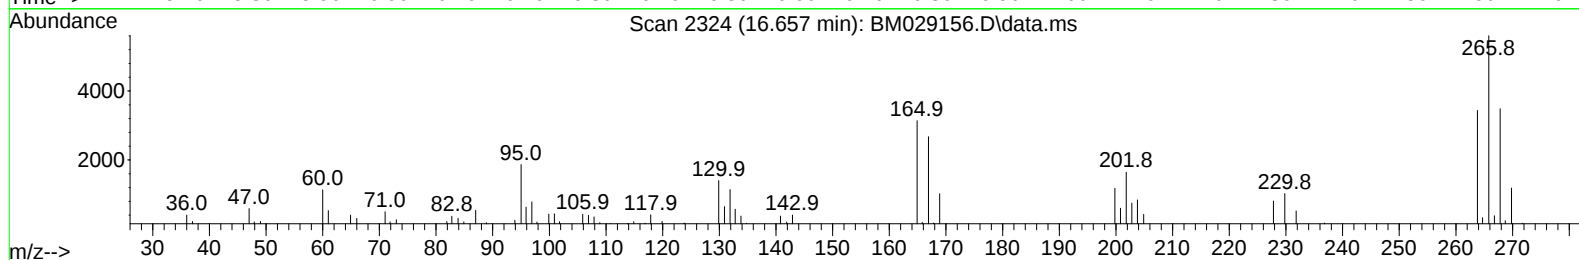


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031721\
Data File : BM029156.D
Acq On : 17 Mar 2021 11:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 12:55:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 17 12:48:14 2021
Response via : Initial Calibration

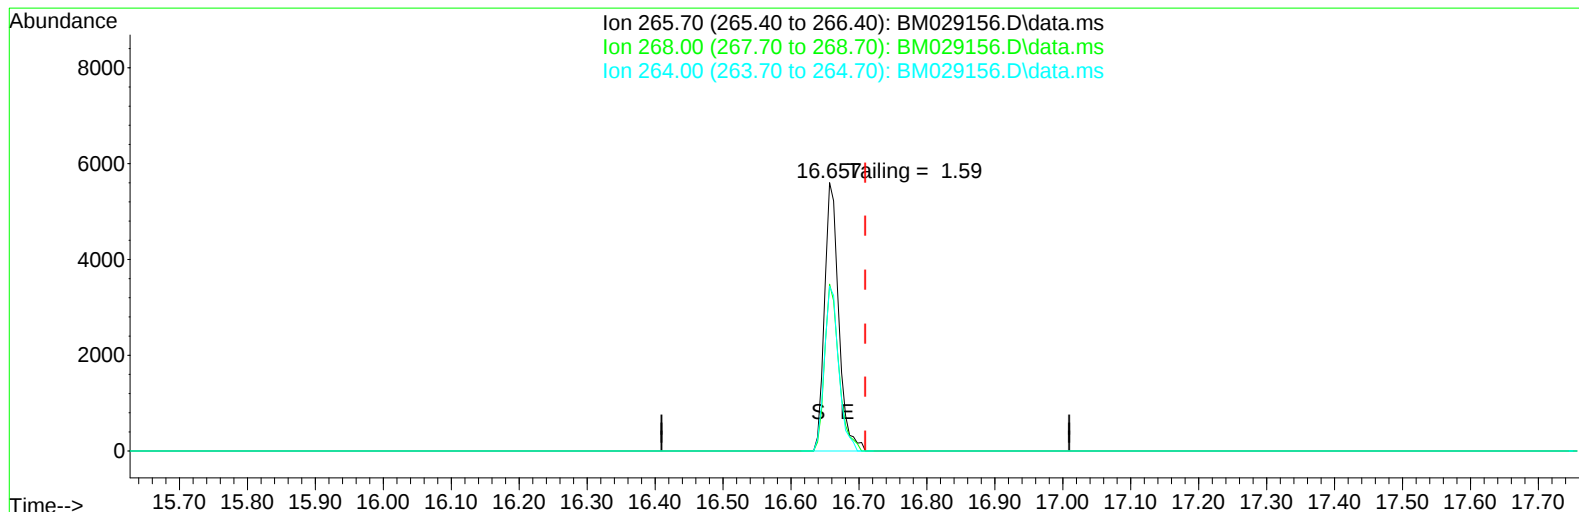

TIC: BM029156.D\data.ms

(70) Pentachlorophenol (C)

16.657min (-0.053) 0.00 ng

response 8129

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	66.48
264.00	63.30	67.14
0.00	0.00	0.00