
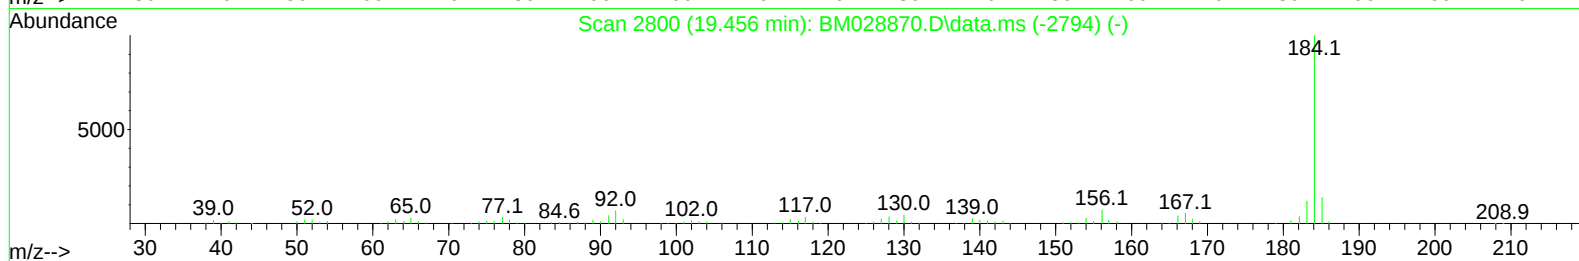
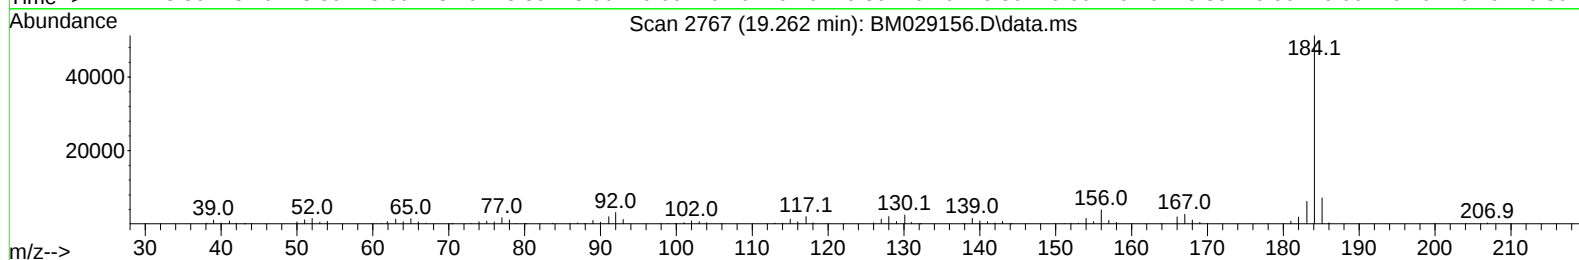


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031721\
Data File : BM029156.D
Acq On : 17 Mar 2021 11:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 12:55:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 17 12:48:14 2021
Response via : Initial Calibration

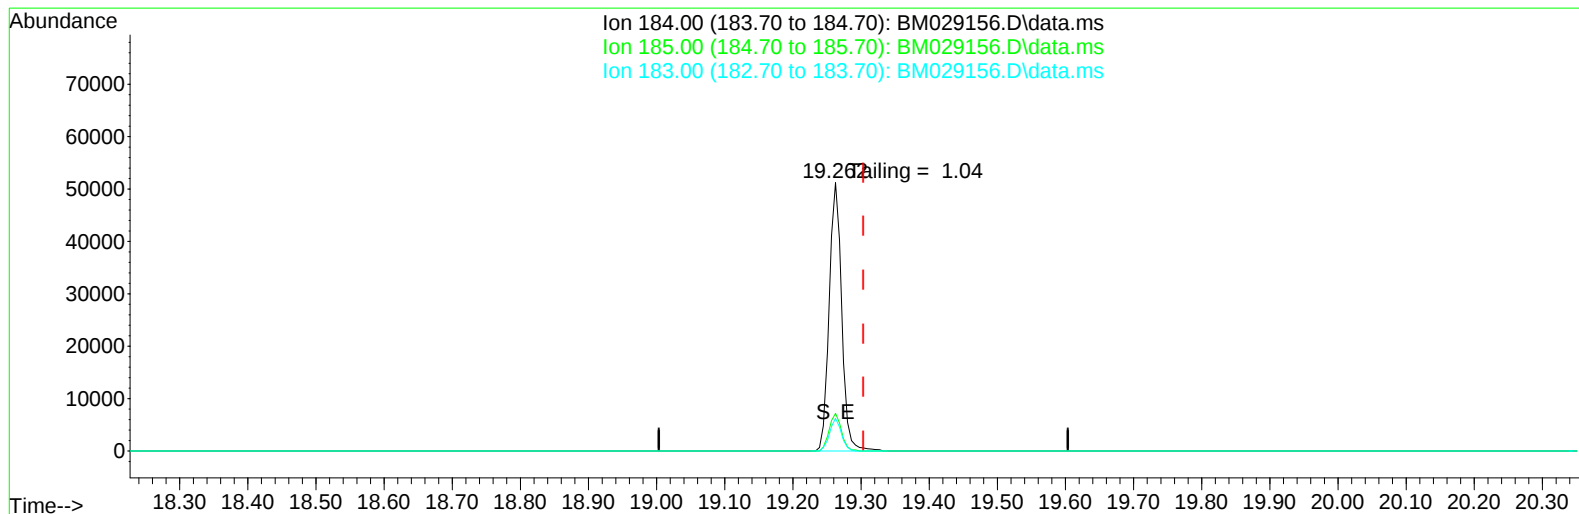

TIC: BM029156.D\data.ms

(77) Benzidine

19.262min (-0.041) 0.00 ng

response 65375

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.00
183.00	12.10	12.17
0.00	0.00	0.00