

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031721\
 Data File : BM029158.D
 Acq On : 17 Mar 2021 16:06
 Operator : CG/JU
 Sample : M1645-10
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.011	19	21	23	rVB	235	219	0.28%	0.069%
2	3.034	23	25	26	rBV	185	186	0.24%	0.058%
3	3.093	34	35	38	rBB	177	175	0.22%	0.055%
4	3.122	39	40	42	rBB	159	111	0.14%	0.035%
5	3.140	42	43	46	rBB	178	179	0.23%	0.056%
6	3.193	50	52	54	rBB	162	165	0.21%	0.052%
7	7.563	791	795	803	rBB	19234	29745	38.18%	9.327%
8	10.351	1263	1269	1278	rBB	25832	39865	51.17%	12.501%
9	14.239	1925	1930	1936	rBB	33531	45339	58.20%	14.217%
10	16.992	2393	2398	2405	rBB	38645	49454	63.48%	15.507%
11	18.092	2583	2585	2586	rBB	180	118	0.15%	0.037%
12	18.345	2626	2628	2629	rBB	180	117	0.15%	0.037%
13	18.398	2635	2637	2638	rBB	215	131	0.17%	0.041%
14	18.421	2639	2641	2643	rBB	198	123	0.16%	0.039%
15	18.451	2643	2646	2647	rBB	169	174	0.22%	0.055%
16	18.486	2651	2652	2654	rBB	165	115	0.15%	0.036%
17	18.504	2654	2655	2656	rBV	161	112	0.14%	0.035%
18	18.563	2663	2665	2667	rVB	221	195	0.25%	0.061%
19	18.580	2667	2668	2670	rBB	227	146	0.19%	0.046%
20	18.598	2670	2671	2672	rBV	220	149	0.19%	0.047%
21	18.633	2675	2677	2680	rVB	198	261	0.34%	0.082%
22	18.674	2682	2684	2687	rBV	216	341	0.44%	0.107%
23	18.880	2717	2719	2724	rBV	125	187	0.24%	0.059%
24	18.951	2728	2731	2733	rBV	124	89	0.11%	0.028%
25	19.162	2766	2767	2769	rBV	164	115	0.15%	0.036%
26	19.262	2781	2784	2785	rBV	75	85	0.11%	0.027%
27	19.315	2791	2793	2794	rBV	253	108	0.14%	0.034%
28	19.368	2800	2802	2804	rBV	120	121	0.16%	0.038%
29	19.427	2809	2812	2813	rBV	160	135	0.17%	0.042%
30	19.445	2813	2815	2817	rVB	104	102	0.13%	0.032%
31	19.474	2817	2820	2822	rVB	108	121	0.16%	0.038%
32	19.510	2822	2826	2827	rBV	171	191	0.25%	0.060%
33	19.533	2829	2830	2833	rBV	117	114	0.15%	0.036%
34	19.651	2849	2850	2852	rBV	264	172	0.22%	0.054%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031721\
 Data File : BM029158.D
 Acq On : 17 Mar 2021 16:06
 Operator : CG/JU
 Sample : M1645-10
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION

35	19.698	2856	2858	2859	rVV	144	78	0.10%	0.024%
36	19.739	2864	2865	2867	rVB	336	210	0.27%	0.066%
37	19.762	2867	2869	2870	rBV	137	101	0.13%	0.032%
38	19.792	2873	2874	2877	rBV	190	152	0.20%	0.048%
39	19.839	2880	2882	2884	rBV	429	204	0.26%	0.064%
40	19.857	2884	2885	2887	rVB	287	199	0.26%	0.062%
41	19.886	2889	2890	2891	rVB	265	94	0.12%	0.029%
42	19.904	2891	2893	2894	rBV	559	334	0.43%	0.105%
43	19.921	2894	2896	2897	rVB	311	210	0.27%	0.066%
44	19.933	2897	2898	2899	rVB	557	197	0.25%	0.062%
45	19.951	2899	2901	2902	rBV	407	294	0.38%	0.092%
46	20.051	2917	2918	2920	rVB	391	176	0.23%	0.055%
47	20.068	2920	2921	2925	rVB	510	522	0.67%	0.164%
48	20.098	2925	2926	2927	rBV	575	389	0.50%	0.122%
49	20.186	2938	2941	2943	rBV3	428	584	0.75%	0.183%
50	20.292	2957	2959	2960	rBV	532	315	0.40%	0.099%
51	20.345	2966	2968	2970	rBV2	285	219	0.28%	0.069%
52	20.374	2971	2973	2976	rVV2	381	357	0.46%	0.112%
53	20.433	2981	2983	2985	rBV	324	306	0.39%	0.096%
54	20.451	2985	2986	2987	rBV	490	200	0.26%	0.063%
55	20.492	2991	2993	2995	rBV2	417	412	0.53%	0.129%
56	20.580	3006	3008	3010	rBV	478	354	0.45%	0.111%
57	20.604	3010	3012	3013	rVB2	564	360	0.46%	0.113%
58	20.633	3013	3017	3019	rVB2	675	855	1.10%	0.268%
59	20.651	3019	3020	3022	rBV	545	498	0.64%	0.156%
60	20.704	3026	3029	3031	rBV3	626	699	0.90%	0.219%
61	20.721	3031	3032	3033	rVB	806	285	0.37%	0.089%
62	20.745	3033	3036	3037	rBV2	1007	1114	1.43%	0.349%
63	20.774	3040	3041	3042	rVB	708	250	0.32%	0.078%
64	20.798	3042	3045	3046	rBV2	922	1001	1.28%	0.314%
65	20.856	3051	3055	3056	rBV3	704	806	1.03%	0.253%
66	21.180	3106	3110	3115	rBV	52210	60271	77.37%	18.899%
67	23.303	3465	3471	3479	rVB2	45958	77901	100.00%	24.427%


Sum of corrected areas: 318907

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031721\
Data File : BM029158.D
Acq On : 17 Mar 2021 16:06
Operator : CG/JU
Sample : M1645-10
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

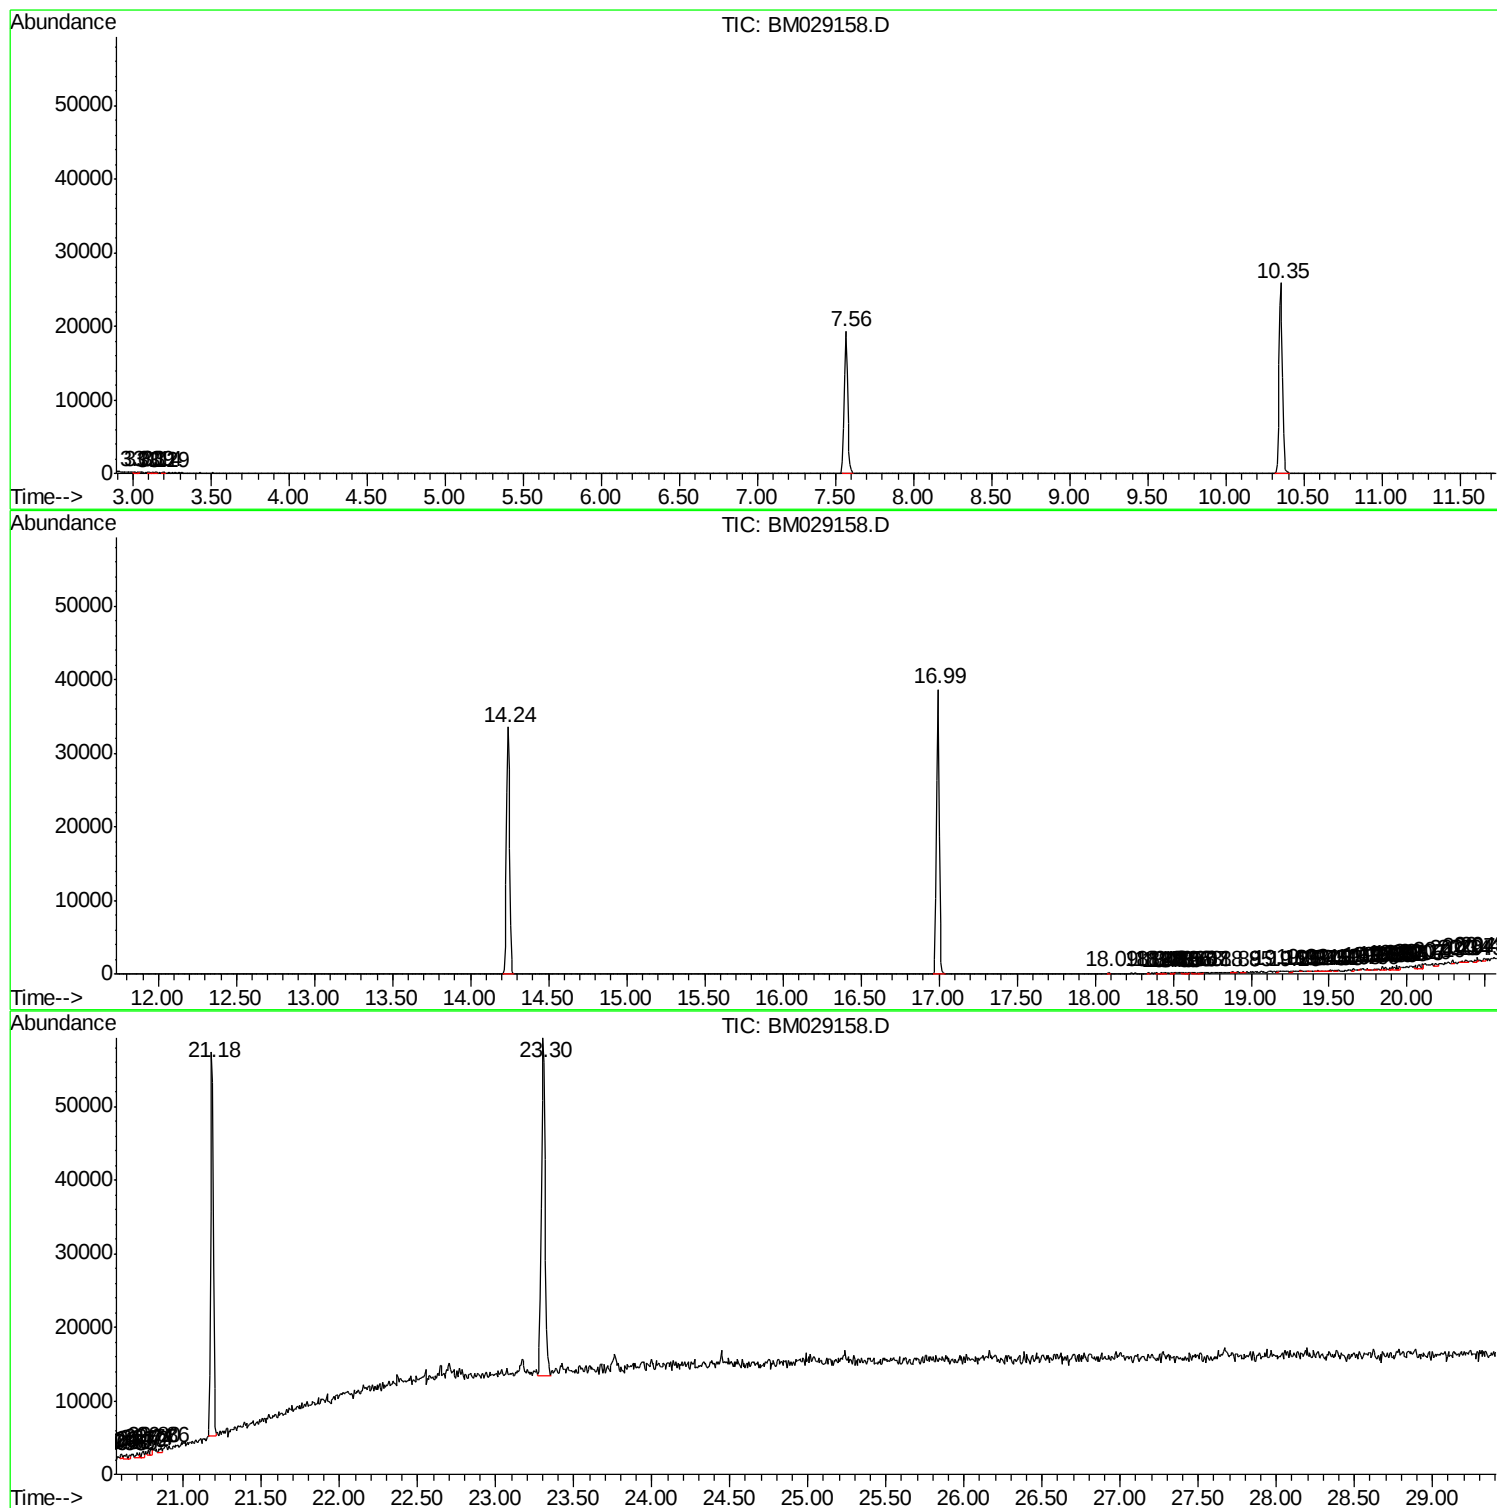

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031721\
Data File : BM029158.D
Acq On : 17 Mar 2021 16:06
Operator : CG/JU
Sample : M1645-10
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031721\
Data File : BM029158.D
Acq On : 17 Mar 2021 16:06
Operator : CG/JU
Sample : M1645-10
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc