


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031721\
 Data File : BM029156.D
 Acq On : 17 Mar 2021 13:43
 Operator : CG/JU
 Sample : DFTPP41
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP41

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION
 Last Update : Wed Mar 17 15:12:40 2021

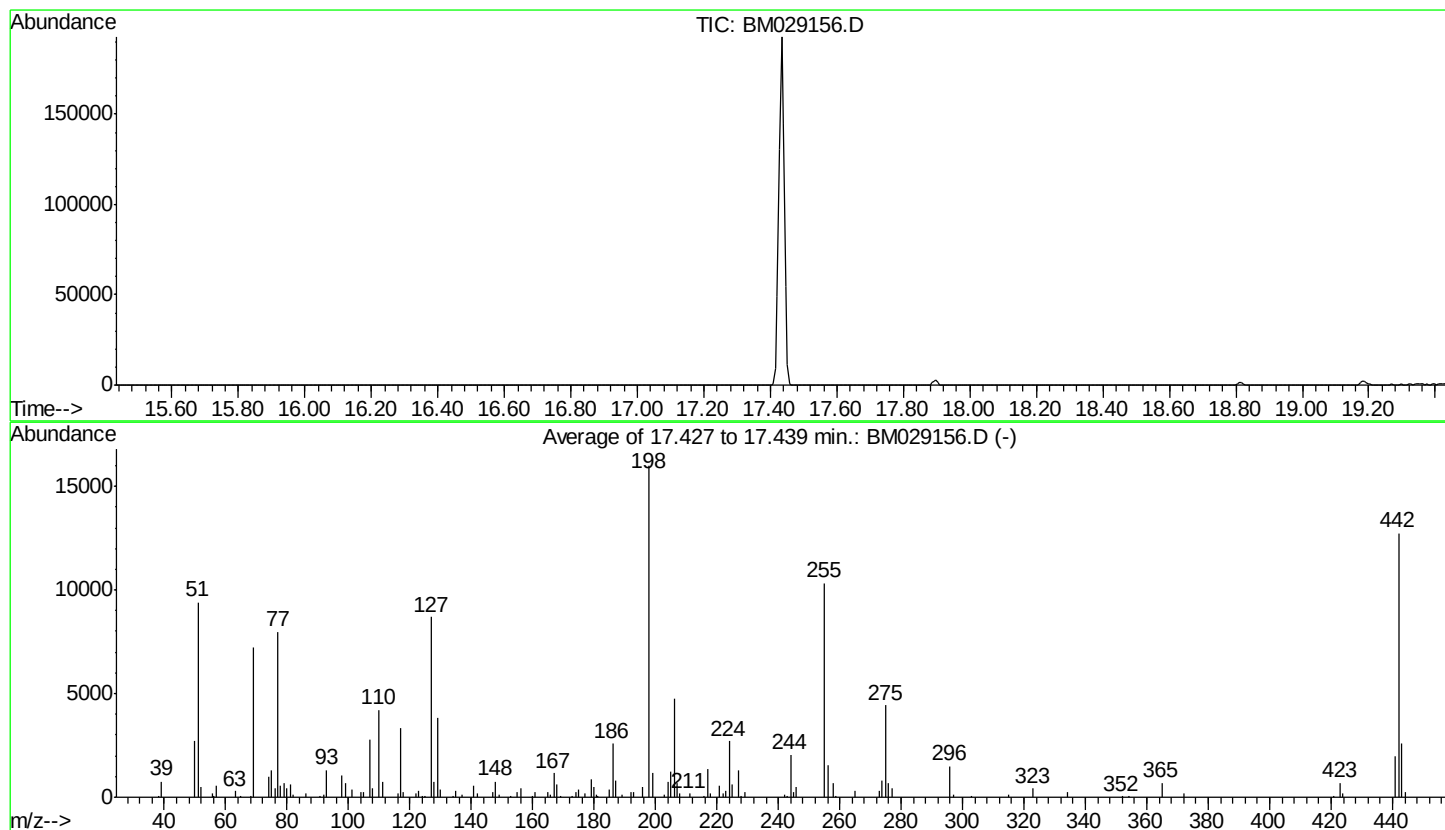

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.8	9405	PASS
68	69	0.00	2	0.8	59	PASS
69	198	0.00	100	45.2	7231	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.4	8696	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15999	PASS
199	198	5	9	7.2	1158	PASS
275	198	10	60	27.8	4444	PASS
365	198	1	100	4.3	690	PASS
441	198	0.01	100	12.3	1971	PASS
442	198	50	100	79.6	12736	PASS
443	442	15	24	20.5	2609	PASS

m/z

Abundance

Instrument :

BNA_M

ClientSampleId :

DFTPP41

m/z	Abundance
39.10	679.0
50.00	2745.0
51.00	9030.0
52.00	567.0
55.90	276.0
57.00	567.0
63.00	292.0
69.00	6865.0
74.00	883.0
75.00	1204.0
76.10	370.0
77.10	7578.0
78.00	530.0
79.00	687.0
79.90	413.0
81.00	675.0
81.90	150.0
85.90	160.0
92.90	1180.0
97.90	1008.0
98.90	792.0
101.00	311.0
103.90	195.0
105.00	234.0
107.00	2527.0
108.00	416.0
110.00	3940.0
111.00	695.0
116.10	160.0
117.00	3121.0
118.00	218.0
122.00	159.0
123.00	303.0
127.00	7643.0
128.00	625.0
129.00	3572.0
129.90	334.0
134.90	253.0
136.90	175.0
140.90	430.0
141.90	174.0
146.90	249.0
147.90	669.0
155.00	254.0
156.00	404.0
160.90	150.0
164.90	164.0
167.00	1031.0
168.00	544.0
173.90	191.0
175.00	304.0
176.90	156.0
178.90	666.0
180.00	444.0
180.90	190.0
185.00	289.0
186.00	2242.0
186.90	605.0
191.90	207.0
193.00	196.0
195.90	425.0
197.90	13238.0
198.90	1110.0
204.00	568.0
205.00	1093.0
206.00	3983.0
207.00	591.0
207.90	202.0
211.00	151.0
217.00	1126.0
217.90	171.0
221.00	536.0
221.80	160.0
223.00	249.0
224.00	2115.0
225.00	509.0
227.00	1135.0
228.90	184.0
244.00	1651.0
245.00	236.0
245.90	365.0
255.00	7972.0
256.00	1271.0
257.90	564.0
265.00	208.0
272.90	198.0
273.90	686.0
275.00	3434.0
276.00	554.0
277.00	300.0
296.00	1157.0
323.00	327.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

334.00	195.0
365.00	548.0
423.00	439.0
423.90	158.0
441.10	1275.0
442.00	8096.0
443.00	1714.0
444.00	177.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

m/z	Abundance
38.00	165.0
39.00	1019.0
50.00	3334.0
51.00	11685.0
52.00	603.0
55.90	291.0
57.00	761.0
63.00	351.0
65.00	161.0
68.10	179.0
69.00	9024.0
74.00	1260.0
75.00	1637.0
76.00	681.0
77.00	9921.0
78.00	617.0
79.00	858.0
80.00	562.0
81.00	727.0
82.00	182.0
85.90	287.0
90.90	192.0
92.00	271.0
93.00	1582.0
98.00	1183.0
98.90	866.0
100.90	426.0
103.90	291.0
104.90	331.0
107.00	3395.0
108.00	438.0
110.00	5235.0
111.00	862.0
115.90	181.0
117.00	4070.0
117.90	322.0
122.00	284.0
122.90	405.0
123.90	173.0
124.90	165.0
127.00	10799.0
128.00	909.0
129.00	4600.0
129.90	469.0
133.90	151.0
135.00	421.0
137.00	183.0
140.90	740.0
141.90	179.0
147.00	344.0
148.00	942.0
148.90	226.0
152.90	204.0
154.90	338.0
156.00	465.0
160.00	192.0
160.90	301.0
164.90	261.0
165.90	216.0
167.00	1438.0
168.00	745.0
169.00	157.0
172.90	170.0
173.90	275.0
174.90	489.0
176.90	248.0
178.90	1055.0
179.90	642.0
181.10	241.0
184.90	395.0
186.00	3020.0
187.00	1139.0
189.00	220.0
192.00	282.0
192.90	368.0
196.00	666.0
197.90	19840.0
198.90	1377.0
202.90	168.0
204.00	1007.0
205.00	1518.0
206.00	5819.0
207.00	768.0
207.90	194.0
211.00	225.0
215.90	159.0
216.90	1751.0
218.00	223.0
220.90	595.0
221.90	209.0
222.90	351.0
224.00	3266.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

225.00	840.0
226.90	1595.0
228.00	210.0
228.90	273.0
241.90	217.0
243.00	230.0
244.00	2565.0
245.00	329.0
246.00	656.0
255.00	12857.0
256.00	1910.0
258.00	928.0
258.90	243.0
264.90	390.0
272.90	381.0
273.90	907.0
275.00	5336.0
275.90	830.0
276.90	561.0
296.00	1751.0
296.90	244.0
303.00	160.0
314.90	190.0
323.00	485.0
333.90	287.0
354.00	157.0
364.90	786.0
372.00	287.0
423.00	797.0
423.90	206.0
441.00	2256.0
442.00	14600.0
443.00	3064.0
444.10	272.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

m/z	Abundance
39.00	610.0
50.00	2133.0
51.00	7500.0
52.00	363.0
56.10	176.0
57.00	434.0
63.00	266.0
69.00	5804.0
74.00	869.0
75.00	1008.0
76.00	340.0
77.00	6459.0
78.00	442.0
79.00	555.0
80.00	413.0
81.00	436.0
86.00	161.0
91.90	190.0
93.00	1145.0
98.00	982.0
99.00	462.0
100.90	291.0
104.00	233.0
104.90	179.0
107.00	2357.0
107.90	423.0
110.00	3517.0
111.00	606.0
116.00	152.0
117.00	2861.0
117.90	157.0
122.00	155.0
123.00	272.0
127.00	7648.0
128.00	606.0
129.00	3380.0
129.90	315.0
135.00	243.0
140.90	514.0
141.80	151.0
146.90	225.0
148.00	683.0
149.00	151.0
154.90	234.0
156.00	383.0
161.00	238.0
164.90	232.0
166.00	171.0
167.00	987.0
167.90	522.0
174.00	198.0
175.00	341.0
177.00	180.0
178.90	878.0
179.90	438.0
180.90	224.0
185.00	384.0
186.00	2457.0
187.00	712.0
188.90	195.0
191.90	242.0
193.00	209.0
196.00	401.0
197.90	14921.0
198.90	987.0
202.90	159.0
204.00	629.0
205.00	1063.0
206.00	4450.0
206.90	648.0
207.90	161.0
211.00	157.0
216.90	1270.0
217.80	163.0
220.90	531.0
221.80	161.0
222.90	307.0
224.00	2726.0
225.00	595.0
226.90	1230.0
228.90	224.0
241.90	154.0
244.00	1903.0
244.90	263.0
246.00	467.0
255.00	10206.0
256.00	1495.0
257.90	642.0
264.90	309.0
272.90	338.0
273.90	836.0
275.00	4564.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

275.90	673.0
277.00	447.0
295.90	1576.0
297.00	217.0
314.90	181.0
323.00	436.0
334.00	265.0
351.90	166.0
364.90	737.0
372.00	215.0
420.80	154.0
423.00	861.0
423.90	188.0
441.00	2383.0
442.00	15514.0
443.00	3051.0
444.00	249.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41