
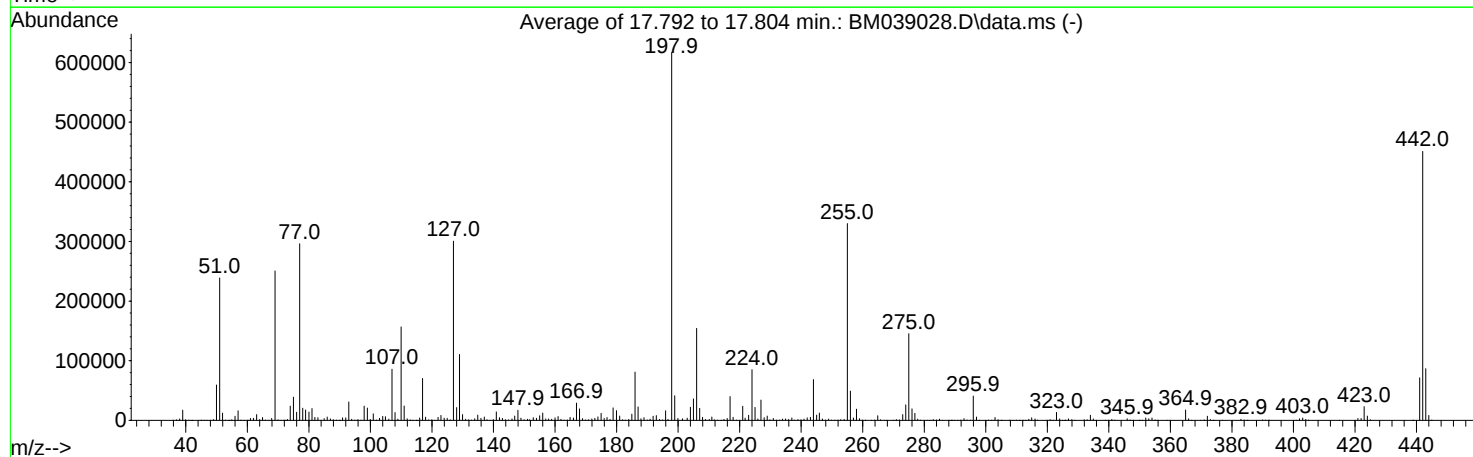


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031723\
 Data File : BM039028.D
 Acq On : 17 Mar 2023 09:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 17 05:25:34 2023

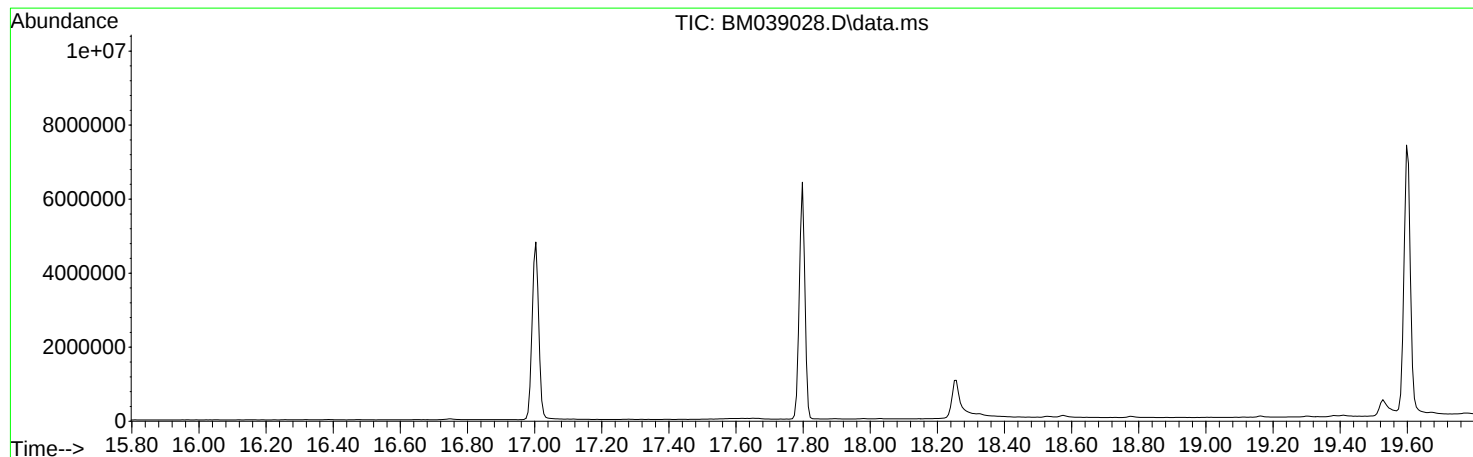

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	238810	PASS
68	69	0.00	2	1.3	3314	PASS
69	198	0.00	100	40.6	250511	PASS
70	69	0.00	2	0.5	1196	PASS
127	198	10	80	48.7	300480	PASS
197	198	0.00	2	0.3	1584	PASS
198	198	100	100	100.0	616789	PASS
199	198	5	9	6.7	41440	PASS
275	198	10	60	23.6	145496	PASS
365	198	1	100	2.8	17514	PASS
441	198	0.01	100	11.6	71272	PASS
442	442	50	100	100.0	451115	PASS
443	442	15	24	19.2	86771	PASS