

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031819\
 Data File : BM019217.D
 Acq On : 18 Mar 2019 16:03
 Operator : JU/SJ
 Sample : PB118000BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 19 07:21:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 11 17:30:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	186221	20.00	ng	-0.01
21) Naphthalene-d8	10.43	136	780659	20.00	ng	-0.02
39) Acenaphthene-d10	14.30	164	490563	20.00	ng	-0.02
64) Phenanthrene-d10	17.06	188	1043826	20.00	ng	-0.02
76) Chrysene-d12	21.26	240	763365	20.00	ng	-0.01
87) Perylene-d12	23.50	264	735334	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	1570426	136.57	ng	0.00
7) Phenol-d6	6.83	99	2283578	135.77	ng	-0.01
23) Nitrobenzene-d5	8.82	82	1382771	83.73	ng	-0.02
42) 2,4,6-Tribromophenol	15.80	330	885575	122.27	ng	-0.02
45) 2-Fluorobiphenyl	12.92	172	3169177	84.03	ng	-0.02
79) Terphenyl-d14	19.70	244	4330983	112.63	ng	-0.01


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031819\
Data File : BM019217.D
Acq On : 18 Mar 2019 16:03
Operator : JU/SJ
Sample : PB118000BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 19 07:21:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 11 17:30:46 2019
Response via : Initial Calibration

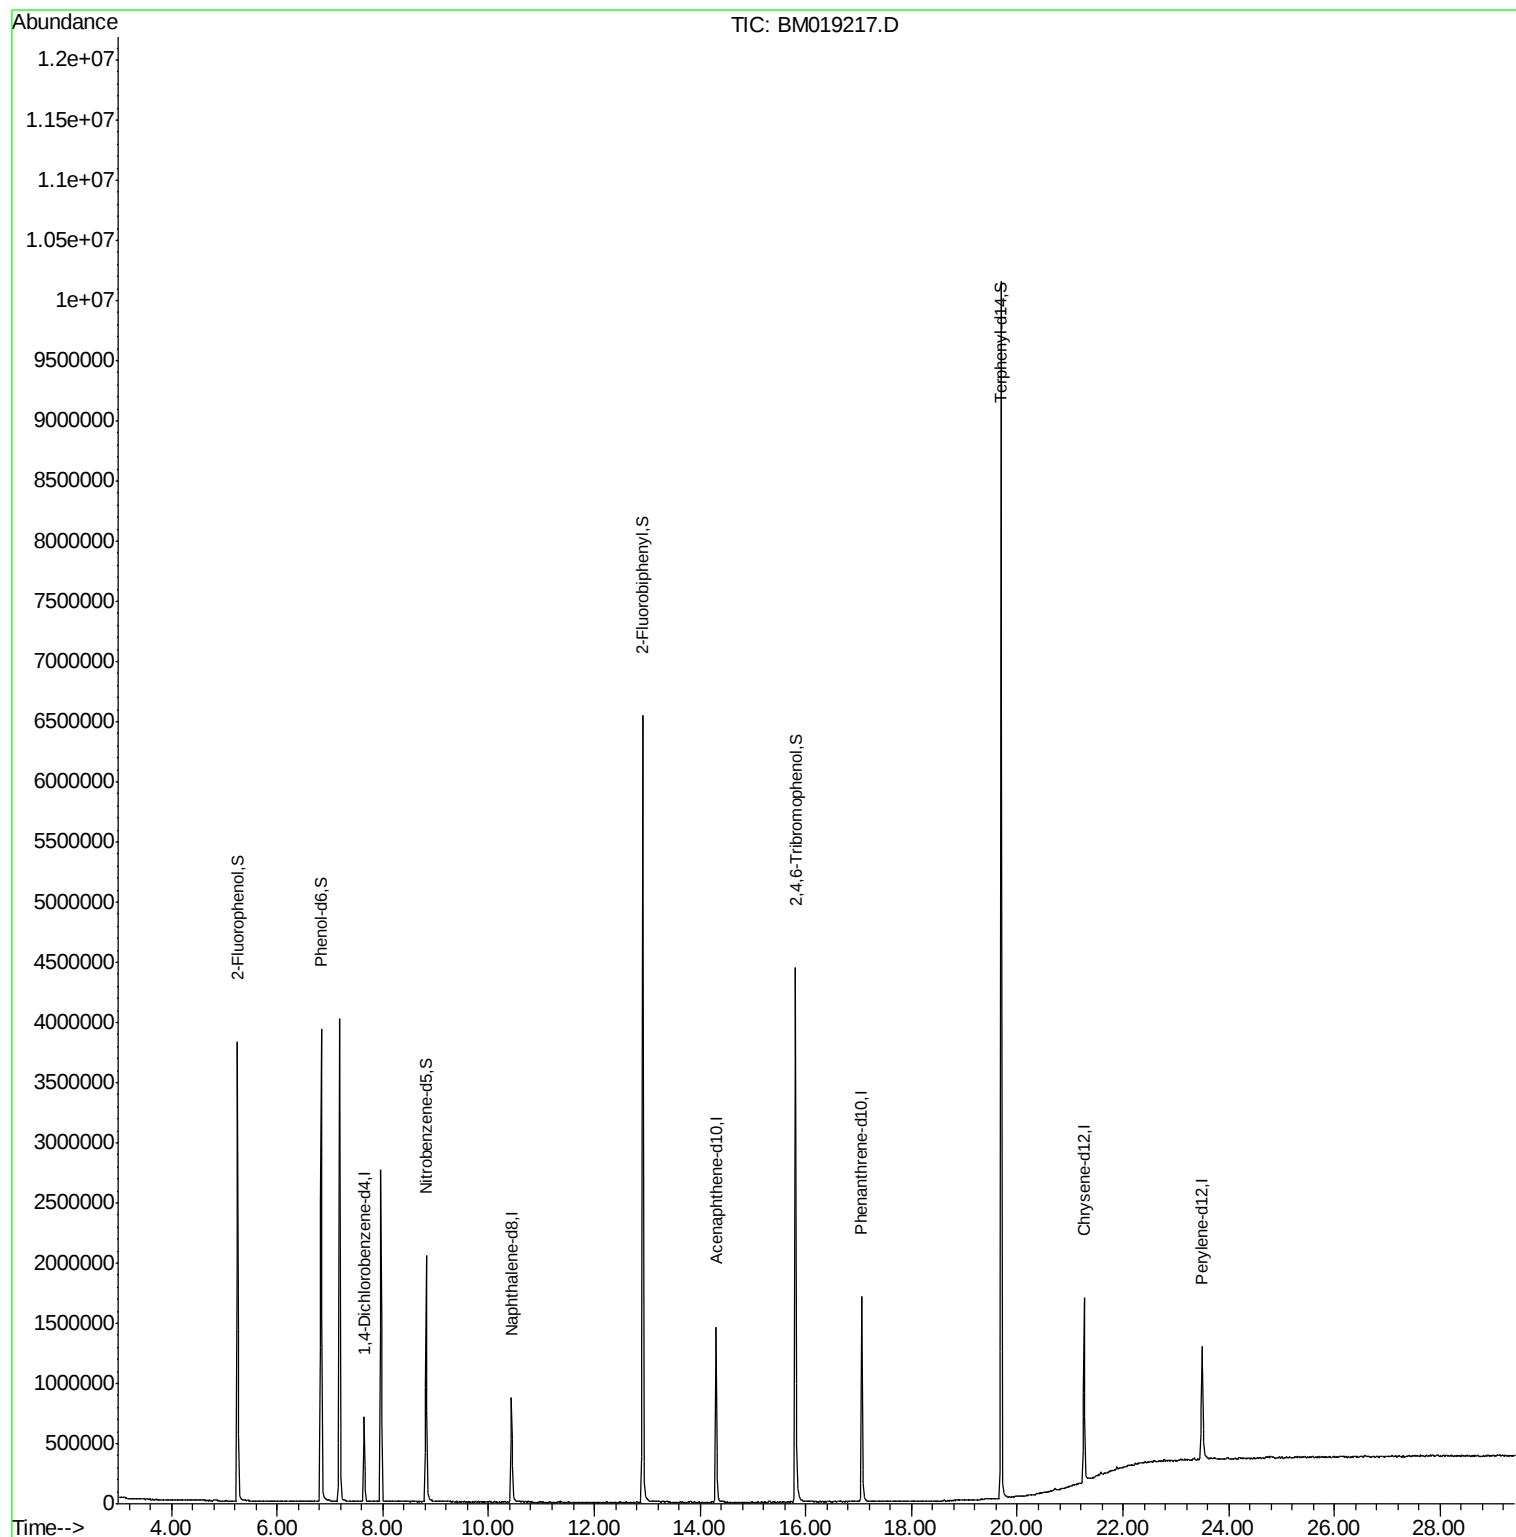




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.65 min Scan# 793
Delta R.T. -0.01 min
Lab File: BM019217.D
Acq: 18 Mar 2019 16:03

Instrument :
BNA_M
ClientSampled :

Tgt Ion:152 Resp: 186221
Ion Ratio Lower Upper
152 100
150 154.4 125.3 187.9
115 61.5 49.4 74.0

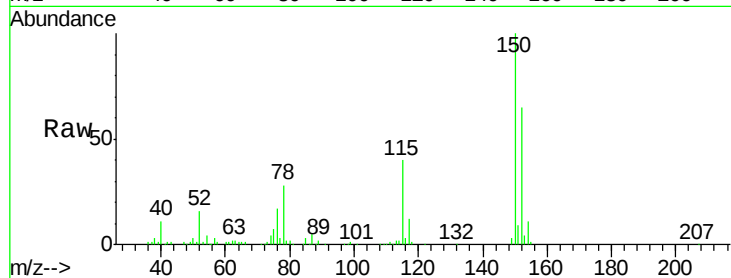


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

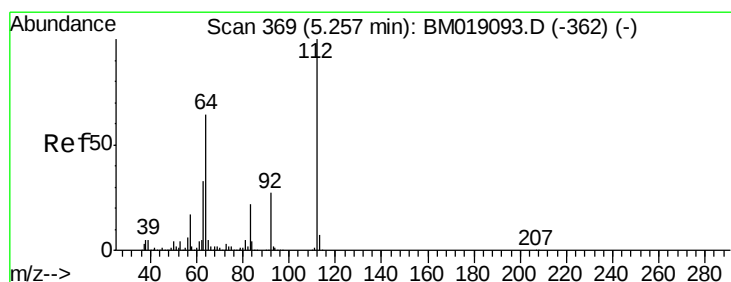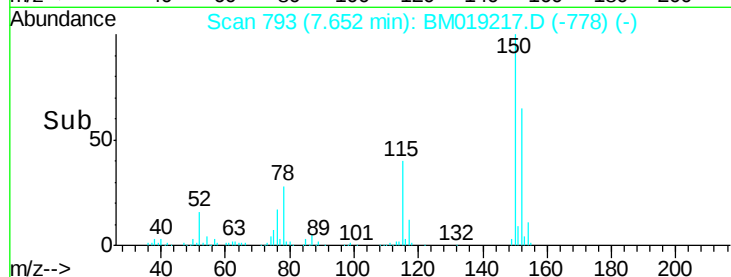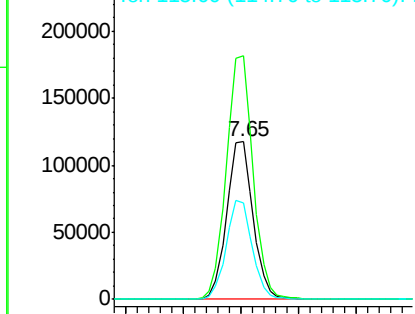



#5

2-Fluorophenol
Concen: 136.573 ng
RT: 5.25 min Scan# 385
Delta R.T. -0.01 min
Lab File: BM019217.D
Acq: 18 Mar 2019 16:03

Tgt Ion:112 Resp: 1570426
Ion Ratio Lower Upper
112 100
64 61.2 51.4 77.0
63 30.9 26.6 40.0

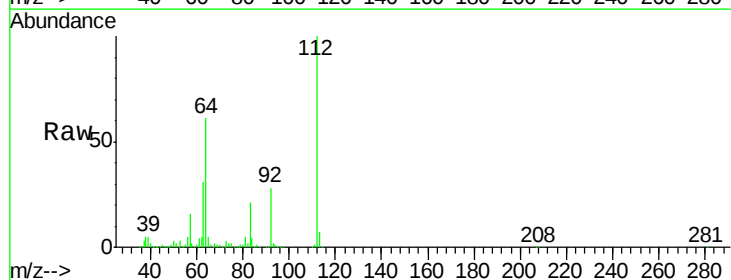

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

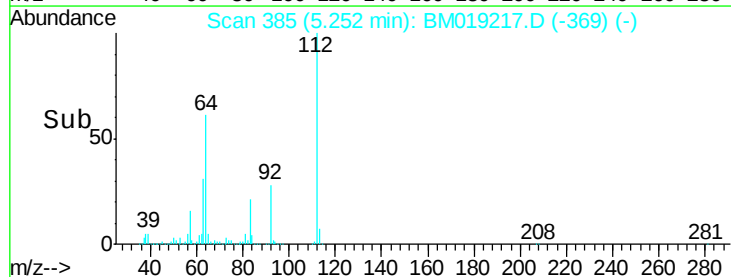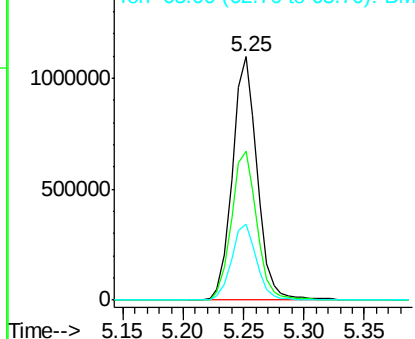



#7

Phenol-d6

Concen: 135.770 ng

RT: 6.83 min Scan# 654

Delta R.T. -0.01 min

Lab File: BM019217.D

Acq: 18 Mar 2019 16:03

Instrument :

BNA_M

ClientSampleId :


Tgt Ion: 99 Resp: 2283578

Ion Ratio Lower Upper

99 100

42 13.4 10.9 16.3




71 36.8 30.3 45.5

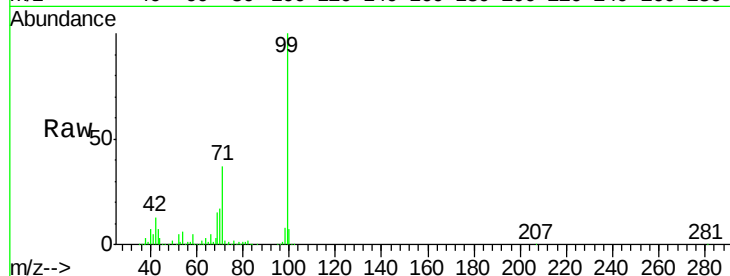

Abundance Ion 99.00 (98.70 to 99.70): BM019093.D (-630) (-)

Ion 42.00 (41.70 to 42.70): BM019093.D (-630) (-)

Ion 71.00 (70.70 to 71.70): BM019093.D (-630) (-)

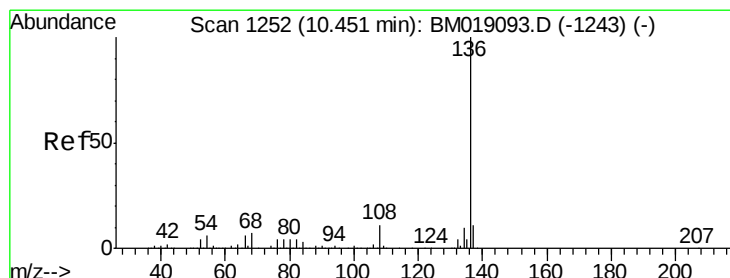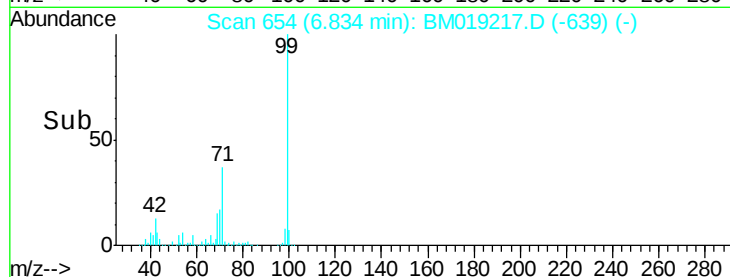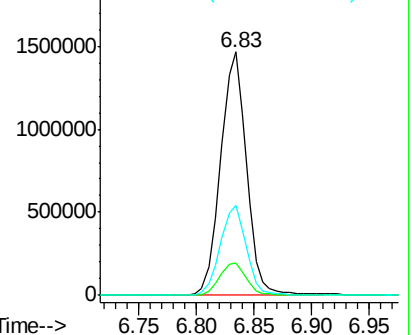

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.43 min Scan# 1266

Delta R.T. -0.02 min

Lab File: BM019217.D

Acq: 18 Mar 2019 16:03

Tgt Ion: 136 Resp: 780659


Ion Ratio Lower Upper

136 100

137 10.7 8.6 13.0

54 6.8 5.2 7.8

68 7.2 5.8 8.8


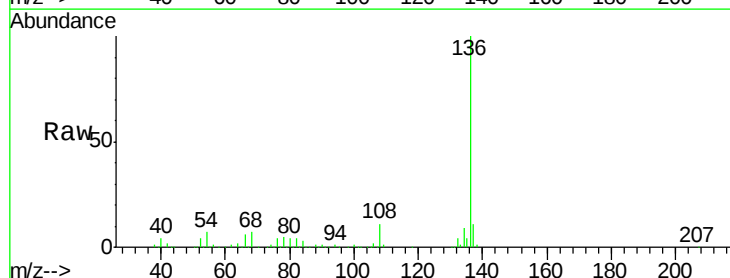


Abundance Ion 136.00 (135.70 to 136.70): BM019093.D (-1243) (-)

Ion 137.00 (136.70 to 137.70): BM019093.D (-1243) (-)

Ion 54.00 (53.70 to 54.70): BM019093.D (-1243) (-)

Ion 68.00 (67.70 to 68.70): BM019093.D (-1243) (-)



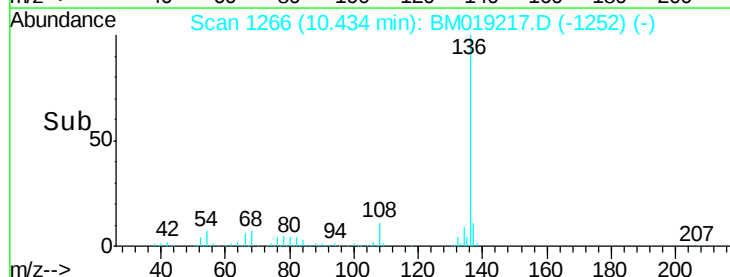
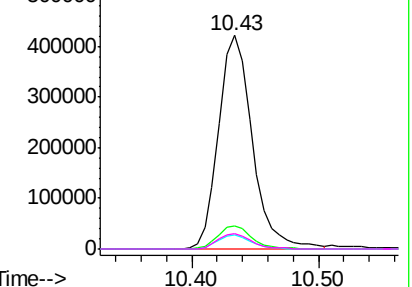




#23
Nitrobenzene-d5
Concen: 83.729 ng
RT: 8.82 min Scan# 991
Delta R.T. -0.02 min
Lab File: BM019217.D
Acq: 18 Mar 2019 16:03




Instrument :
BNA_M
ClientSampleId :


Tgt Ion: 82 Resp: 1382771
Ion Ratio Lower Upper
82 100
128 37.0 29.4 44.2
54 37.9 29.9 44.9

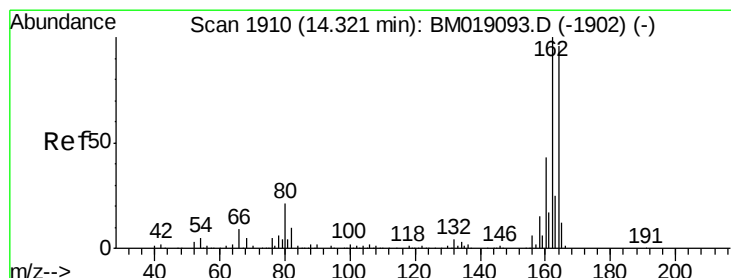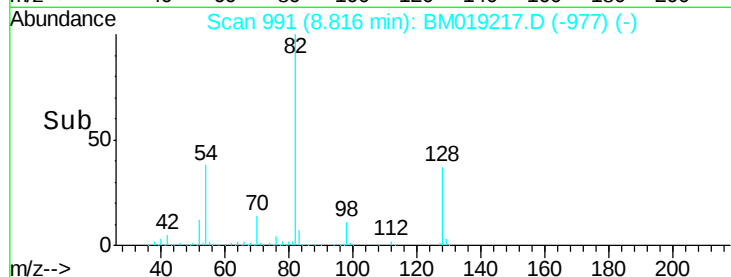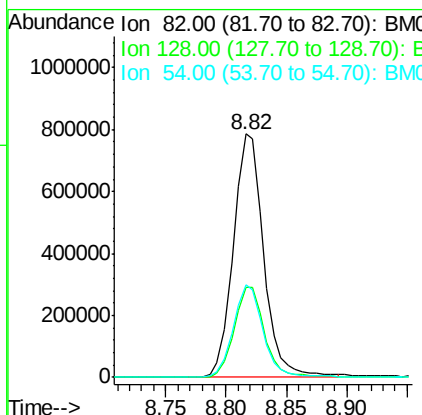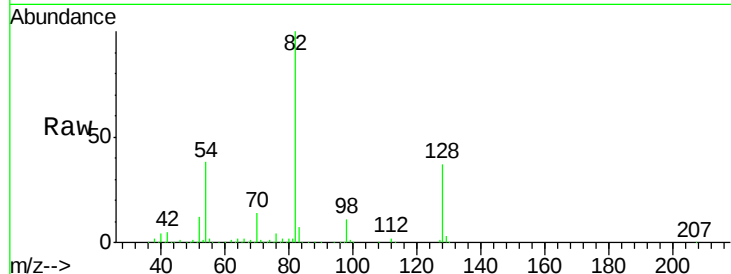

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.30 min Scan# 1924
Delta R.T. -0.02 min
Lab File: BM019217.D
Acq: 18 Mar 2019 16:03

Tgt Ion: 164 Resp: 490563
Ion Ratio Lower Upper
164 100
162 104.4 83.5 125.3
160 45.8 36.3 54.5

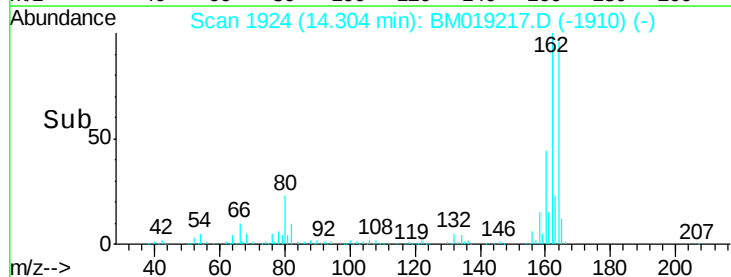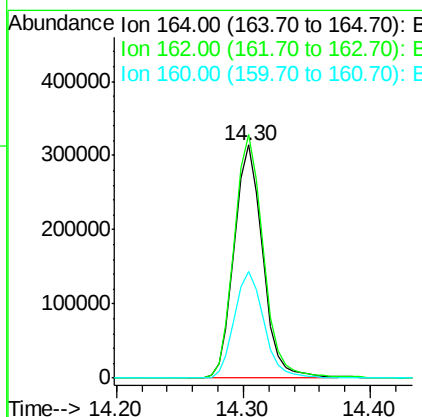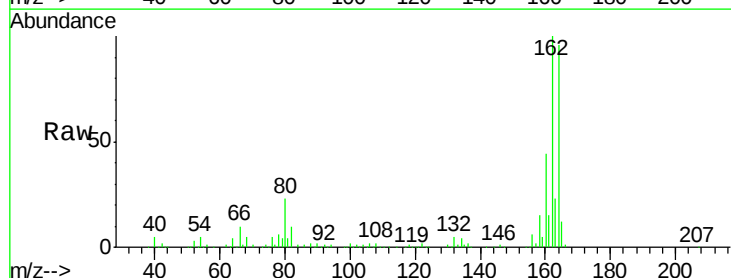


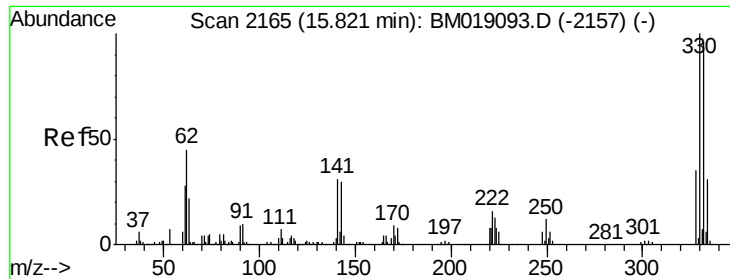




#42
 2,4,6-Tribromophenol
 Concen: 122.266 ng
 RT: 15.80 min Scan# 2179
 Delta R.T. -0.02 min
 Lab File: BM019217.D
 Acq: 18 Mar 2019 16:03

Instrument :
 BNA_M
 ClientSampleId :

Tgt Ion:330 Resp: 885575
 Ion Ratio Lower Upper
 330 100
 332 95.9 76.8 115.2
 141 33.0 27.0 40.4

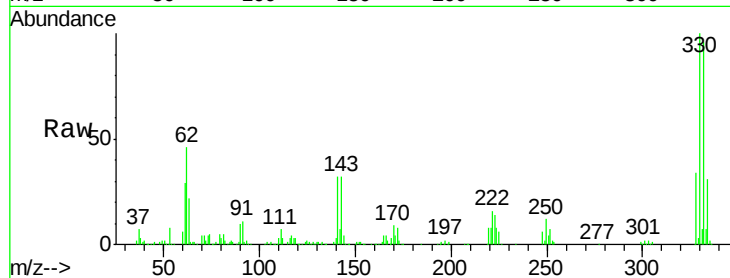


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

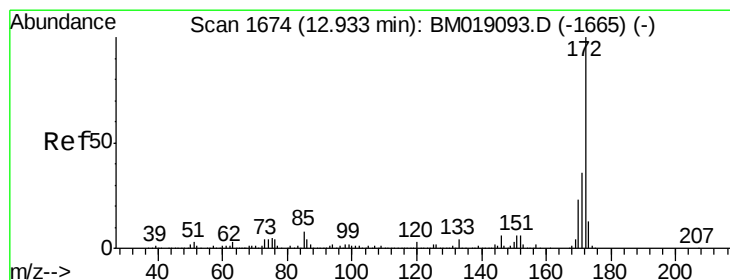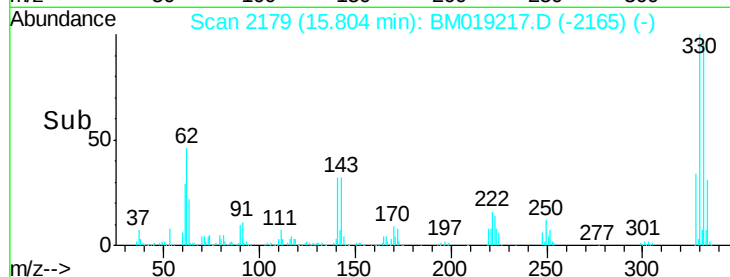
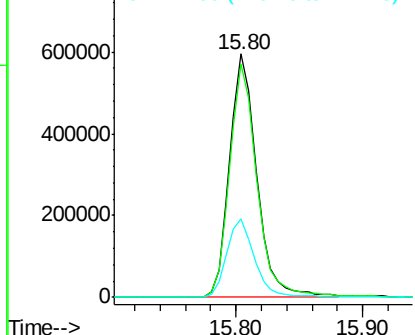



#45
 2-Fluorobiphenyl
 Concen: 84.033 ng
 RT: 12.92 min Scan# 1688
 Delta R.T. -0.02 min
 Lab File: BM019217.D
 Acq: 18 Mar 2019 16:03

Tgt Ion:172 Resp: 3169177
 Ion Ratio Lower Upper
 172 100
 171 35.9 28.6 42.8
 170 23.1 18.6 28.0

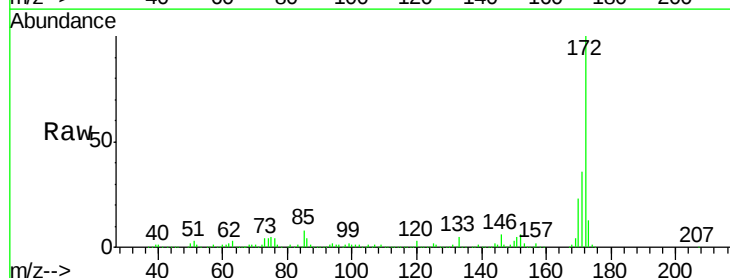

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



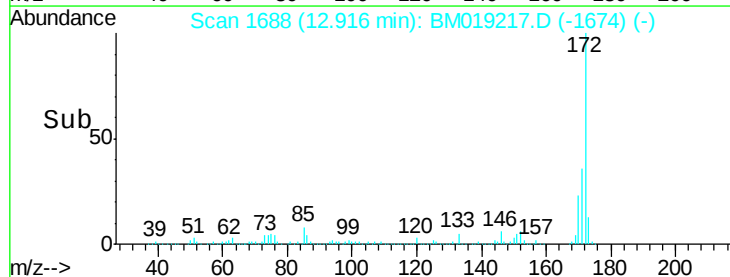
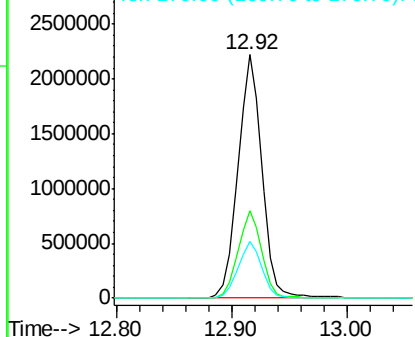


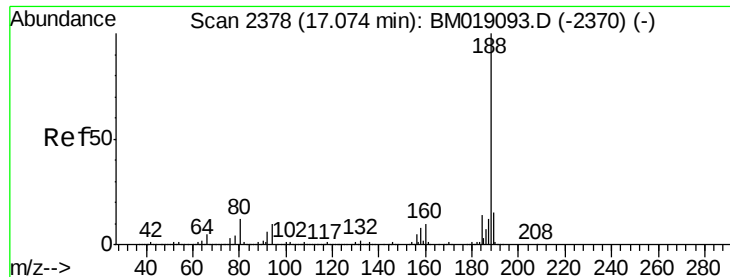

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.06 min Scan# 2392
Delta R.T. -0.02 min
Lab File: BM019217.D
Acq: 18 Mar 2019 16:03




Instrument :
BNA_M
ClientSampleId :

Tgt Ion:188 Resp: 1043826
Ion Ratio Lower Upper
188 100
94 9.8 8.1 12.1
80 12.6 9.7 14.5

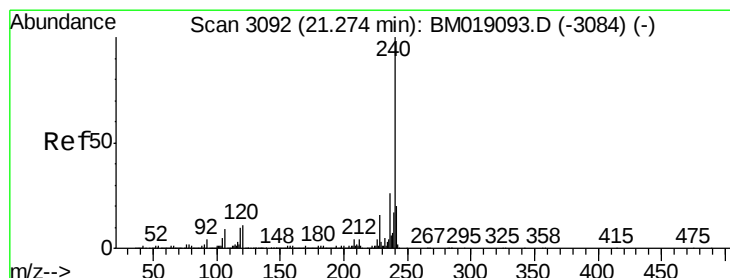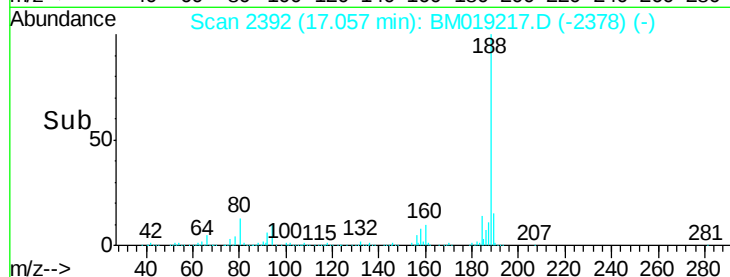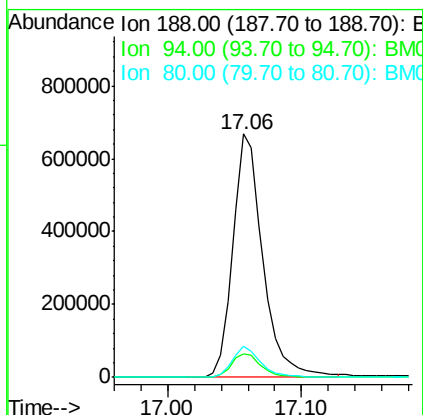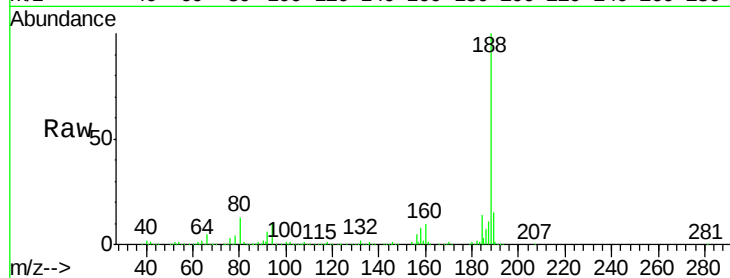

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.26 min Scan# 3107
Delta R.T. -0.01 min
Lab File: BM019217.D
Acq: 18 Mar 2019 16:03

Tgt Ion:240 Resp: 763365
Ion Ratio Lower Upper
240 100
120 11.2 8.9 13.3
236 25.5 21.0 31.4


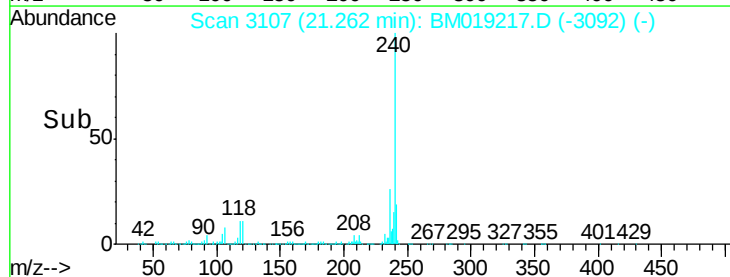
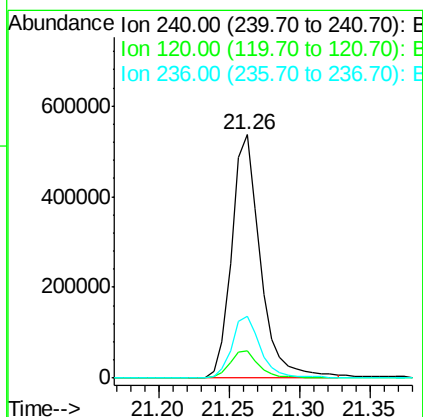
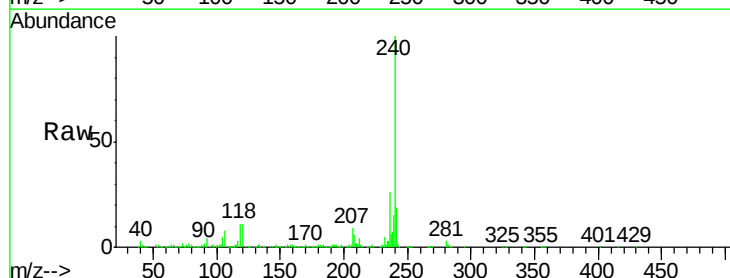




#79
 Terphenyl-d14
 Concen: 112.632 ng
 RT: 19.70 min Scan# 2841
 Delta R.T. -0.01 min
 Lab File: BM019217.D
 Acq: 18 Mar 2019 16:03

Instrument :
 BNA_M
 ClientSampled :

Tgt Ion:244 Resp: 4330983
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.4 8.2
 122 11.1 9.4 14.2

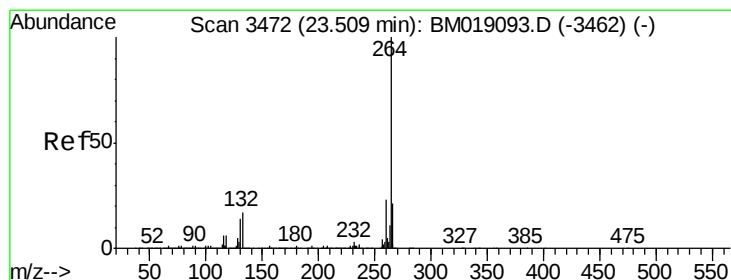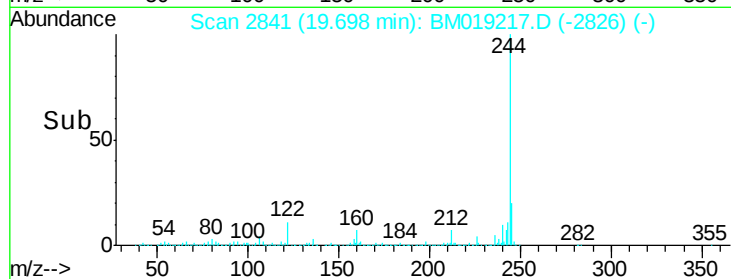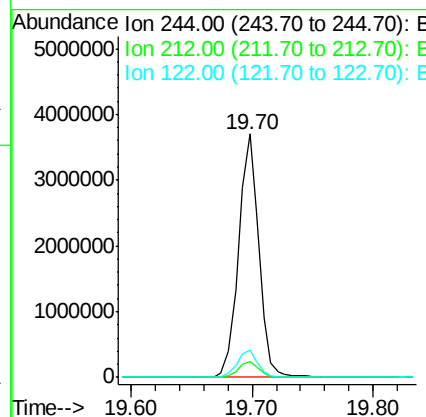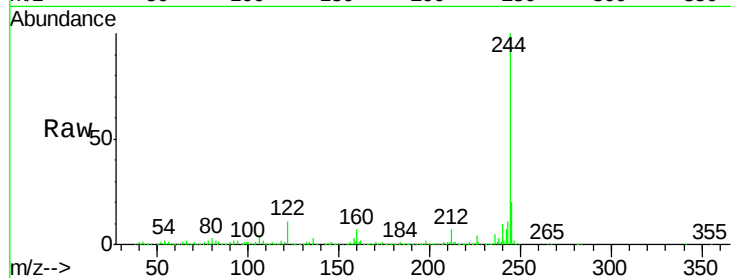

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.50 min Scan# 3487
 Delta R.T. -0.01 min
 Lab File: BM019217.D
 Acq: 18 Mar 2019 16:03

Tgt Ion:264 Resp: 735334
 Ion Ratio Lower Upper
 264 100
 260 24.1 18.6 28.0
 265 22.7 17.3 25.9

