

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031819\
 Data File : BM019217.D
 Acq On : 18 Mar 2019 16:03
 Operator : JU/SJ
 Sample : PB118000BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB118000BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.252	378	385	403	rBV	3815316	5531938	45.90%	8.332%
2	6.834	646	654	676	rBV	3925382	6254074	51.89%	9.419%
3	7.187	706	714	734	rBV	4007053	6348880	52.67%	9.562%
4	7.646	785	792	802	rBV	703818	1124166	9.33%	1.693%
5	7.963	839	846	862	rBV	2757361	4367098	36.23%	6.577%
6	8.816	984	991	1011	rBV	2046873	3630942	30.12%	5.469%
7	10.434	1258	1266	1278	rBV	866958	1617365	13.42%	2.436%
8	12.916	1681	1688	1704	rBV	6533438	9355808	77.62%	14.091%
9	14.304	1917	1924	1940	rBV2	1457569	2389462	19.82%	3.599%
10	15.804	2172	2179	2208	rBV	4444410	6867876	56.98%	10.344%
11	17.057	2386	2392	2409	rBV2	1701604	2693288	22.34%	4.056%
12	19.698	2835	2841	2862	rBV	10112246	12053343	100.00%	18.153%
13	21.262	3102	3107	3121	rBV	1525997	2254108	18.70%	3.395%
14	23.498	3481	3487	3499	rVB	917718	1908634	15.83%	2.875%


Sum of corrected areas: 66396982

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031819\
Data File : BM019217.D
Acq On : 18 Mar 2019 16:03
Operator : JU/SJ
Sample : PB118000BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB118000BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

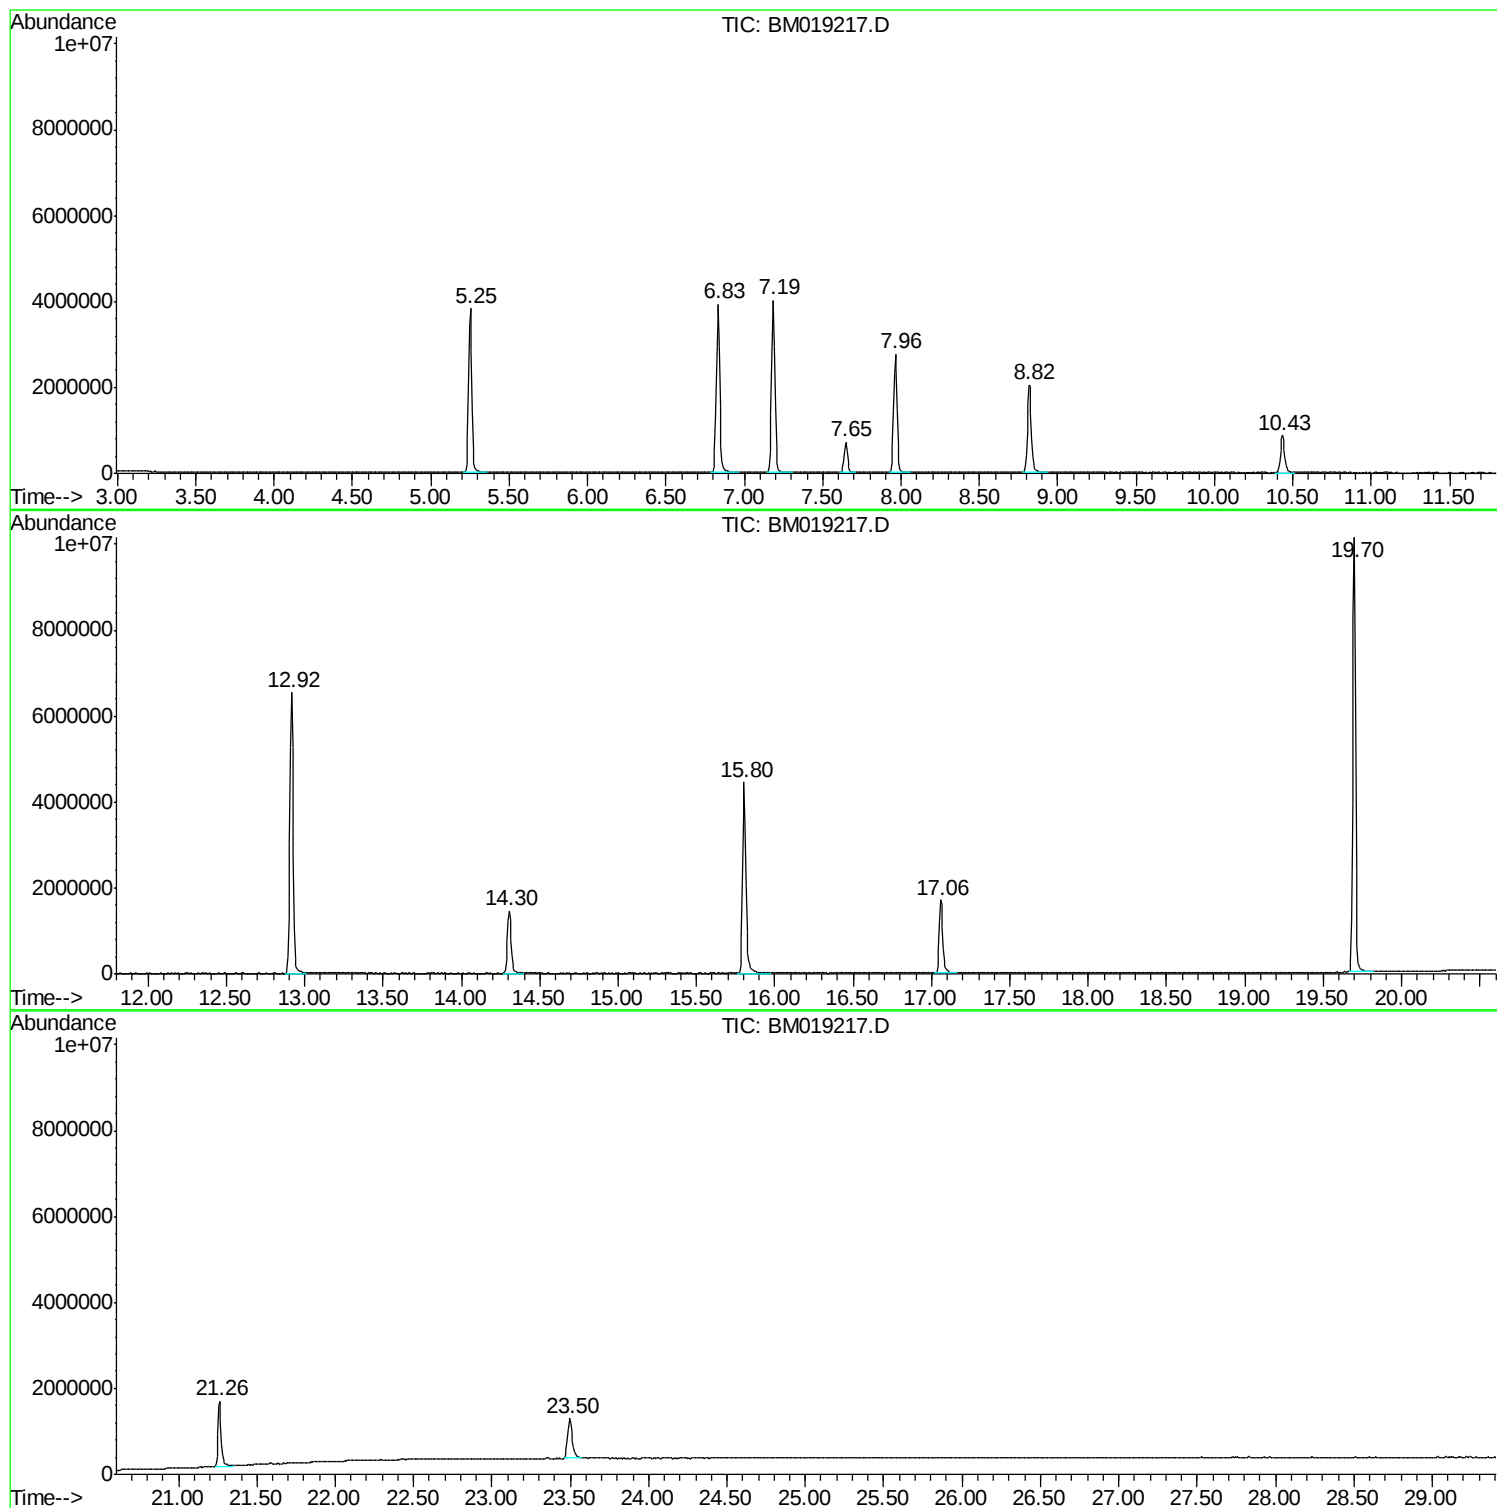

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031819\
Data File : BM019217.D
Acq On : 18 Mar 2019 16:03
Operator : JU/SJ
Sample : PB118000BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB118000BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.19 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.19	112.95 ng	6348880	1,4-Dichlorobenzene-d4	7.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
2		Tranvlcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
4		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

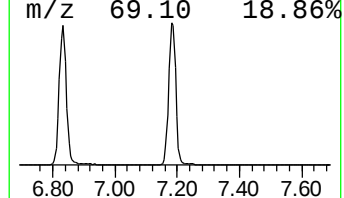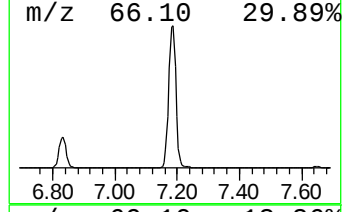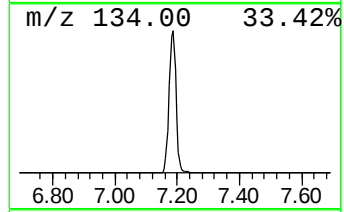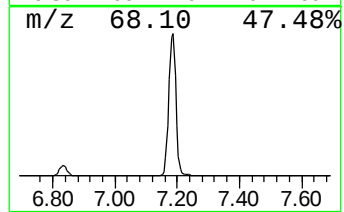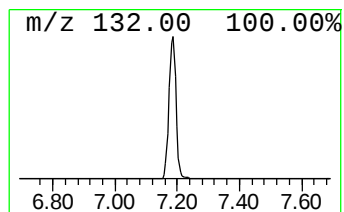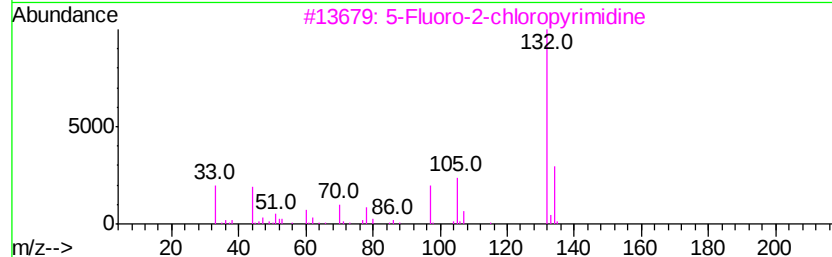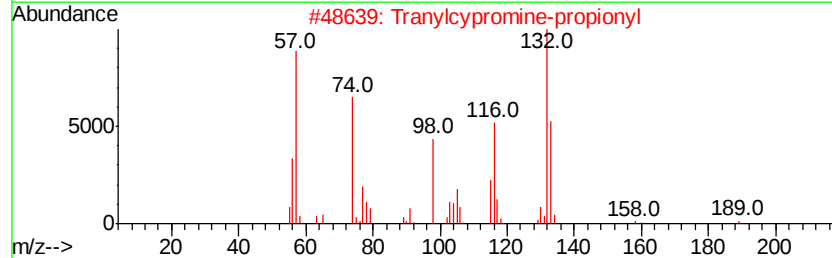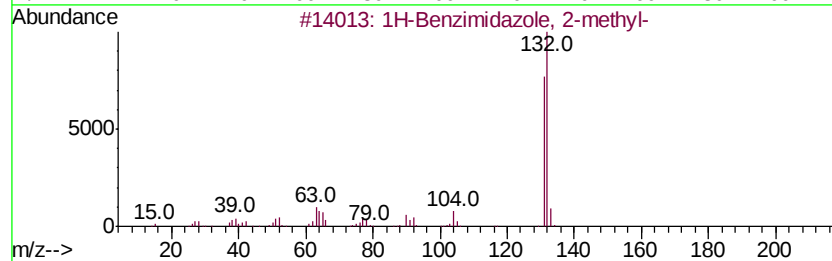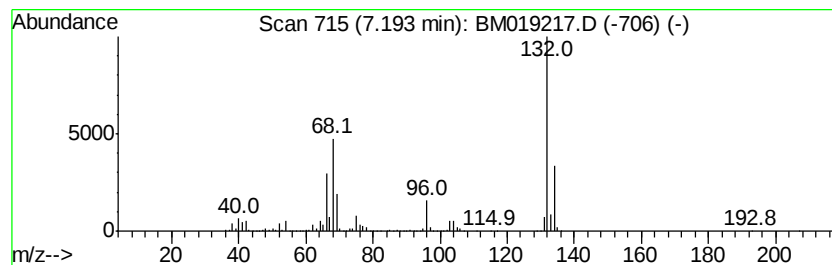

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031819\
Data File : BM019217.D
Acq On : 18 Mar 2019 16:03
Operator : JU/SJ
Sample : PB118000BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB118000BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.19	7.19	113.0	ng	6348880	1	7.65	1124170	20.0