


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031819\
 Data File : BM019211.D
 Acq On : 18 Mar 2019 11:50
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 11 17:30:46 2019

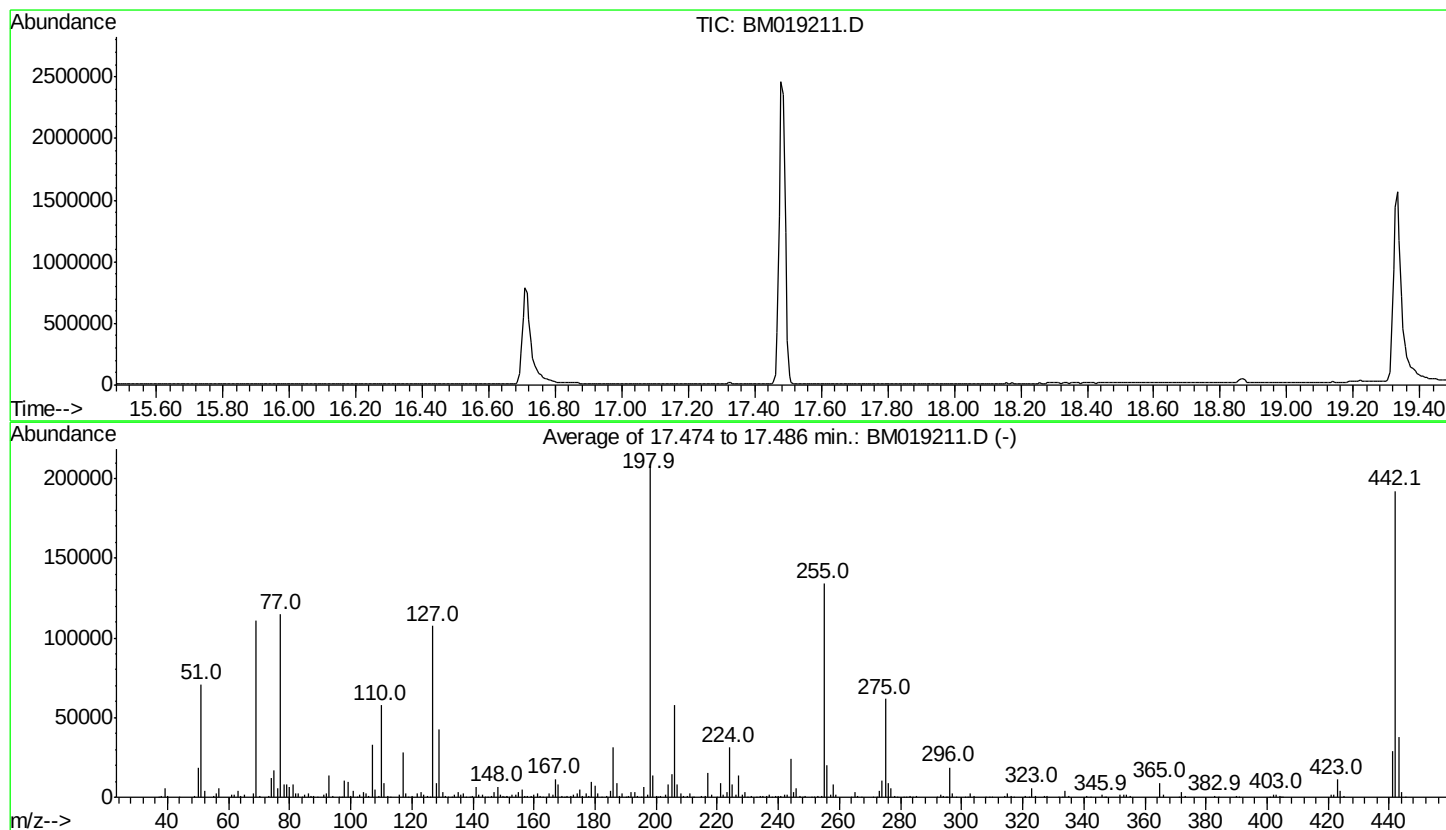

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	70669	PASS
68	69	0.00	2	1.9	2097	PASS
69	198	0.00	100	53.3	110896	PASS
70	69	0.00	2	0.6	612	PASS
127	198	10	80	51.7	107645	PASS
197	198	0.00	2	0.8	1563	PASS
198	198	100	100	100.0	208170	PASS
199	198	5	9	6.6	13738	PASS
275	198	10	60	29.6	61624	PASS
365	198	1	100	4.4	9189	PASS
441	198	0.01	100	14.1	29320	PASS
442	198	50	100	92.3	192128	PASS
443	442	15	24	19.6	37584	PASS