

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031822\
 Data File : BM034277.D
 Acq On : 18 Mar 2022 10:23
 Operator : CG/JU
 Sample : PB143392BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB143392BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034277.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.496	378	384	395	rBV	4164732	6045914	46.28%	10.339%
2	7.107	649	658	673	rBV	3857308	6317236	48.36%	10.803%
3	7.943	794	800	808	rBV	784615	1229343	9.41%	2.102%
4	9.107	990	998	1019	rBV	2432278	4048947	30.99%	6.924%
5	10.760	1270	1279	1288	rBV	990408	1707028	13.07%	2.919%
6	13.213	1689	1696	1708	rBV	6388803	9393274	71.90%	16.064%
7	14.583	1922	1929	1941	rBV	1577562	2318113	17.74%	3.964%
8	16.066	2175	2181	2206	rBV	5013003	7076643	54.17%	12.102%
9	17.324	2388	2395	2409	rBV	1756247	2606117	19.95%	4.457%
10	19.942	2834	2840	2855	rBV	10437588	13064184	100.00%	22.341%
11	21.495	3099	3104	3121	rBV	1696958	2507982	19.20%	4.289%
12	23.912	3508	3515	3534	rVB2	967907	2160242	16.54%	3.694%




Sum of corrected areas: 58475023

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031822\
Data File : BM034277.D
Acq On : 18 Mar 2022 10:23
Operator : CG/JU
Sample : PB143392BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143392BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

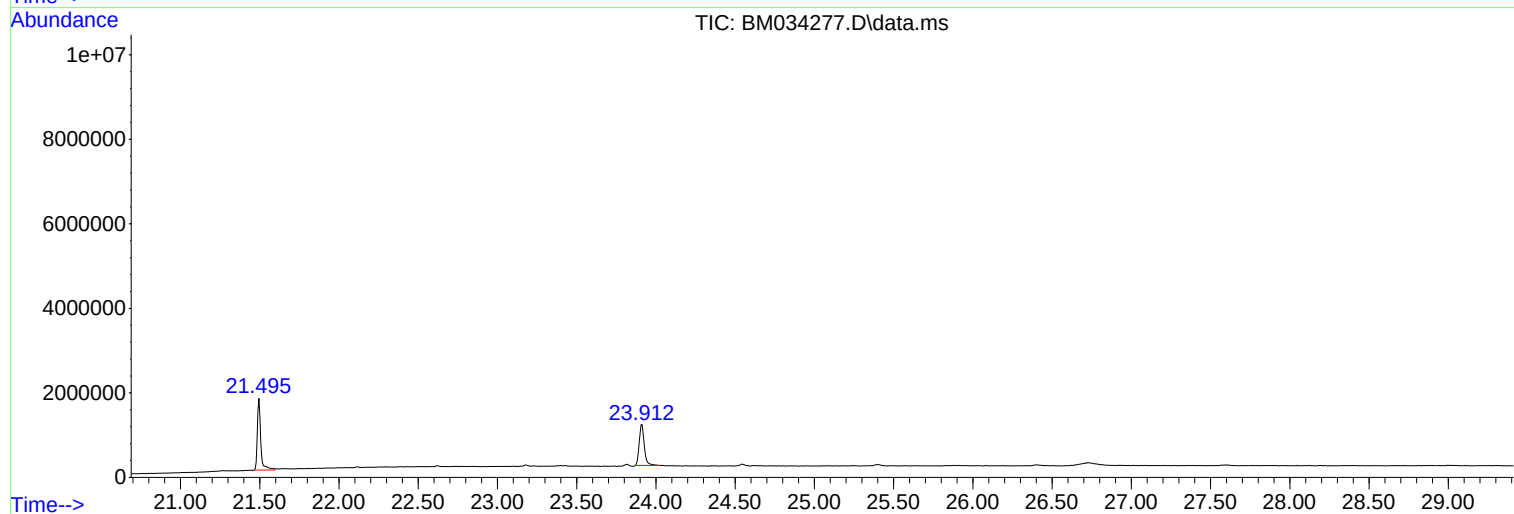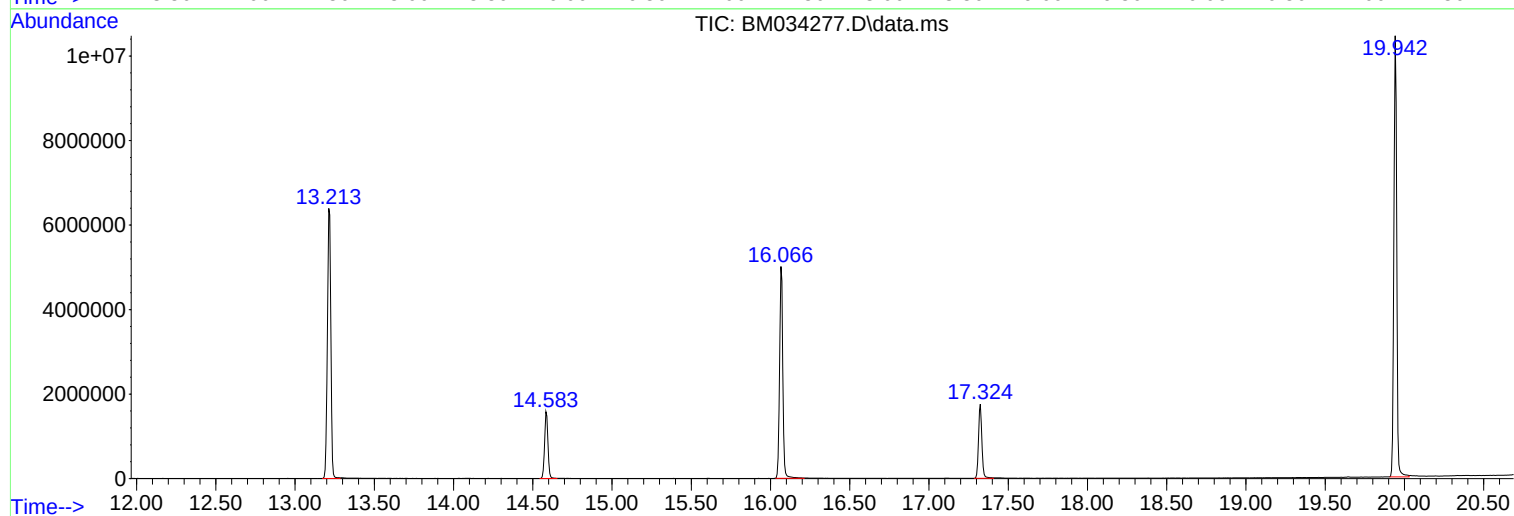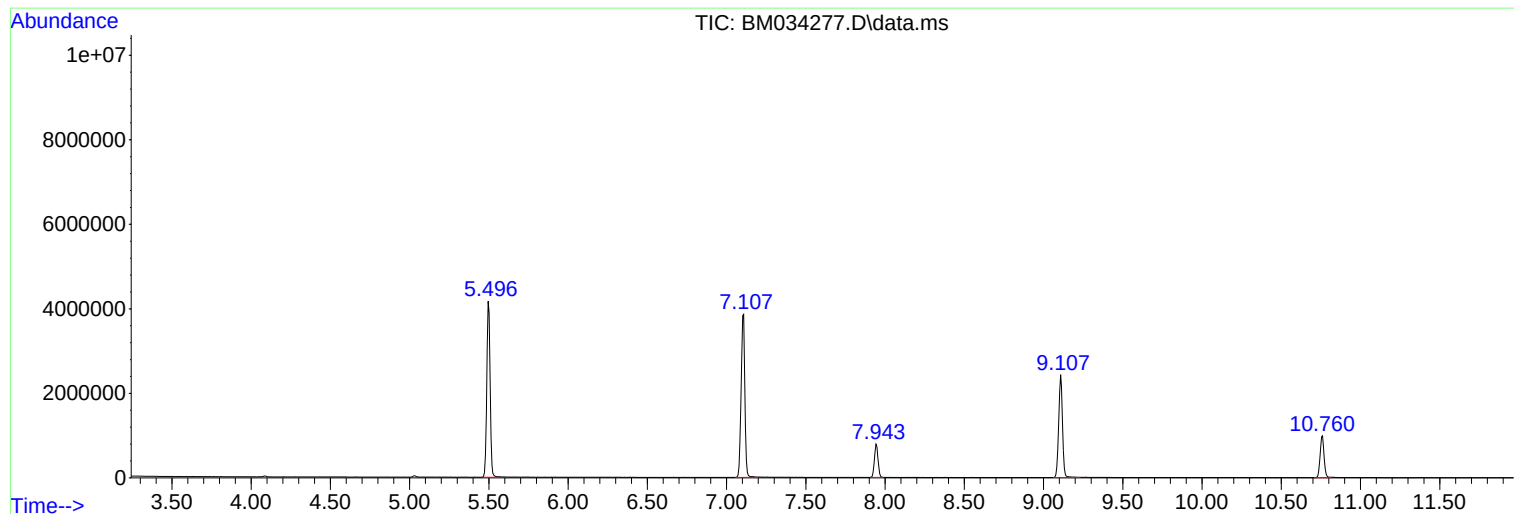

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031822\
Data File : BM034277.D
Acq On : 18 Mar 2022 10:23
Operator : CG/JU
Sample : PB143392BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143392BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031822\
Data File : BM034277.D
Acq On : 18 Mar 2022 10:23
Operator : CG/JU
Sample : PB143392BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143392BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------