
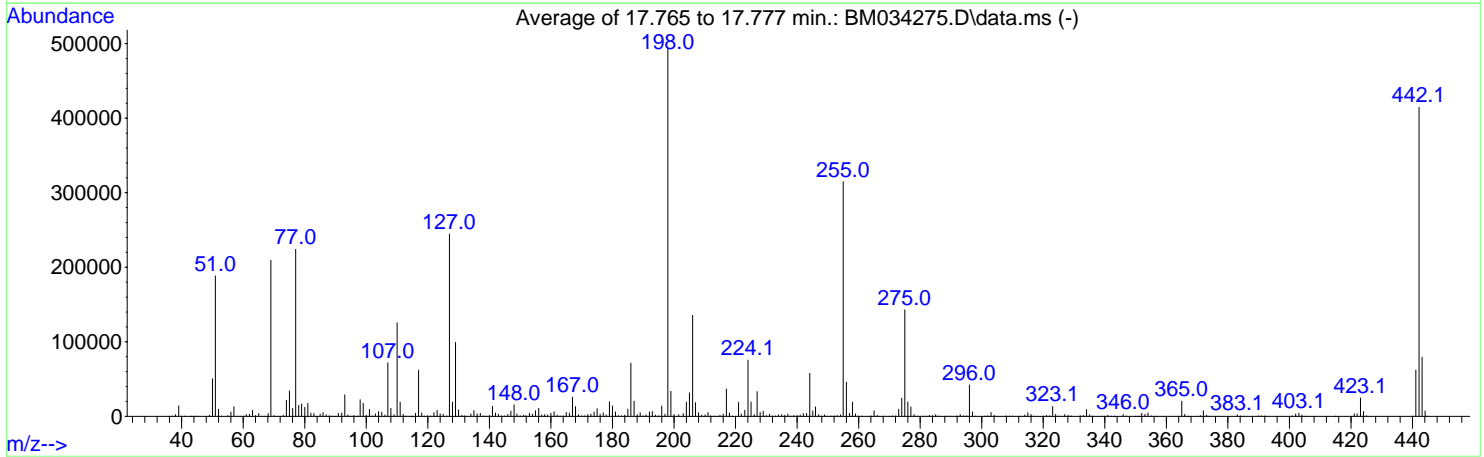


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031822\  
 Data File : BM034275.D  
 Acq On : 18 Mar 2022 08:54  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031522.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Mar 16 02:38:26 2022

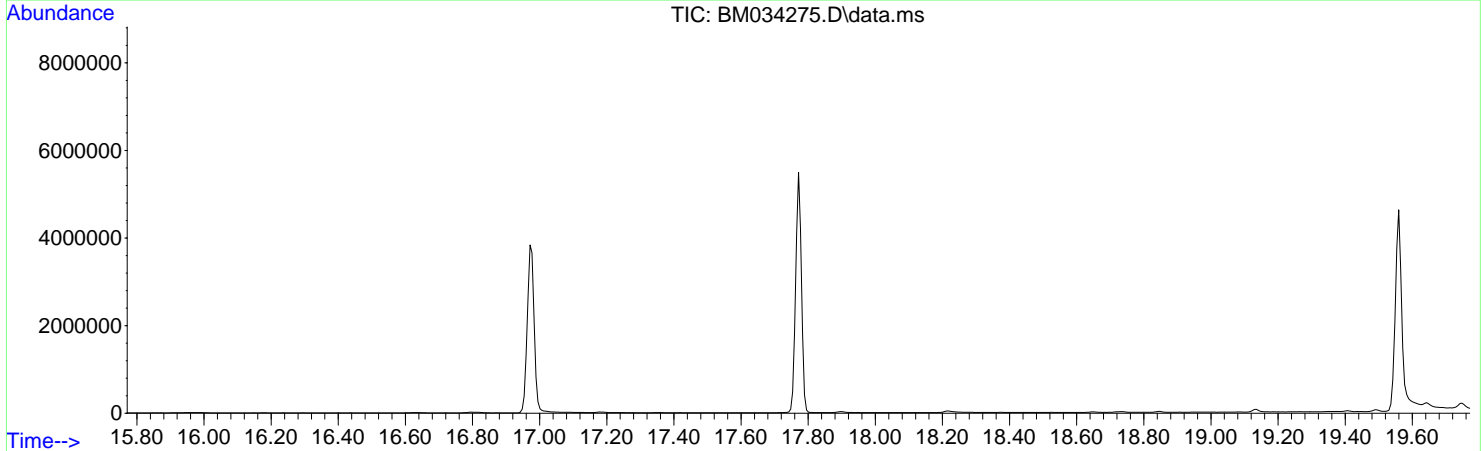




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	188548	PASS
68	69	0.00	2	1.9	3972	PASS
69	198	0.00	100	42.4	209451	PASS
70	69	0.00	2	0.5	1141	PASS
127	198	10	80	49.6	244565	PASS
197	198	0.00	2	0.6	2982	PASS
198	198	100	100	100.0	493461	PASS
199	198	5	9	6.8	33763	PASS
275	198	10	60	29.0	142973	PASS
365	198	1	100	4.1	20447	PASS
441	198	0.01	100	12.6	62077	PASS
442	442	50	100	100.0	414571	PASS
443	442	15	24	19.2	79469	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031822\  
 Data File : BM034275.D  
 Acq On : 18 Mar 2022 08:54  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Quant Time: Mar 18 18:09:41 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031522.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Mar 16 02:38:26 2022  
 Response via : Initial Calibration

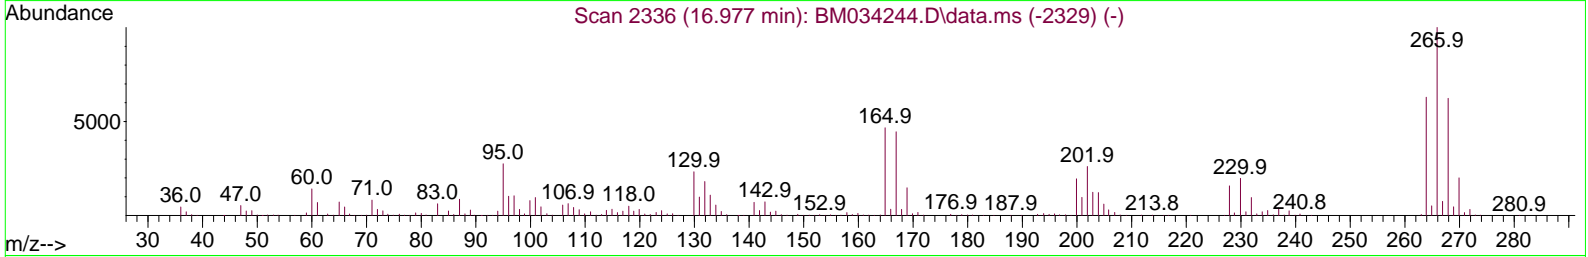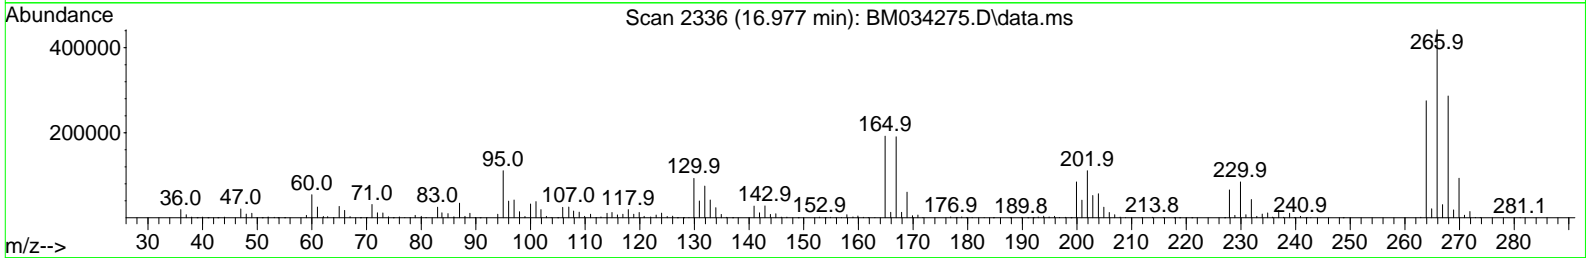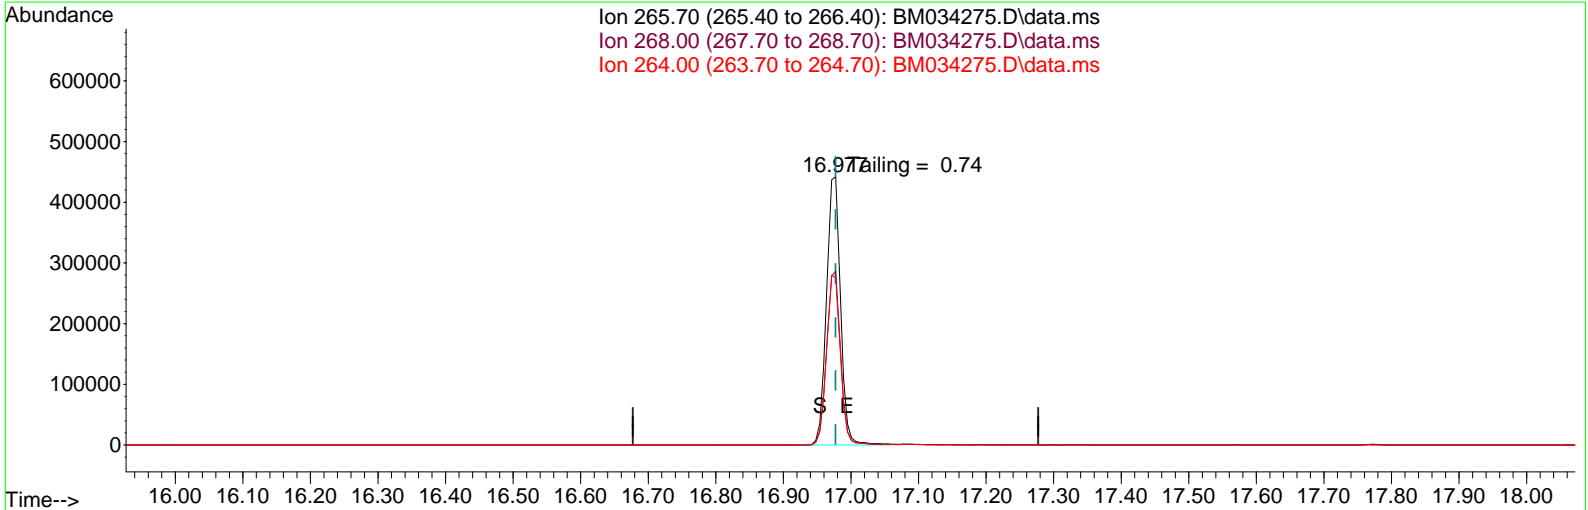

TIC: BM034275.D\data.ms

(70) Pentachlorophenol (C)

16.977min (+ 0.000) 213852.64 ng




response 640032

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.82
264.00	62.90	62.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031822\  
 Data File : BM034275.D  
 Acq On : 18 Mar 2022 08:54  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_M  
**ClientSampleId :**  
 DFTPP

Quant Time: Mar 18 18:09:41 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031522.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Mar 16 02:38:26 2022  
 Response via : Initial Calibration

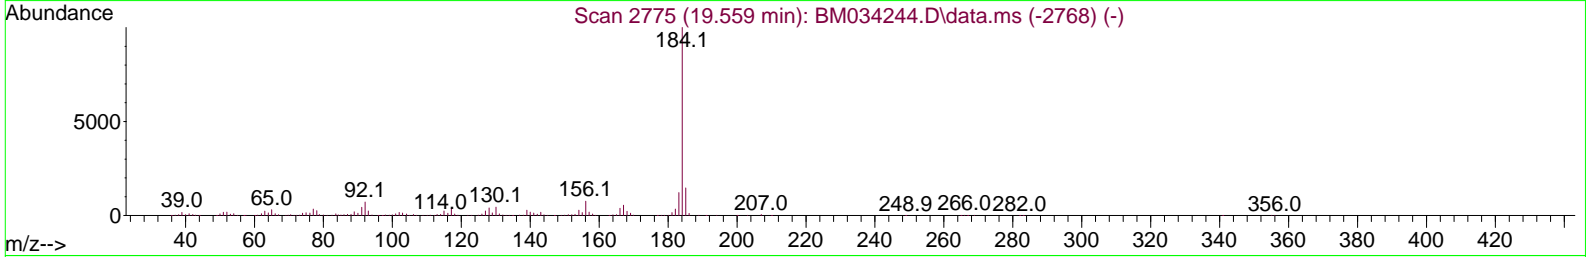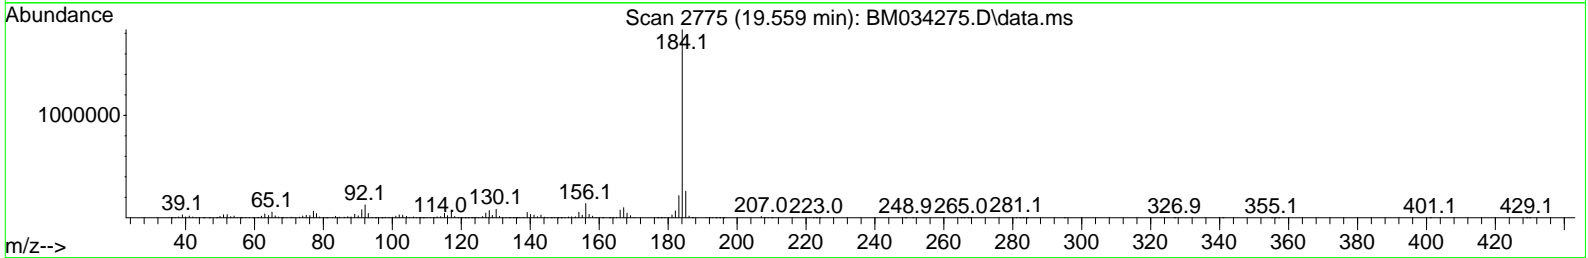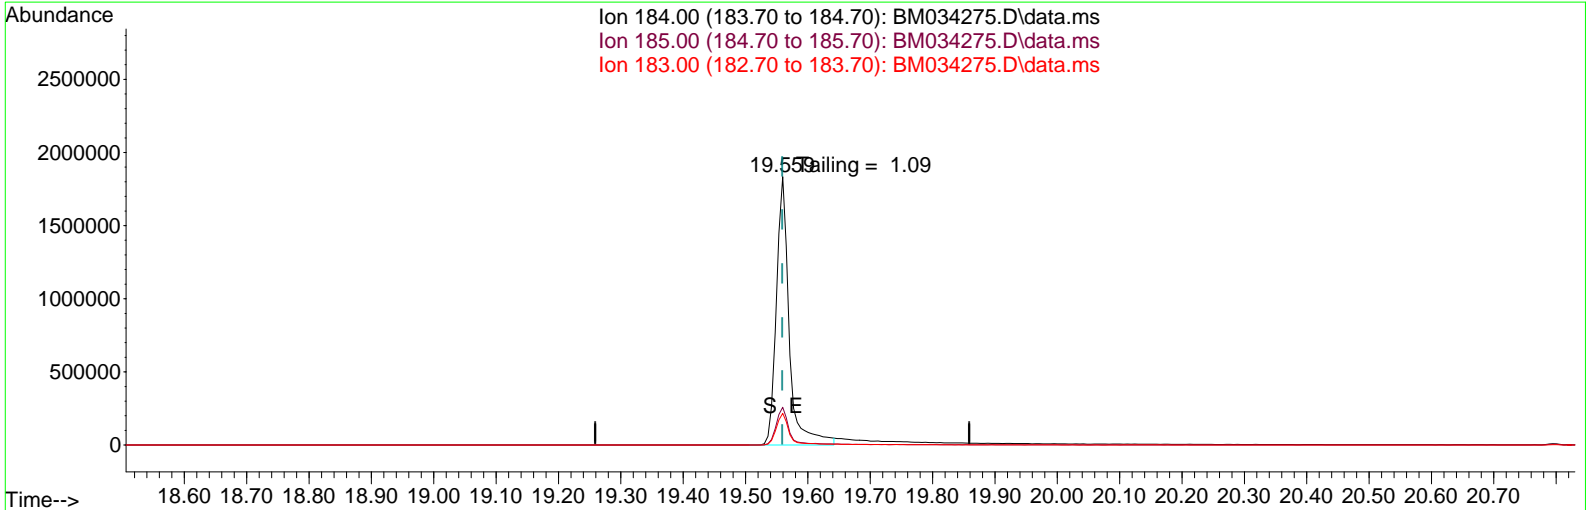

TIC: BM034275.D\data.ms

(77) Benzidine

19.559min (+ 0.000) 21946.82 ng

response 2926067

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.10
183.00	12.20	11.80
0.00	0.00	0.00

**DDT Breakdown**

Date	Instrument Name	DFTPP Data File
3/18/2022	BNA_M	<u>BM034275.D</u>
Compound Name	Response	Retention Time
DDT	1888300	20.486
DDD	12704	20.057
DDE	16181809	19.569
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16194513	18082813	89.56

Instrument :  
 BNA\_M  
 Client:Sampled :  
 DFTPP