

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031919\
 Data File : BM019240.D
 Acq On : 19 Mar 2019 17:18
 Operator : JU/SJ
 Sample : K1958-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-1

Quant Time: Mar 20 05:11:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 11 17:30:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	162999	20.00	ng	-0.02
21) Naphthalene-d8	10.42	136	658085	20.00	ng	-0.03
39) Acenaphthene-d10	14.29	164	429906	20.00	ng	-0.03
64) Phenanthrene-d10	17.05	188	1001300	20.00	ng	-0.02
76) Chrysene-d12	21.25	240	919965	20.00	ng	-0.02
87) Perylene-d12	23.49	264	817016	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.24	112	1389071	138.01	ng	-0.02
7) Phenol-d6	6.82	99	1807106	122.75	ng	-0.02
23) Nitrobenzene-d5	8.81	82	1358139	97.55	ng	-0.02
42) 2,4,6-Tribromophenol	15.80	330	1056231	166.40	ng	-0.02
45) 2-Fluorobiphenyl	12.90	172	3141474	95.05	ng	-0.03
79) Terphenyl-d14	19.69	244	5597153	120.78	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031919\
Data File : BM019240.D
Acq On : 19 Mar 2019 17:18
Operator : JU/SJ
Sample : K1958-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-1

Quant Time: Mar 20 05:11:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 11 17:30:46 2019
Response via : Initial Calibration

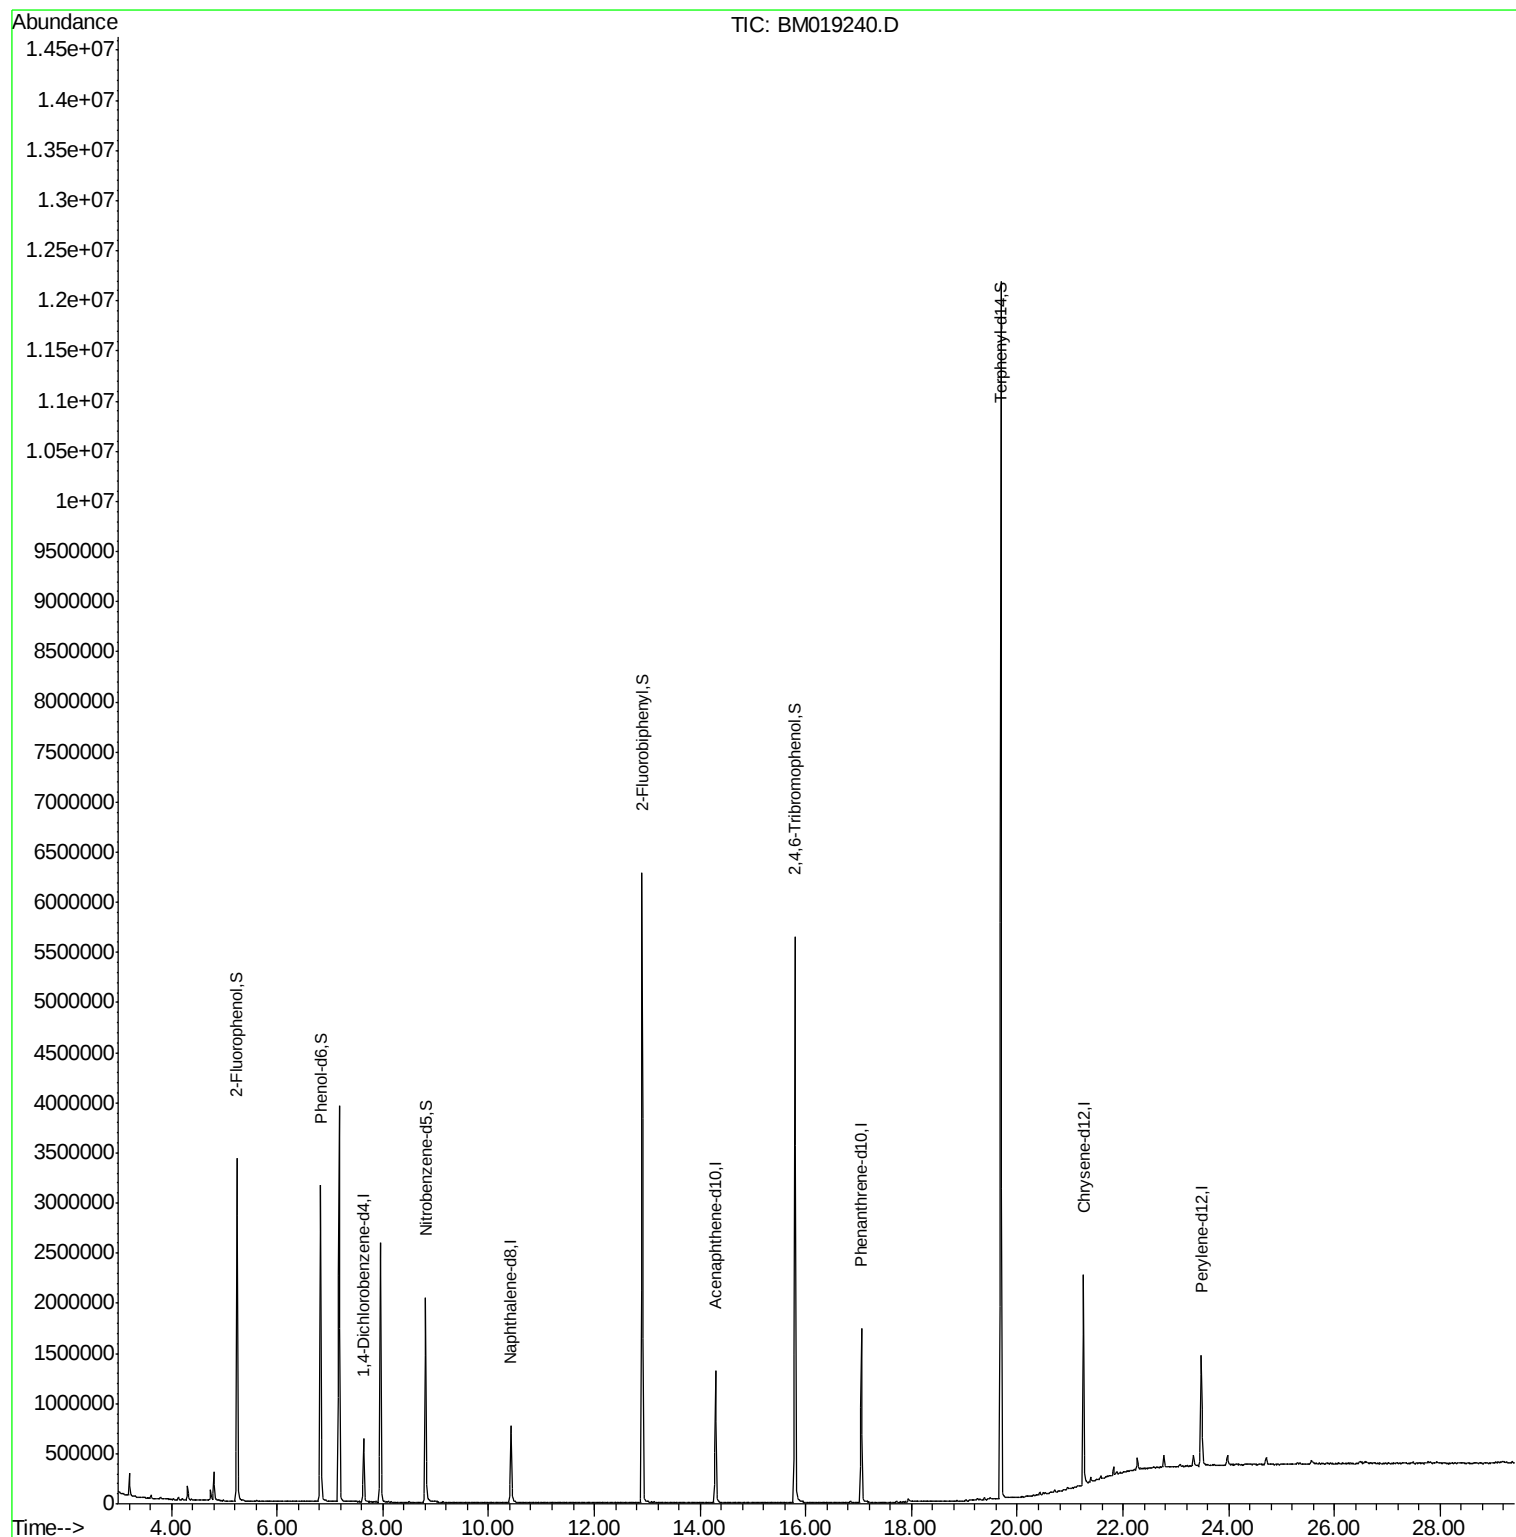

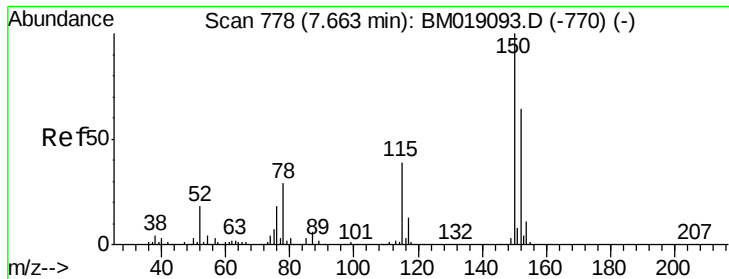


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.64 min Scan# 791
Delta R.T. -0.02 min
Lab File: BM019240.D
Acq: 19 Mar 2019 17:18

Instrument :
BNA_M
ClientSampled :
TP-1

Tgt Ion:152 Resp: 162999
Ion Ratio Lower Upper
152 100
150 156.0 125.3 187.9
115 59.9 49.4 74.0

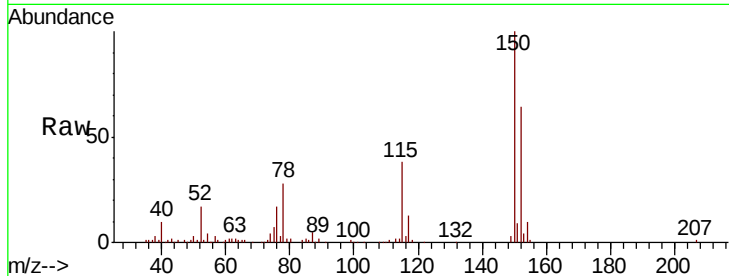


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

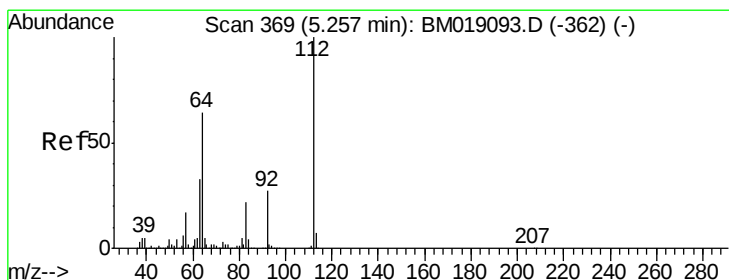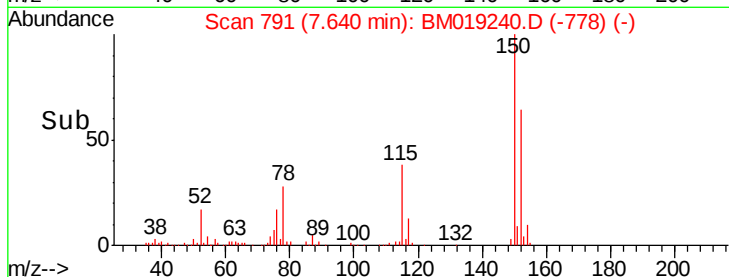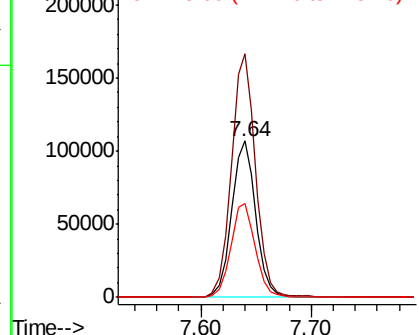



#5


2-Fluorophenol
Concen: 138.011 ng
RT: 5.24 min Scan# 383
Delta R.T. -0.02 min
Lab File: BM019240.D
Acq: 19 Mar 2019 17:18

Tgt Ion:112 Resp: 1389071
Ion Ratio Lower Upper
112 100
64 61.5 51.4 77.0
63 31.8 26.6 40.0

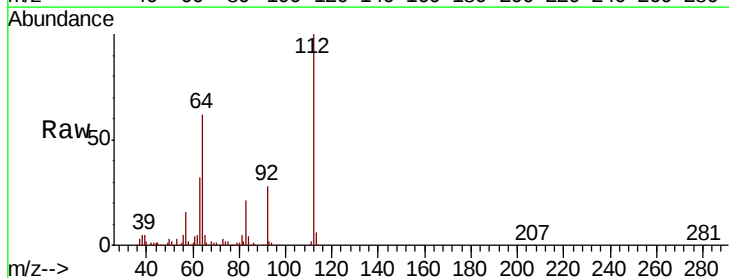

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

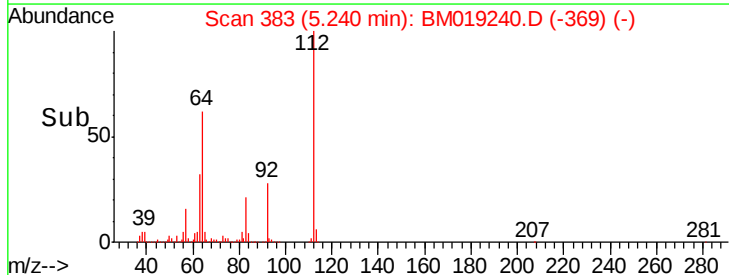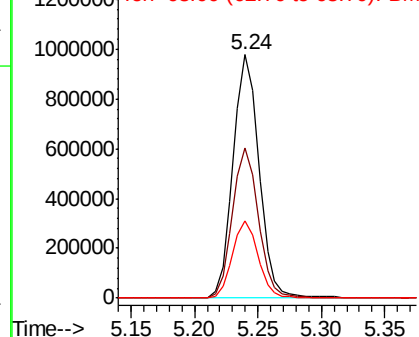



#7

Phenol-d6

Concen: 122.749 ng

RT: 6.82 min Scan# 652

Delta R.T. -0.02 min

Lab File: BM019240.D

Acq: 19 Mar 2019 17:18

Instrument :

BNA_M

ClientSampleId :

TP-1


Tgt Ion: 99 Resp: 1807106

Ion Ratio Lower Upper

99 100

42 13.6 10.9 16.3

71 37.2 30.3 45.5






Abundance

Ion 99.00 (98.70 to 99.70): BM019240.D (-639) (-)

Ion 42.00 (41.70 to 42.70): BM019240.D (-639) (-)

Ion 71.00 (70.70 to 71.70): BM019240.D (-639) (-)

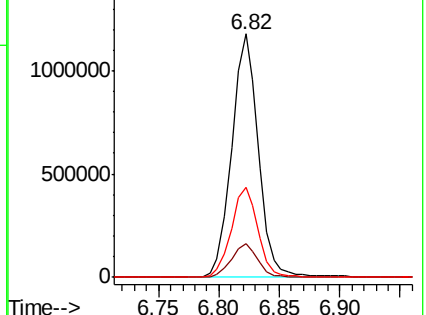

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.42 min Scan# 1264

Delta R.T. -0.03 min

Lab File: BM019240.D

Acq: 19 Mar 2019 17:18

Tgt Ion: 136 Resp: 658085


Ion Ratio Lower Upper

136 100

137 10.5 8.6 13.0

54 6.6 5.2 7.8

68 7.4 5.8 8.8





Abundance

Ion 136.00 (135.70 to 136.70): BM019240.D (-1252) (-)

Ion 137.00 (136.70 to 137.70): BM019240.D (-1252) (-)

Ion 54.00 (53.70 to 54.70): BM019240.D (-1252) (-)

Ion 68.00 (67.70 to 68.70): BM019240.D (-1252) (-)

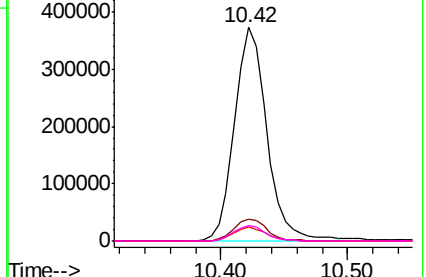







#23
Nitrobenzene-d5
Concen: 97.555 ng
RT: 8.81 min Scan# 990
Delta R.T. -0.02 min
Lab File: BM019240.D
Acq: 19 Mar 2019 17:18

Instrument :
BNA_M
ClientSampled :
TP-1

Tgt Ion: 82 Resp: 1358139
Ion Ratio Lower Upper
82 100
128 38.4 29.4 44.2
54 35.9 29.9 44.9

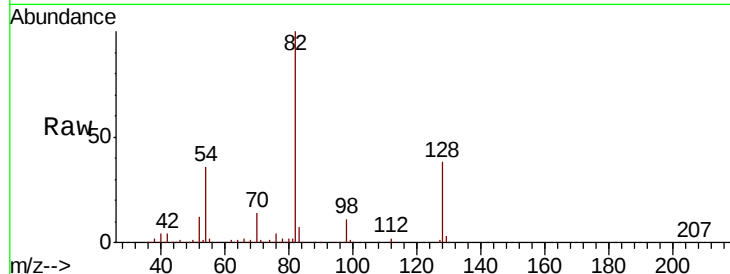


Abundance Ion 82.00 (81.70 to 82.70): BM019240.D (-977) (-)
Ion 128.00 (127.70 to 128.70): BM019240.D (-977) (-)
Ion 54.00 (53.70 to 54.70): BM019240.D (-977) (-)

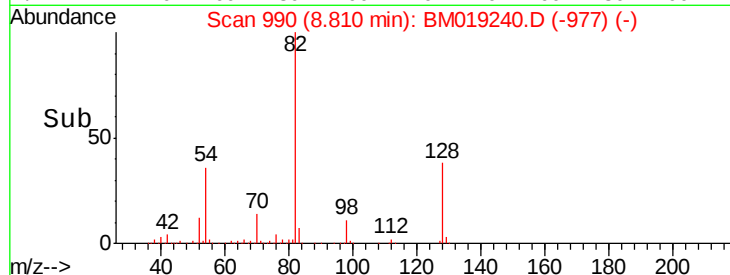
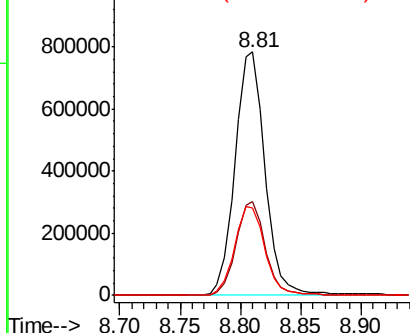



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.29 min Scan# 1922
Delta R.T. -0.03 min
Lab File: BM019240.D
Acq: 19 Mar 2019 17:18

Tgt Ion: 164 Resp: 429906
Ion Ratio Lower Upper
164 100
162 104.2 83.5 125.3
160 45.9 36.3 54.5

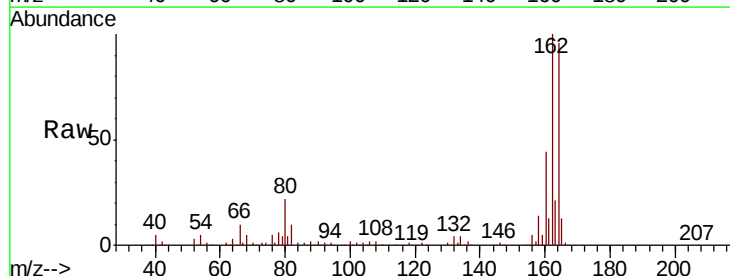

Abundance Ion 164.00 (163.70 to 164.70): BM019240.D (-1910) (-)
Ion 162.00 (161.70 to 162.70): BM019240.D (-1910) (-)
Ion 160.00 (159.70 to 160.70): BM019240.D (-1910) (-)

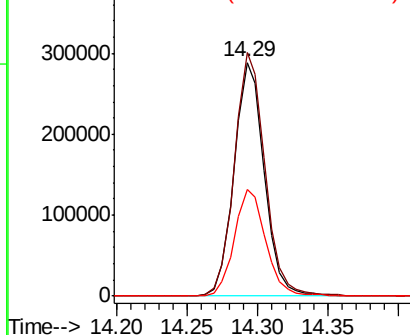







#42
 2,4,6-Tribromophenol
 Concen: 166.403 ng
 RT: 15.80 min Scan# 2178
 Delta R.T. -0.02 min
 Lab File: BM019240.D
 Acq: 19 Mar 2019 17:18

Instrument :
 BNA_M
 ClientSampled :
 TP-1

Tgt Ion:330 Resp: 1056231
 Ion Ratio Lower Upper
 330 100
 332 97.0 76.8 115.2
 141 31.6 27.0 40.4

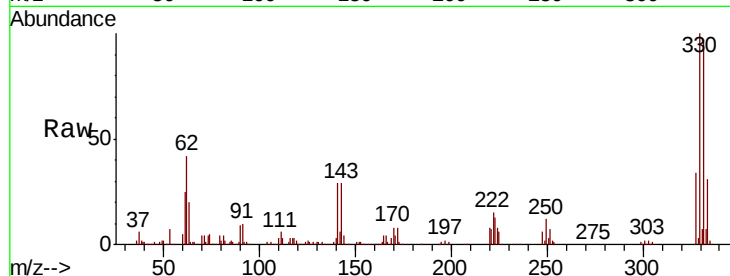


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


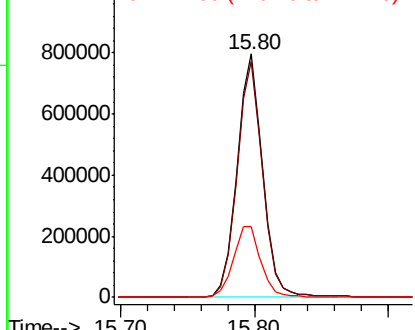



#45
 2-Fluorobiphenyl
 Concen: 95.051 ng
 RT: 12.90 min Scan# 1686
 Delta R.T. -0.03 min
 Lab File: BM019240.D
 Acq: 19 Mar 2019 17:18

Tgt Ion:172 Resp: 3141474
 Ion Ratio Lower Upper
 172 100
 171 35.8 28.6 42.8
 170 23.6 18.6 28.0



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

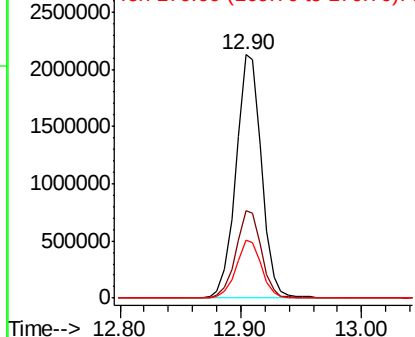


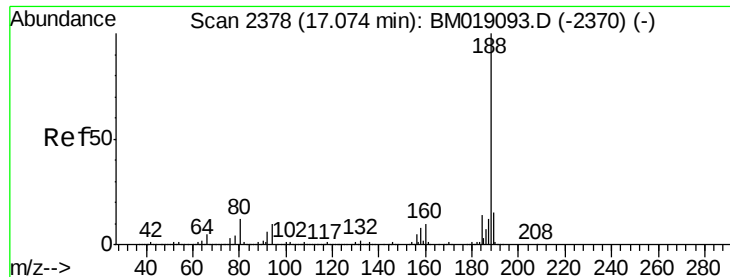




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.05 min Scan# 2391
Delta R.T. -0.02 min
Lab File: BM019240.D
Acq: 19 Mar 2019 17:18

Instrument :
BNA_M
ClientSampleId :
TP-1

Tgt Ion:188 Resp: 1001300
Ion Ratio Lower Upper
188 100
94 9.4 8.1 12.1
80 11.4 9.7 14.5




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM

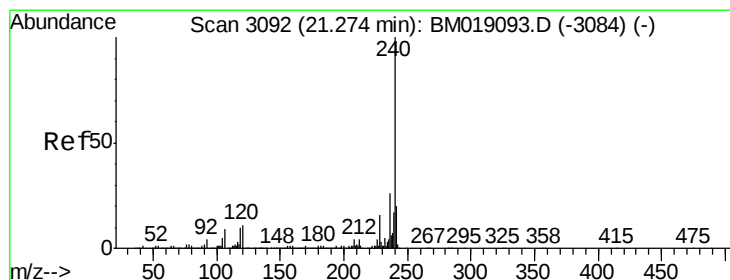
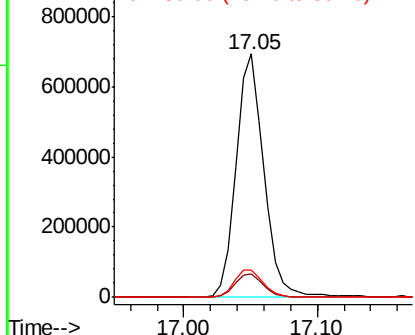



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.25 min Scan# 3105
Delta R.T. -0.02 min
Lab File: BM019240.D
Acq: 19 Mar 2019 17:18

Tgt Ion:240 Resp: 919965
Ion Ratio Lower Upper
240 100
120 11.3 8.9 13.3
236 25.5 21.0 31.4



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

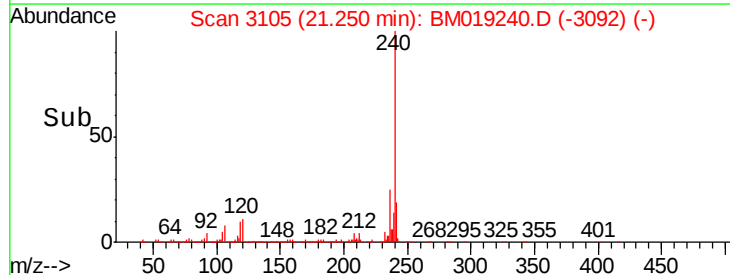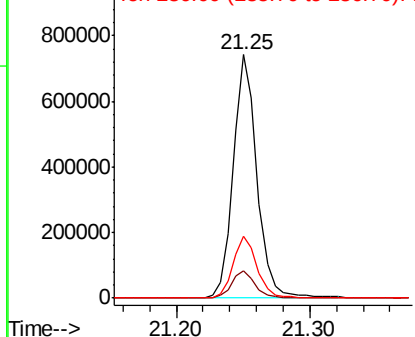

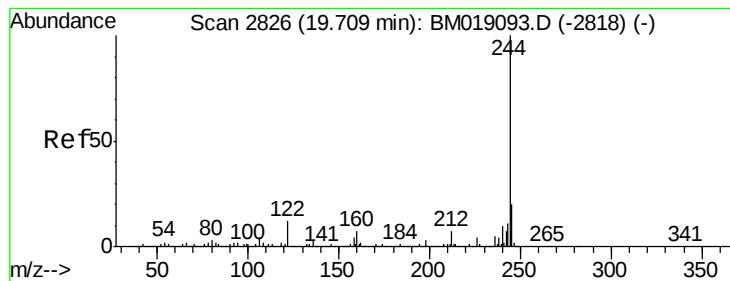

#79

Terphenyl-d14

Concen: 120.783 ng

RT: 19.69 min Scan# 2840

Delta R.T. -0.02 min

Lab File: BM019240.D

Acq: 19 Mar 2019 17:18

Instrument :

BNA_M

ClientSampleId :

TP-1


Tgt Ion:244 Resp: 5597153

Ion Ratio Lower Upper

244 100

212 6.7 5.4 8.2




122 11.0 9.4 14.2



Abundance Ion 244.00 (243.70 to 244.70): E

6000000 Ion 212.00 (211.70 to 212.70): E

5000000 Ion 122.00 (121.70 to 122.70): E

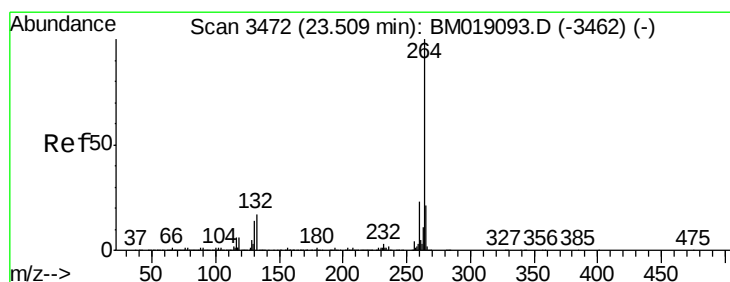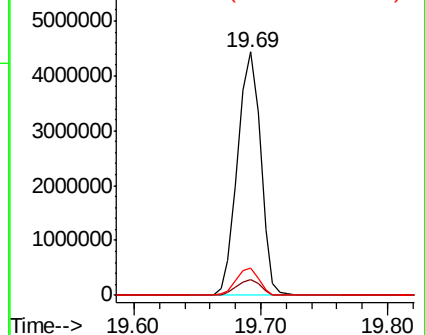

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.49 min Scan# 3485

Delta R.T. -0.02 min

Lab File: BM019240.D

Acq: 19 Mar 2019 17:18


Tgt Ion:264 Resp: 817016

Ion Ratio Lower Upper

264 100

260 24.2 18.6 28.0

265 21.7 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E

500000 Ion 260.00 (259.70 to 260.70): E

400000 Ion 265.00 (264.70 to 265.70): E

