

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031919\
 Data File : BM019258.D
 Acq On : 20 Mar 2019 07:43
 Operator : JU/SJ
 Sample : K1948-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 INV-025-SW03-031319

Quant Time: Mar 20 09:41:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 11 17:30:46 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	184990	20.00	ng	-0.03
21) Naphthalene-d8	10.42	136	767448	20.00	ng	-0.03
39) Acenaphthene-d10	14.29	164	506481	20.00	ng	-0.03
64) Phenanthrene-d10	17.05	188	1192690	20.00	ng	-0.03
76) Chrysene-d12	21.25	240	1132313	20.00	ng	-0.02
87) Perylene-d12	23.47	264	1011575	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.23	112	1798851	157.48	ng	-0.02
7) Phenol-d6	6.82	99	2671786	159.91	ng	-0.02
23) Nitrobenzene-d5	8.80	82	1585388	97.65	ng	-0.03
42) 2,4,6-Tribromophenol	15.79	330	1265015	169.16	ng	-0.03
45) 2-Fluorobiphenyl	12.90	172	3162989	81.23	ng	-0.03
79) Terphenyl-d14	19.69	244	5497534	96.39	ng	-0.02
Target Compounds						
10) Phenol	6.85	94	66074	3.669	ng	91
50) Dimethylphthalate	13.76	163	299159	6.905	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031919\
Data File : BM019258.D
Acq On : 20 Mar 2019 07:43
Operator : JU/SJ
Sample : K1948-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
INV-025-SW03-031319

Quant Time: Mar 20 09:41:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 11 17:30:46 2019
Response via : Initial Calibration

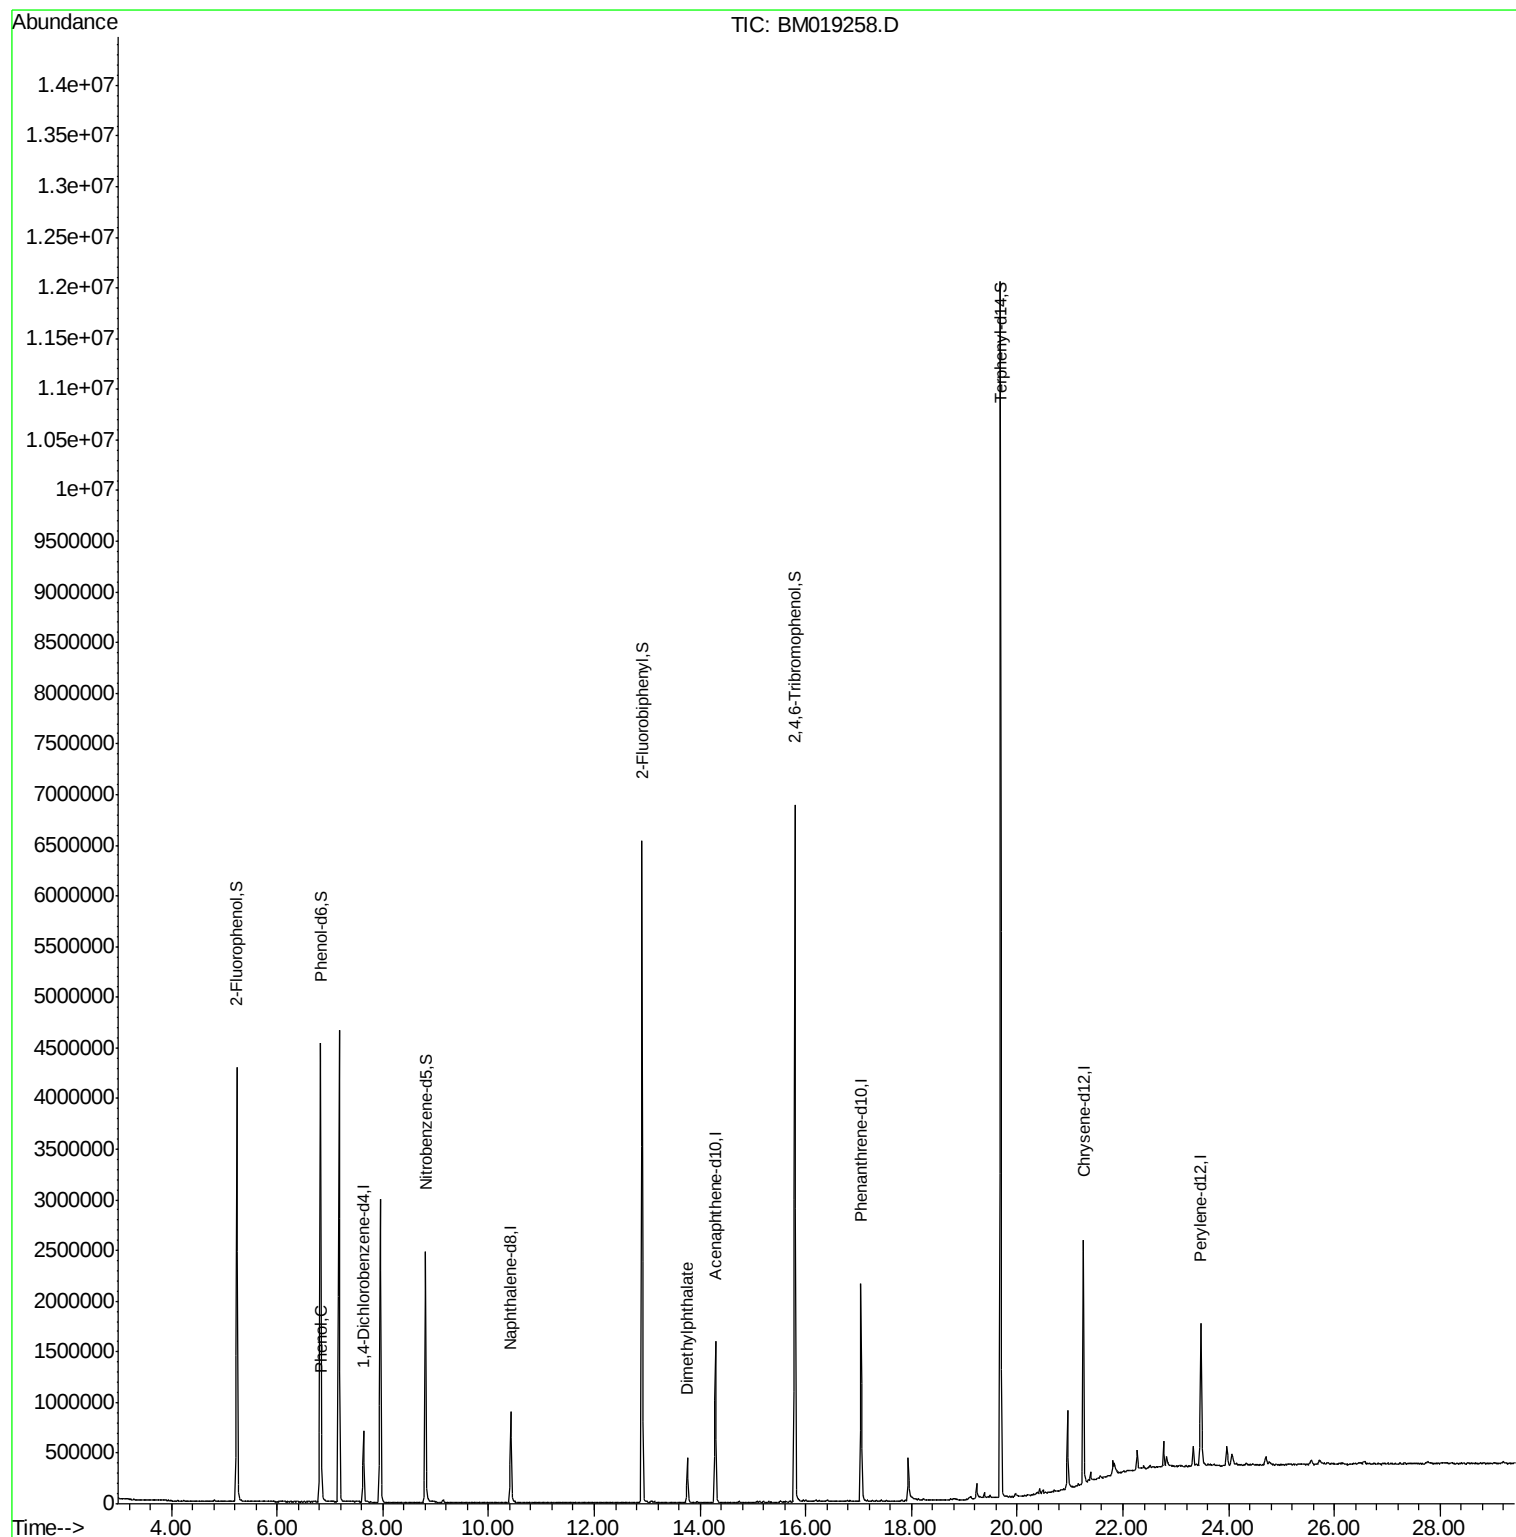

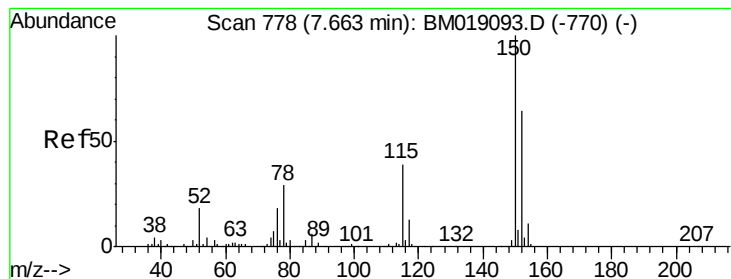


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.63 min Scan# 790
Delta R.T. -0.03 min
Lab File: BM019258.D
Acq: 20 Mar 2019 07:43

Instrument :
BNA_M
ClientSampleId :
INV-025-SW03-031319

Tgt Ion:152 Resp: 184990
Ion Ratio Lower Upper
152 100
150 155.2 125.3 187.9
115 63.0 49.4 74.0




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

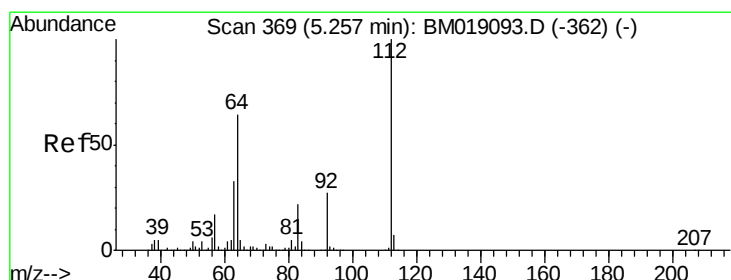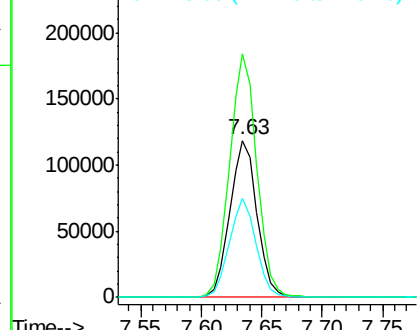



#5


2-Fluorophenol
Concen: 157.479 ng
RT: 5.23 min Scan# 382
Delta R.T. -0.02 min
Lab File: BM019258.D
Acq: 20 Mar 2019 07:43

Tgt Ion:112 Resp: 1798851
Ion Ratio Lower Upper
112 100
64 62.1 51.4 77.0
63 32.1 26.6 40.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

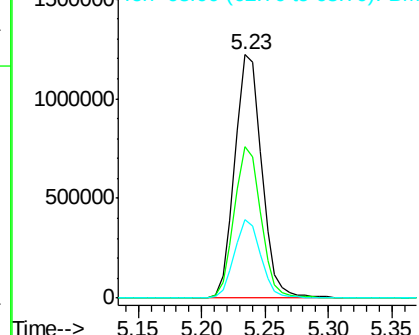



#7

Phenol-d6

Concen: 159.908 ng

RT: 6.82 min Scan# 652

Delta R.T. -0.02 min

Lab File: BM019258.D

Acq: 20 Mar 2019 07:43

Instrument :

BNA_M

ClientSampleId :

INV-025-SW03-031319


Tgt Ion: 99 Resp: 2671786

Ion Ratio Lower Upper

99 100

42 13.3 10.9 16.3




71 36.9 30.3 45.5



Abundance Ion 99.00 (98.70 to 99.70): BM019258.D (-639) (-)

Ion 42.00 (41.70 to 42.70): BM019258.D (-639) (-)

Ion 71.00 (70.70 to 71.70): BM019258.D (-639) (-)

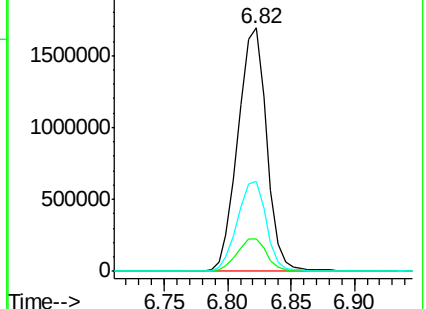

#10

Phenol

Concen: 3.669 ng

RT: 6.85 min Scan# 656

Delta R.T. -0.02 min

Lab File: BM019258.D

Acq: 20 Mar 2019 07:43


Tgt Ion: 94 Resp: 66074

Ion Ratio Lower Upper

94 100

65 32.9 9.7 49.7



66 46.0 19.2 59.2




Abundance Ion 94.00 (93.70 to 94.70): BM019258.D (-643) (-)

Ion 65.00 (64.70 to 65.70): BM019258.D (-643) (-)

Ion 66.00 (65.70 to 66.70): BM019258.D (-643) (-)

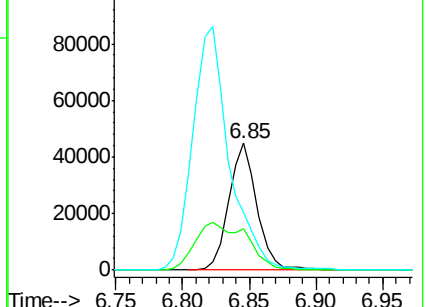


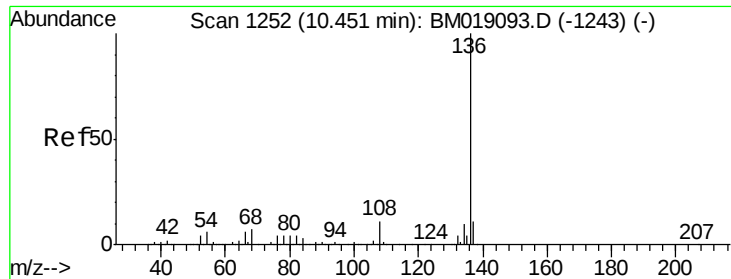




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.42 min Scan# 1263
Delta R.T. -0.03 min
Lab File: BM019258.D
Acq: 20 Mar 2019 07:43

Instrument :
BNA_M
ClientSampleId :
INV-025-SW03-031319

Tgt Ion:	136	Resp:	767448
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.6	13.0
54	6.7	5.2	7.8
68	7.4	5.8	8.8




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM

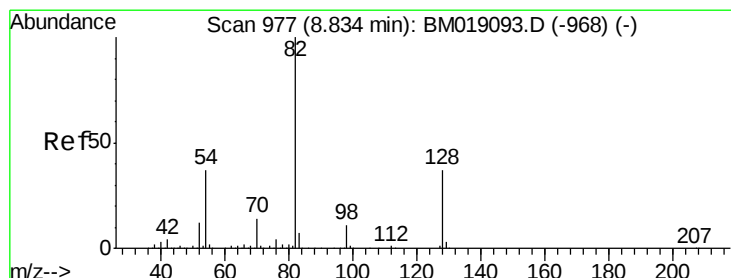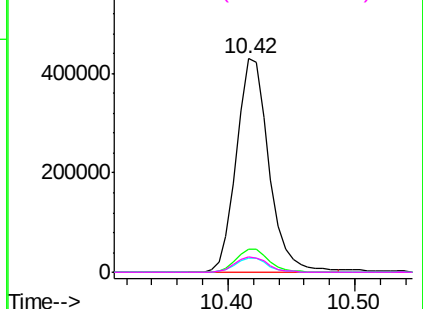




#23
Nitrobenzene-d5
Concen: 97.650 ng
RT: 8.80 min Scan# 989
Delta R.T. -0.03 min
Lab File: BM019258.D
Acq: 20 Mar 2019 07:43

Tgt Ion:	82	Resp:	1585388
Ion	Ratio	Lower	Upper
82	100		
128	37.6	29.4	44.2
54	37.3	29.9	44.9



Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM



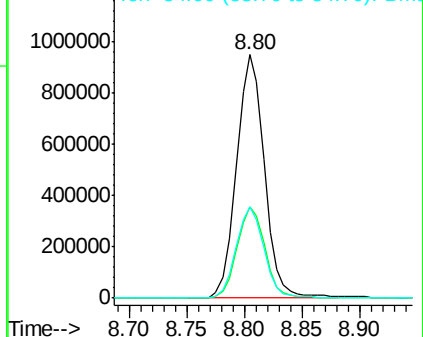
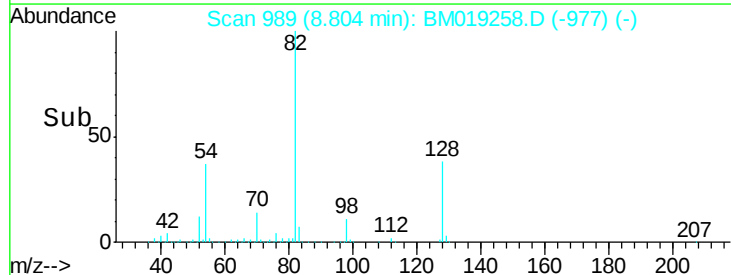


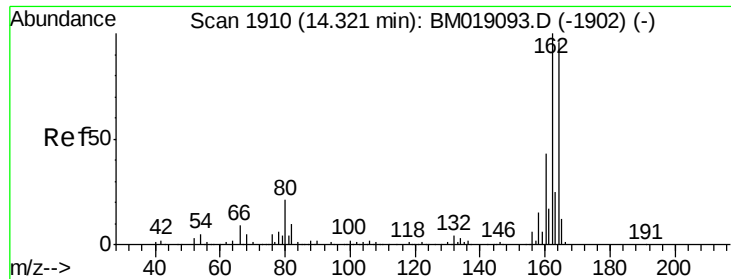

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.29 min Scan# 1922
Delta R.T. -0.03 min
Lab File: BM019258.D
Acq: 20 Mar 2019 07:43




Instrument :
BNA_M
ClientSampleId :
INV-025-SW03-031319


Tgt Ion:164 Resp: 506481
Ion Ratio Lower Upper
164 100
162 106.9 83.5 125.3
160 46.7 36.3 54.5

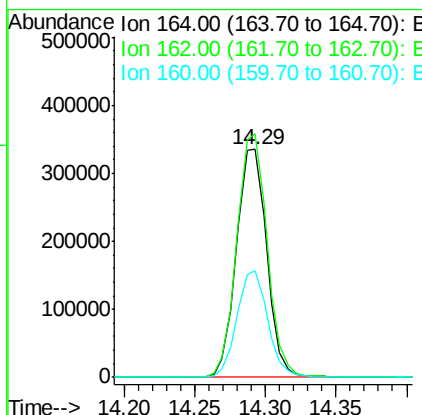

#42
2,4,6-Tribromophenol
Concen: 169.165 ng
RT: 15.79 min Scan# 2177
Delta R.T. -0.03 min
Lab File: BM019258.D
Acq: 20 Mar 2019 07:43

Tgt Ion:330 Resp: 1265015
Ion Ratio Lower Upper
330 100
332 96.7 76.8 115.2
141 31.5 27.0 40.4



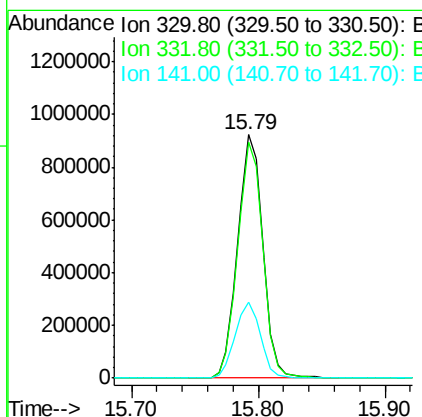



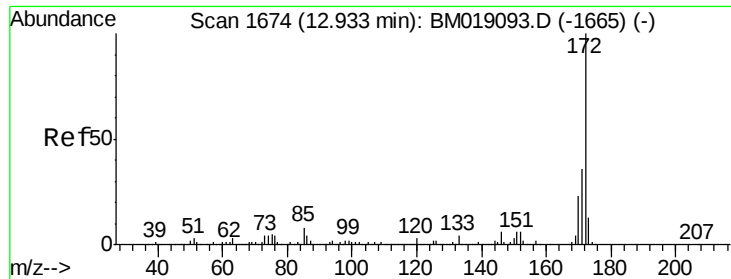

#45
 2-Fluorobiphenyl
 Concen: 81.233 ng
 RT: 12.90 min Scan# 1686
 Delta R.T. -0.03 min
 Lab File: BM019258.D
 Acq: 20 Mar 2019 07:43




Instrument :
 BNA_M
 ClientSampleId :
 INV-025-SW03-031319

Tgt Ion:172 Resp: 3162989
 Ion Ratio Lower Upper
 172 100
 171 35.9 28.6 42.8
 170 23.3 18.6 28.0

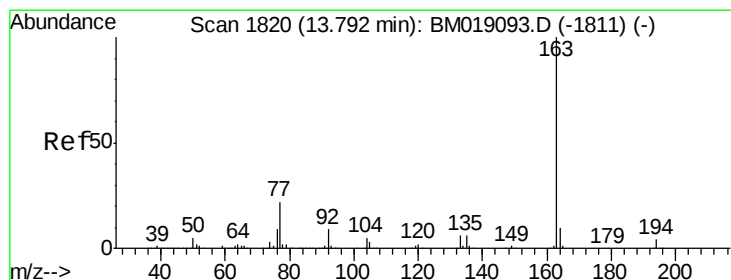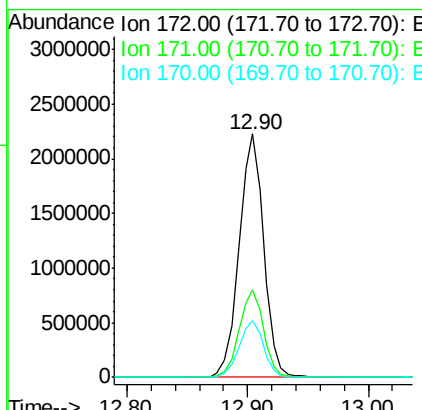

#50
 Dimethylphthalate
 Concen: 6.905 ng
 RT: 13.76 min Scan# 1831
 Delta R.T. -0.03 min
 Lab File: BM019258.D
 Acq: 20 Mar 2019 07:43

Tgt Ion:163 Resp: 299159
 Ion Ratio Lower Upper
 163 100
 194 4.0 3.3 4.9
 164 10.0 7.7 11.5



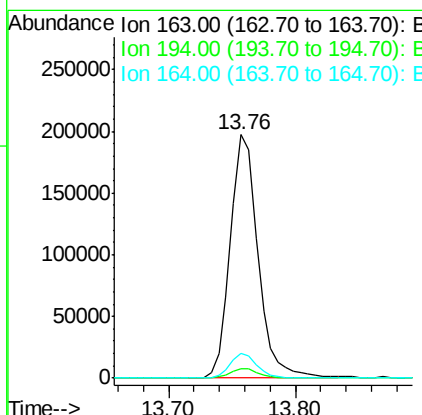





#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.05 min Scan# 2390
Delta R.T. -0.03 min
Lab File: BM019258.D
Acq: 20 Mar 2019 07:43




Instrument :
BNA_M
ClientSampleId :
INV-025-SW03-031319

Tgt Ion:188 Resp: 1192690
Ion Ratio Lower Upper
188 100
94 10.0 8.1 12.1
80 12.3 9.7 14.5

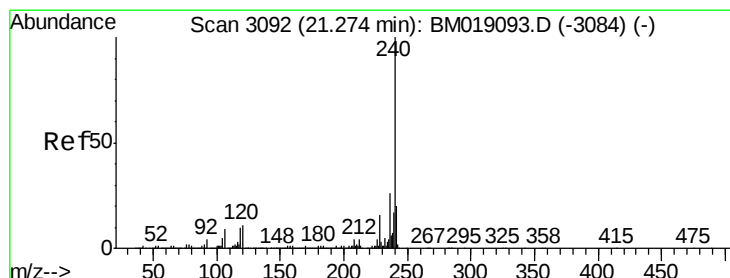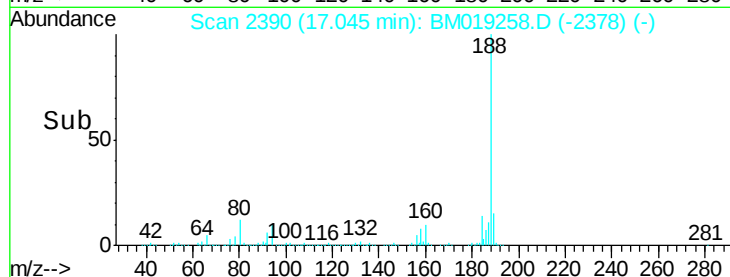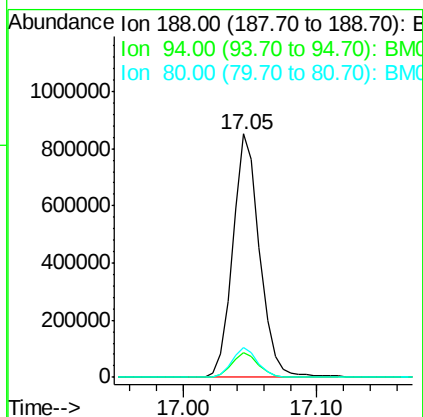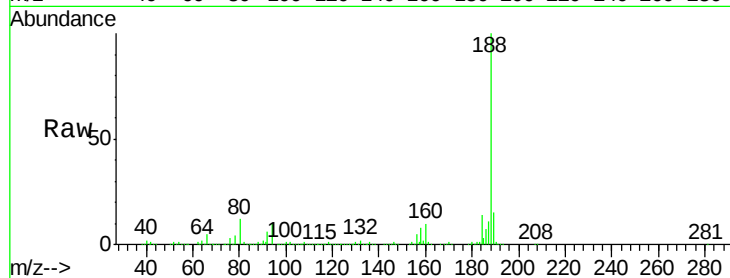

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.25 min Scan# 3105
Delta R.T. -0.02 min
Lab File: BM019258.D
Acq: 20 Mar 2019 07:43

Tgt Ion:240 Resp: 1132313
Ion Ratio Lower Upper
240 100
120 10.6 8.9 13.3
236 26.0 21.0 31.4

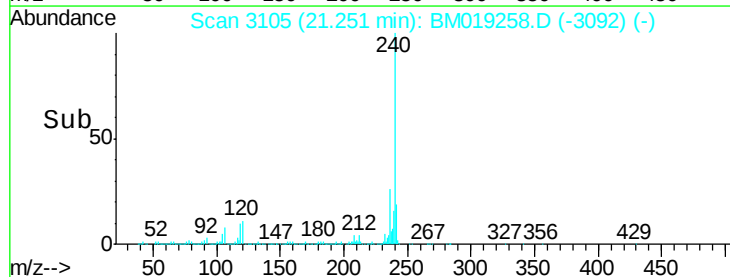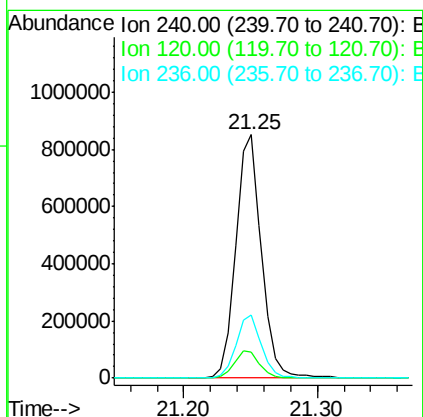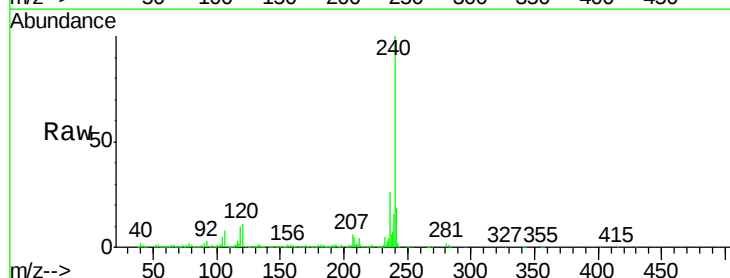



#79

Terphenyl-d14

Concen: 96.385 ng

RT: 19.69 min Scan# 2840

Delta R.T. -0.02 min

Lab File: BM019258.D

Acq: 20 Mar 2019 07:43

Instrument :

BNA_M

ClientSampleId :

INV-025-SW03-031319


Tgt Ion:244 Resp: 5497534

Ion Ratio Lower Upper




244 100

212 6.6 5.4 8.2

122 10.5 9.4 14.2



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

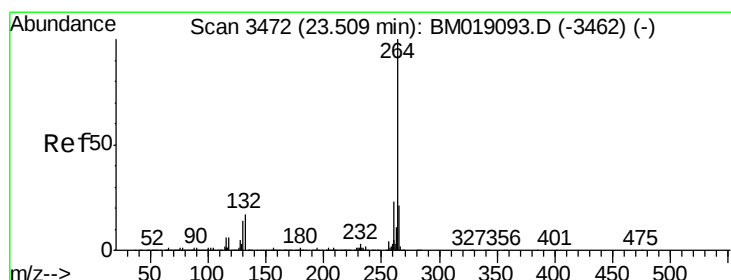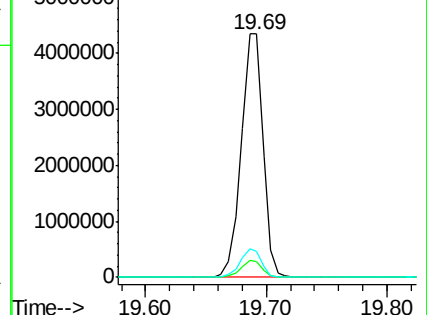

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.47 min Scan# 3483

Delta R.T. -0.03 min

Lab File: BM019258.D

Acq: 20 Mar 2019 07:43


Tgt Ion:264 Resp: 1011575

Ion Ratio Lower Upper

264 100

260 22.8 18.6 28.0

265 21.7 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

