


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031919\
 Data File : BM019248.D
 Acq On : 20 Mar 2019 01:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 11 17:30:46 2019

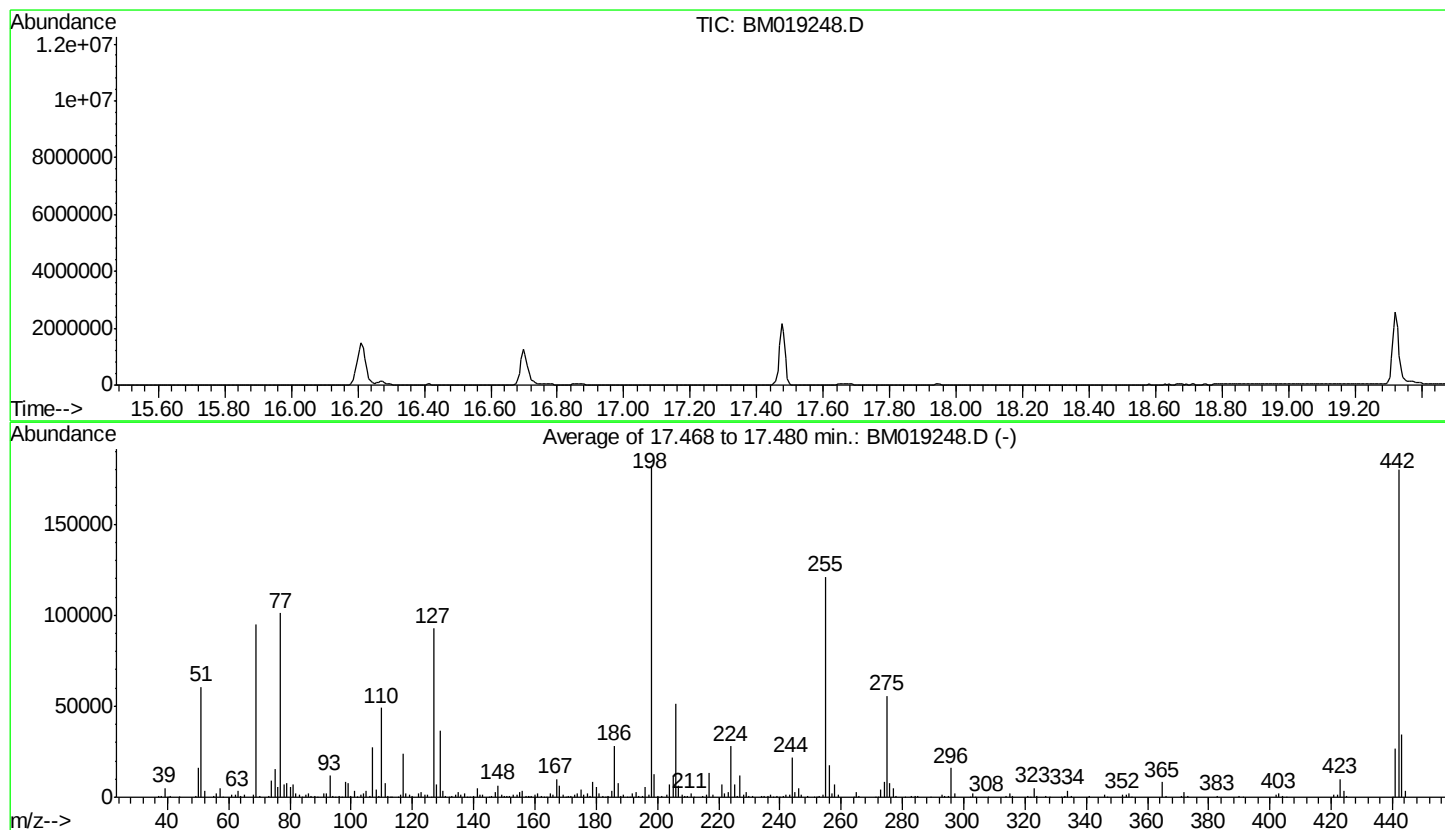

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	60744	PASS
68	69	0.00	2	1.8	1701	PASS
69	198	0.00	100	52.1	94928	PASS
70	69	0.00	2	0.6	566	PASS
127	198	10	80	50.9	92658	PASS
197	198	0.00	2	0.7	1236	PASS
198	198	100	100	100.0	182101	PASS
199	198	5	9	6.9	12551	PASS
275	198	10	60	30.6	55688	PASS
365	198	1	100	4.5	8171	PASS
441	198	0.01	100	14.7	26732	PASS
442	198	50	100	98.7	179664	PASS
443	442	15	24	19.3	34669	PASS